



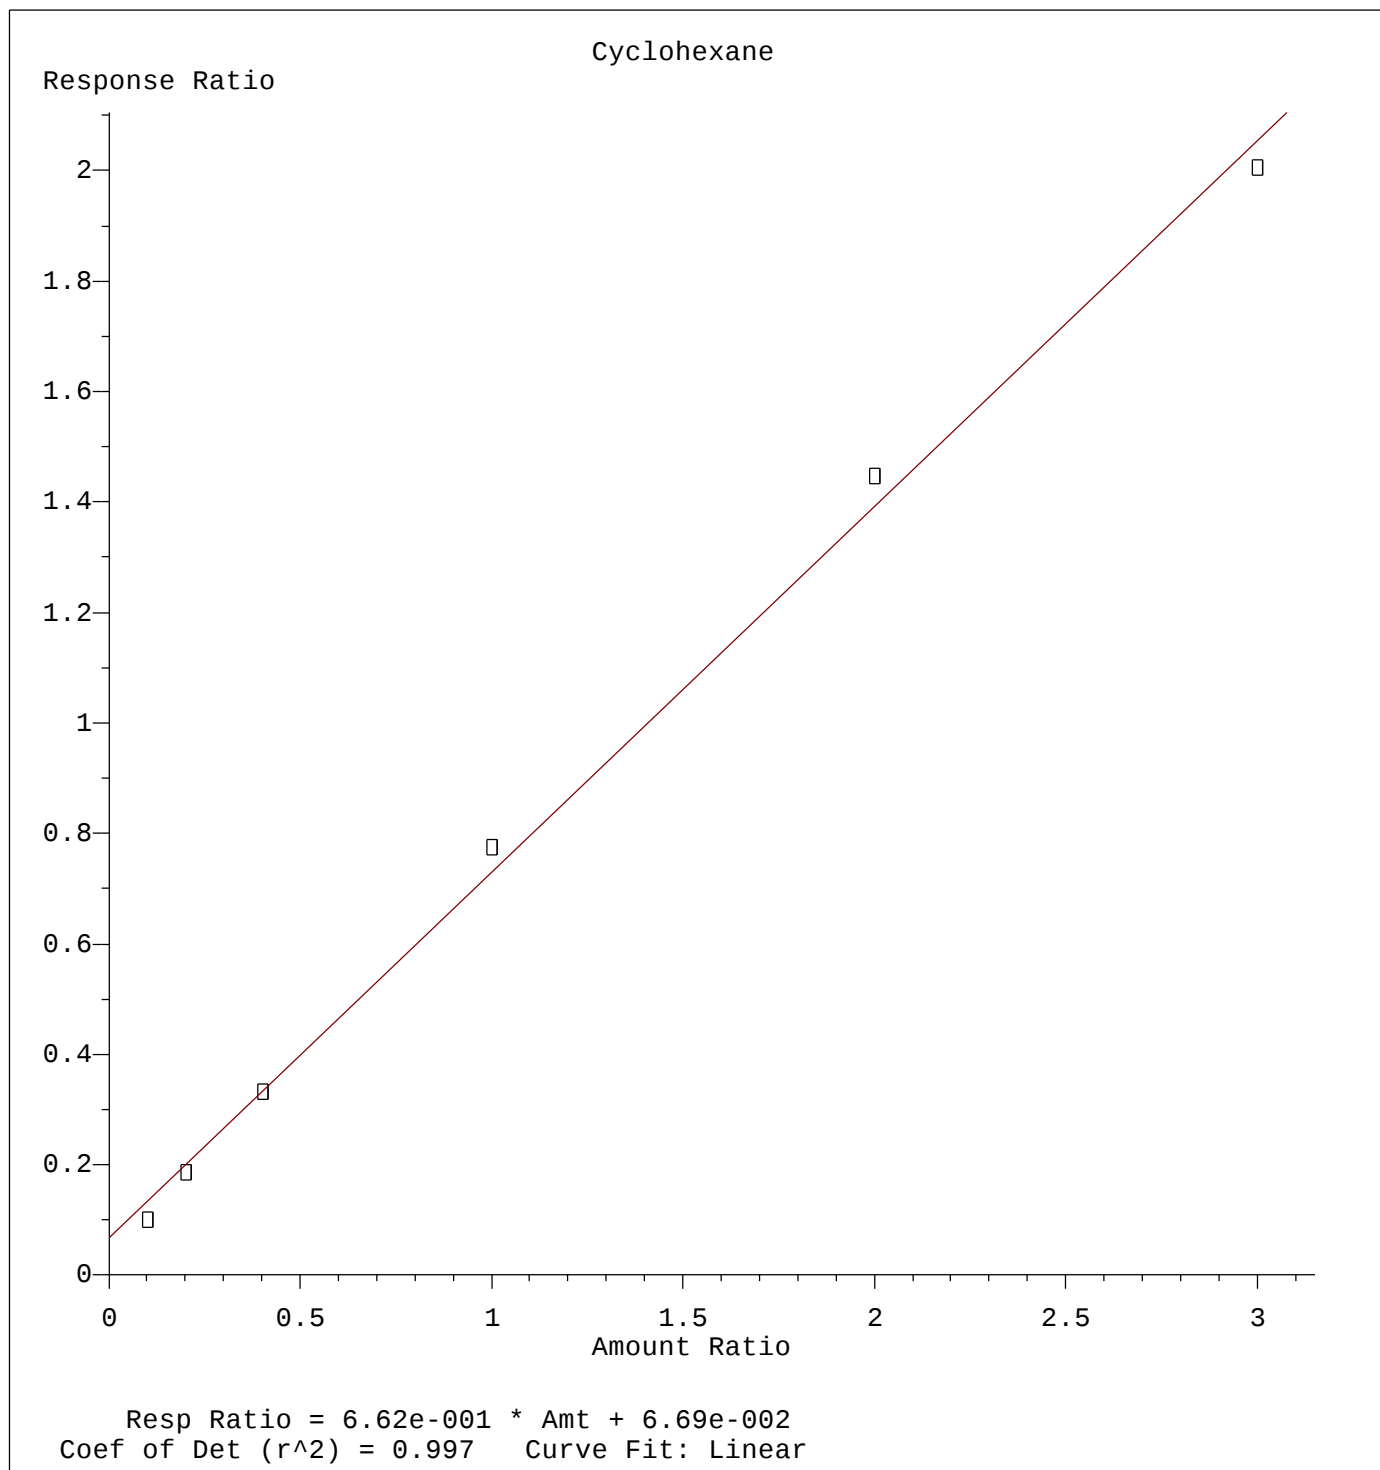

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Calibration Table Last Updated: Fri Nov 29 07:18:03 2019

1,2-Dibromo-3-Chloropropane

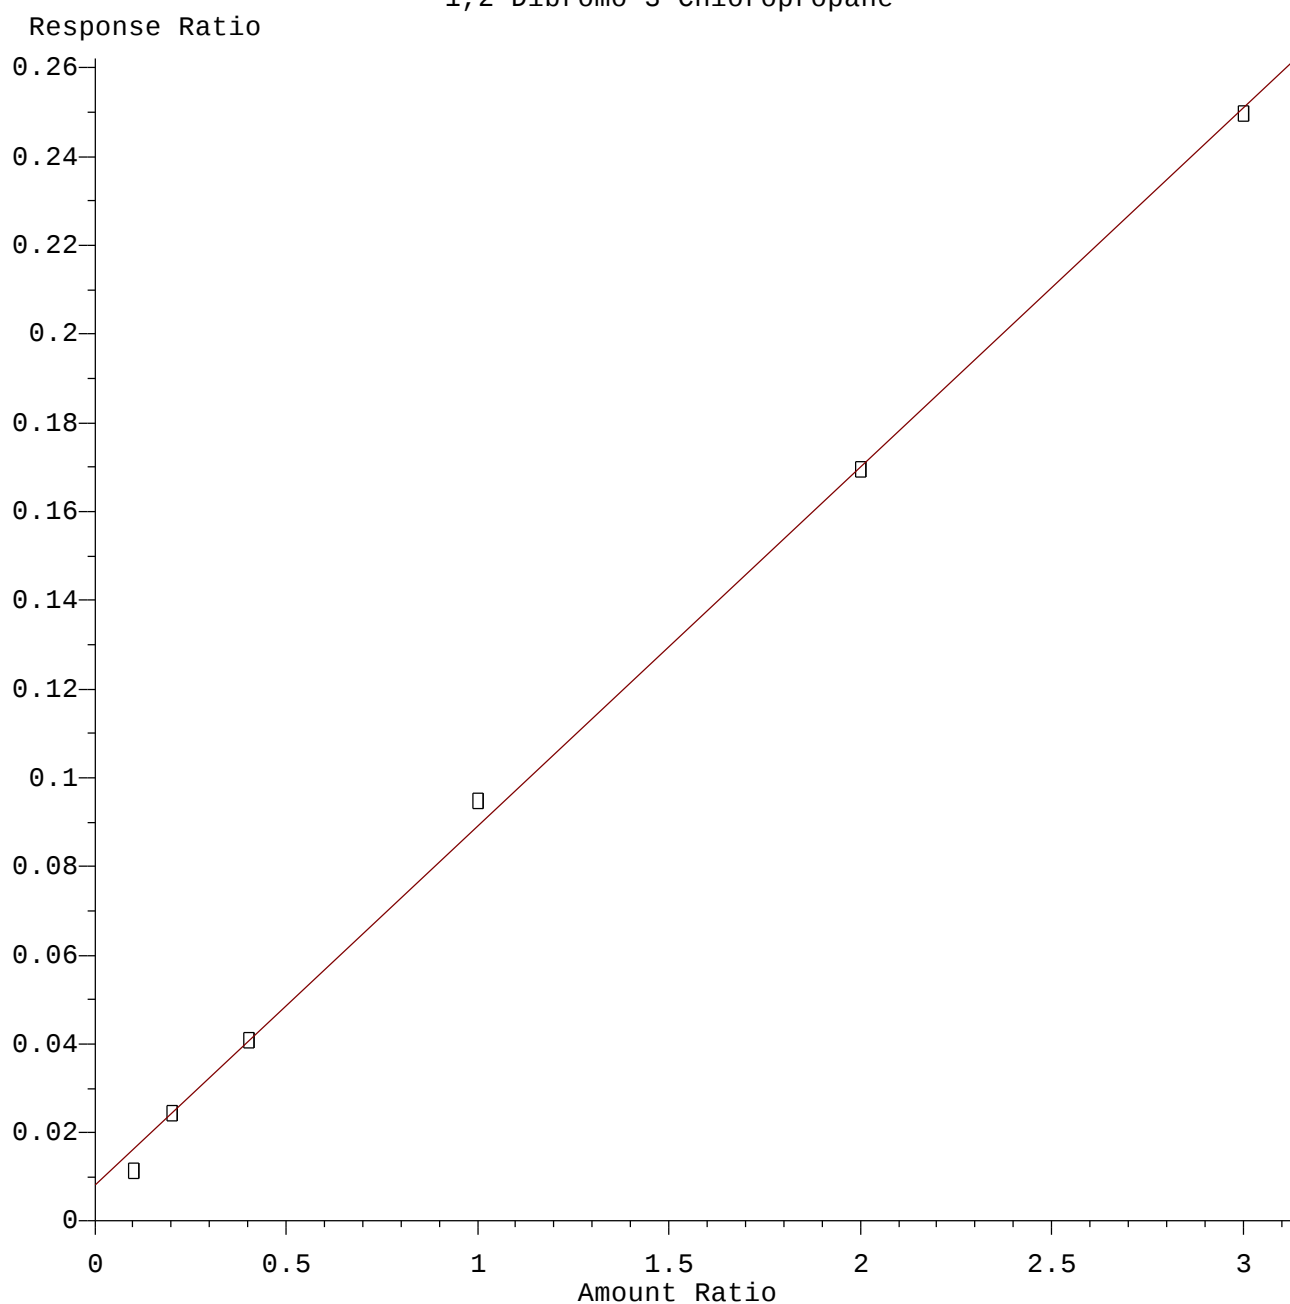


Resp Ratio = $8.11 \times 10^{-2} \times \text{Amt} + 7.79 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Calibration Table Last Updated: Fri Nov 29 07:18:03 2019

Methylene Chloride

Response Ratio

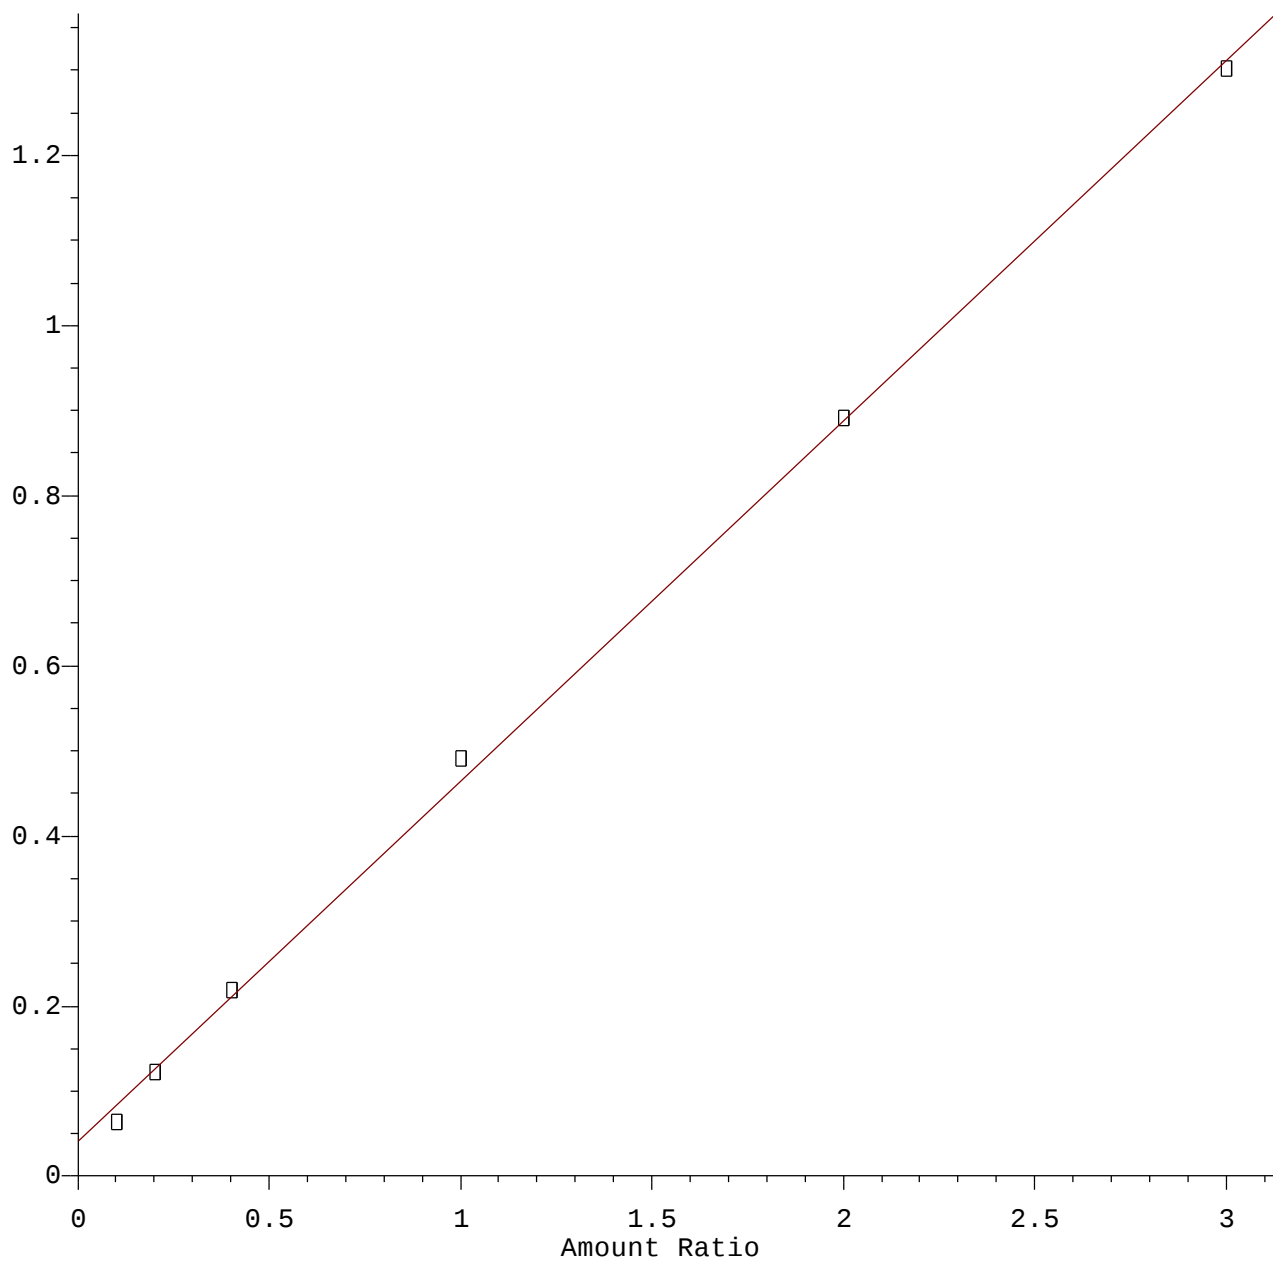

Resp Ratio = $4.23 \times 10^{-1} \times \text{Amt} + 4.13 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Calibration Table Last Updated: Fri Nov 29 07:18:03 2019