


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD112918\
Data File : VD060457.D
Acq On : 29 Nov 2018 9:41
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Title : SW846 8260
Last Update : Mon Nov 19 16:31:59 2018

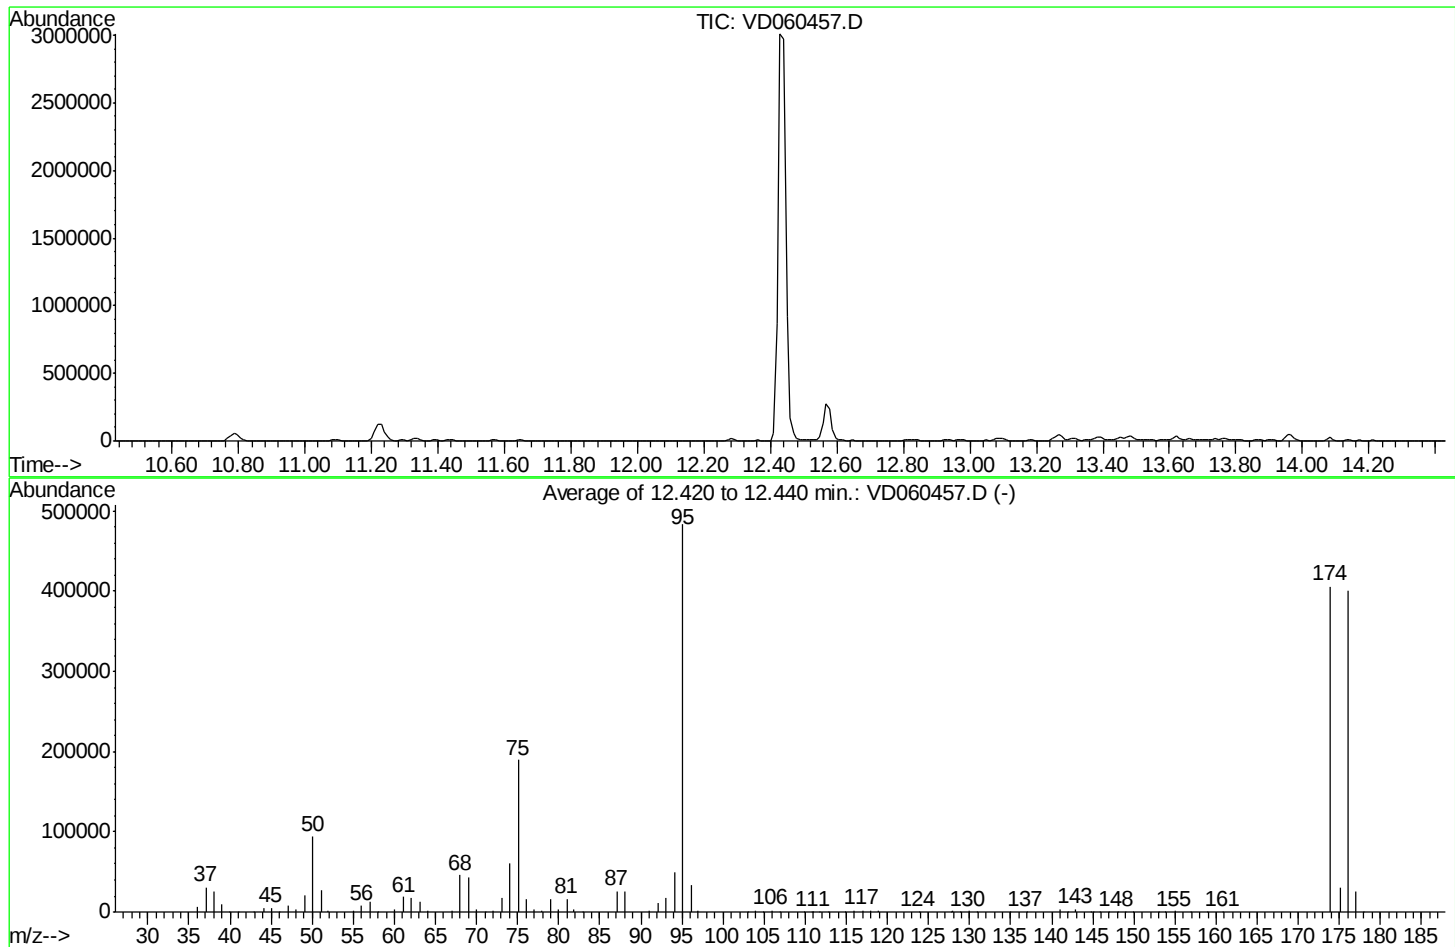

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1103

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	93978	PASS
75	95	30	60	39.3	189848	PASS
95	95	100	100	100.0	483541	PASS
96	95	5	9	6.8	32799	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.0	406093	PASS
175	174	5	9	7.4	29860	PASS
176	174	95	101	98.7	400810	PASS
177	176	5	9	6.5	26184	PASS