


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD113021\
 Data File : VD071079.D
 Acq On : 30 Nov 2021 09:10
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Title : SW846 8260
 Last Update : Mon Nov 29 17:54:09 2021

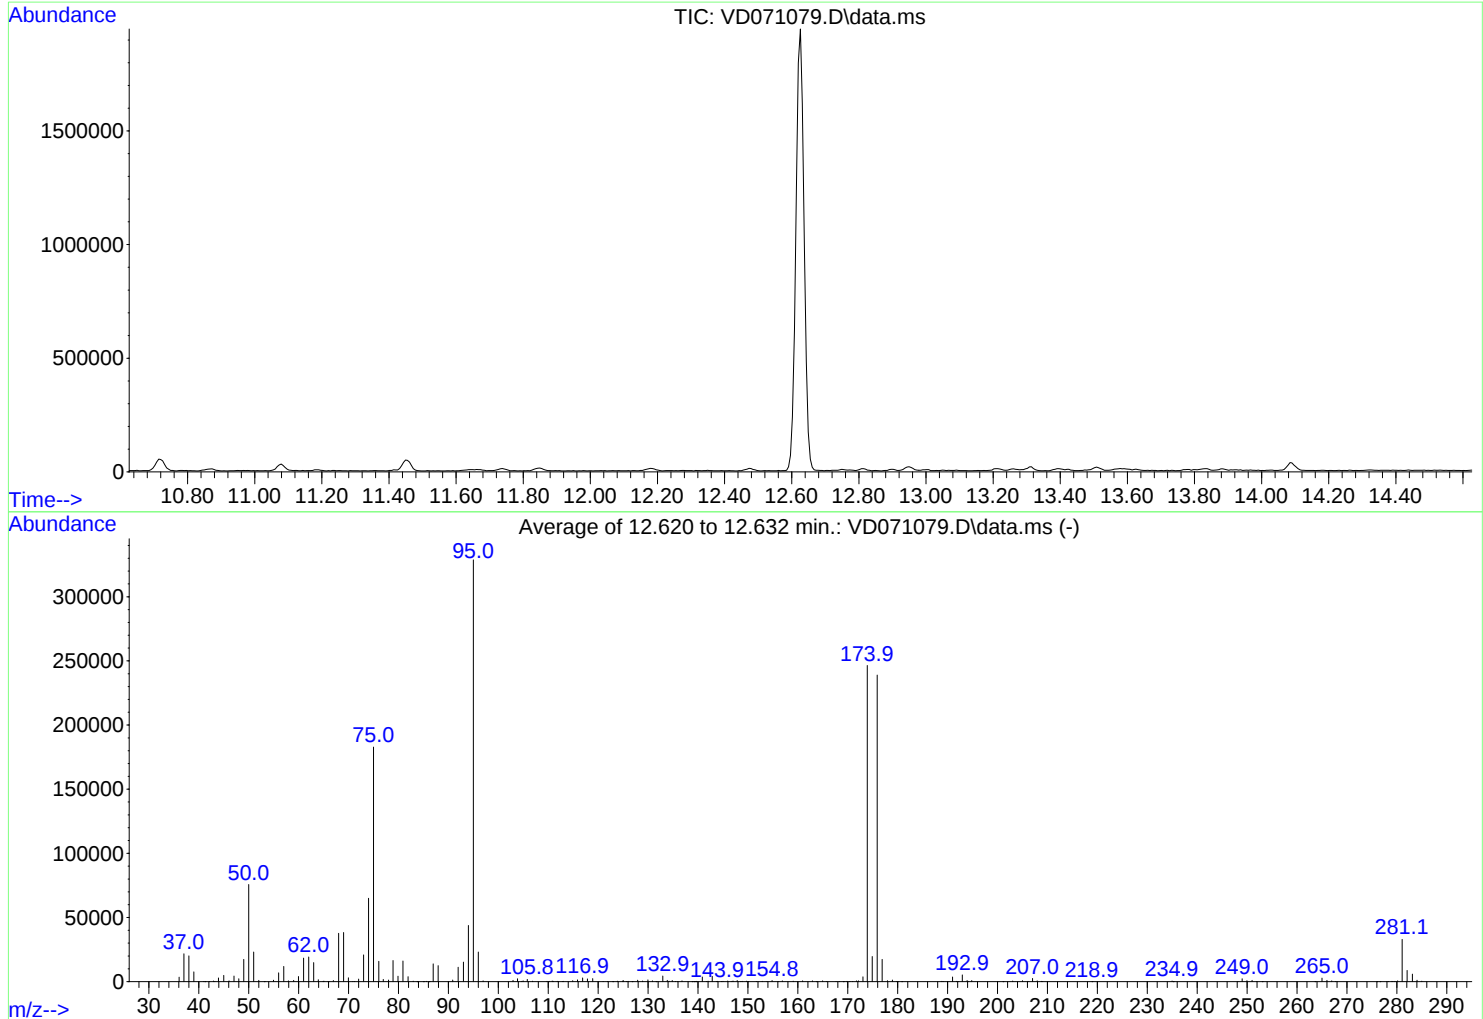

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	75693	PASS
75	95	30	60	55.6	182848	PASS
95	95	100	100	100.0	328789	PASS
96	95	5	9	7.0	23083	PASS
173	174	0.00	2	1.5	3800	PASS
174	95	50	100	74.9	246400	PASS
175	174	5	9	8.0	19632	PASS
176	174	95	101	97.0	238912	PASS
177	176	5	9	7.2	17305	PASS