




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD113023\
 Data File : VD077710.D
 Acq On : 30 Nov 2023 16:55
 Operator : JC/SY
 Sample : 04929-05
 Misc : 3.41G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Nov 30 23:01:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 30 23:00:23 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/01/2023
 Supervised By :Semsettin Yesilyurt 12/01/2023

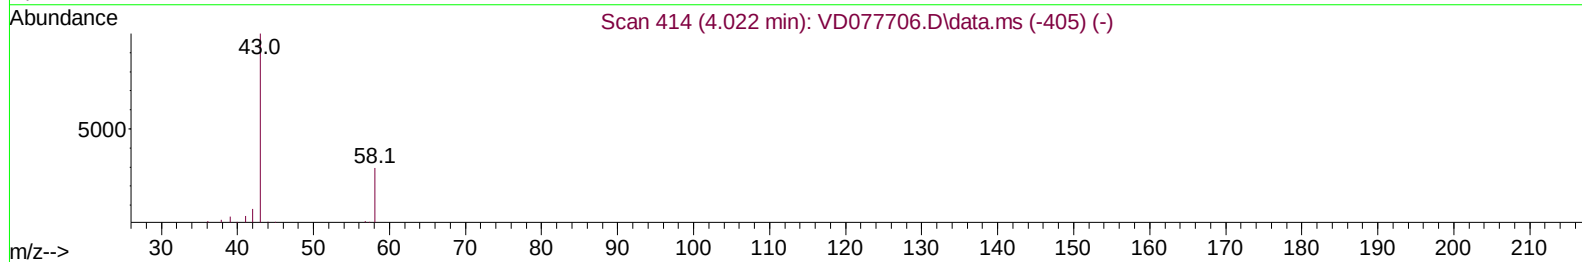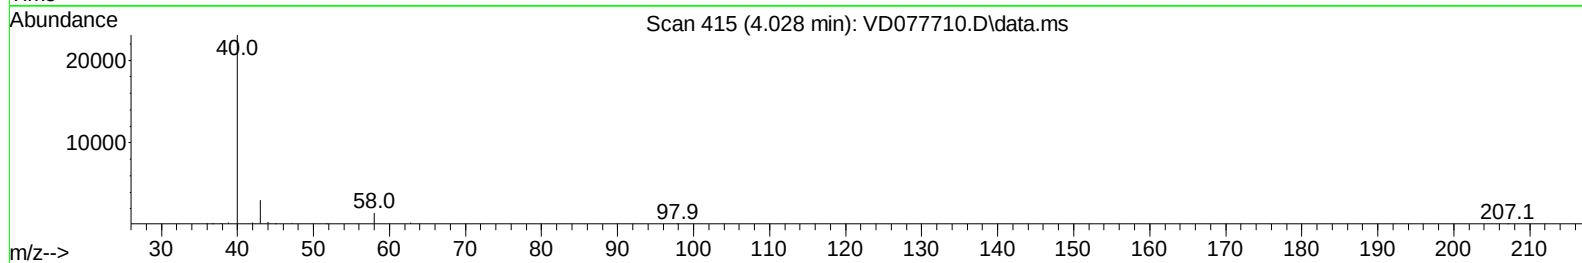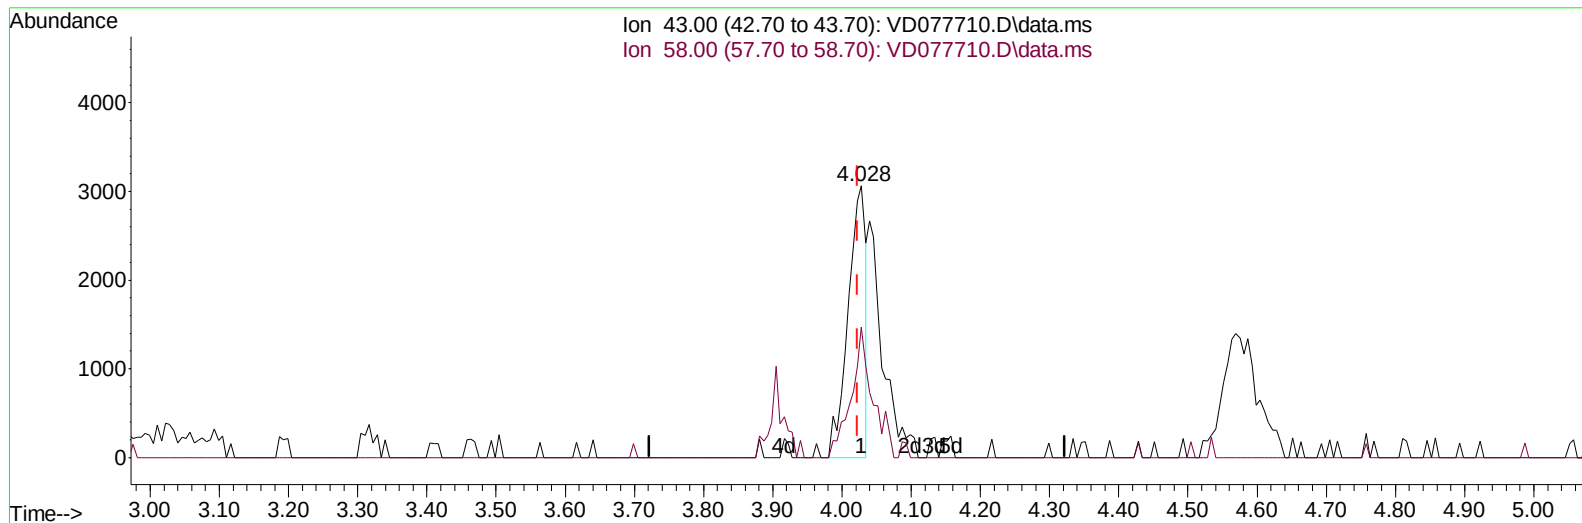

TIC: VD077710.D\data.ms

(13) Acetone (T)

4.028min (+ 0.006) 2.90 ug/L

response 5397

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	53.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD113023\
 Data File : VD077710.D
 Acq On : 30 Nov 2023 16:55
 Operator : JC/SY
 Sample : 04929-05
 Misc : 3.41G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Nov 30 23:01:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 30 23:00:23 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/01/2023
 Supervised By :Semsettin Yesilyurt 12/01/2023

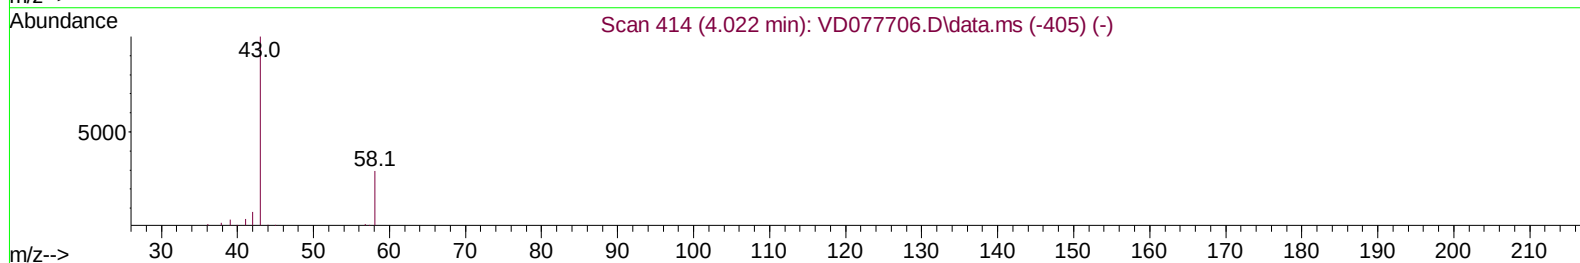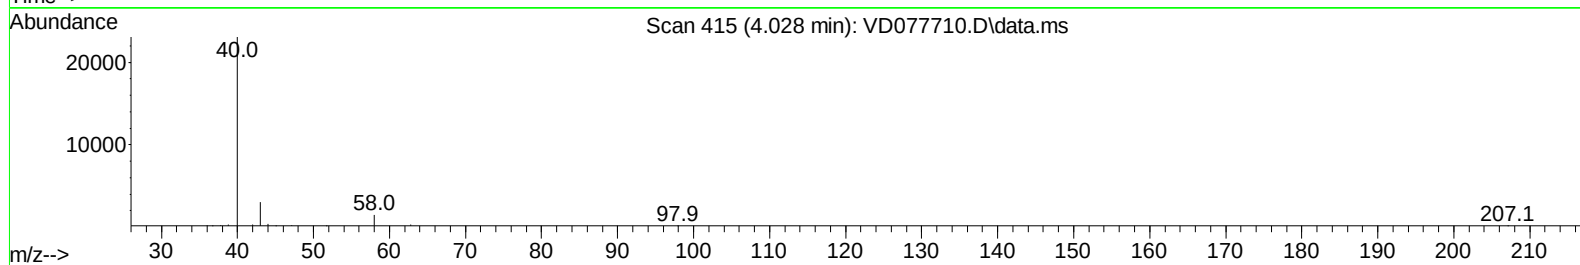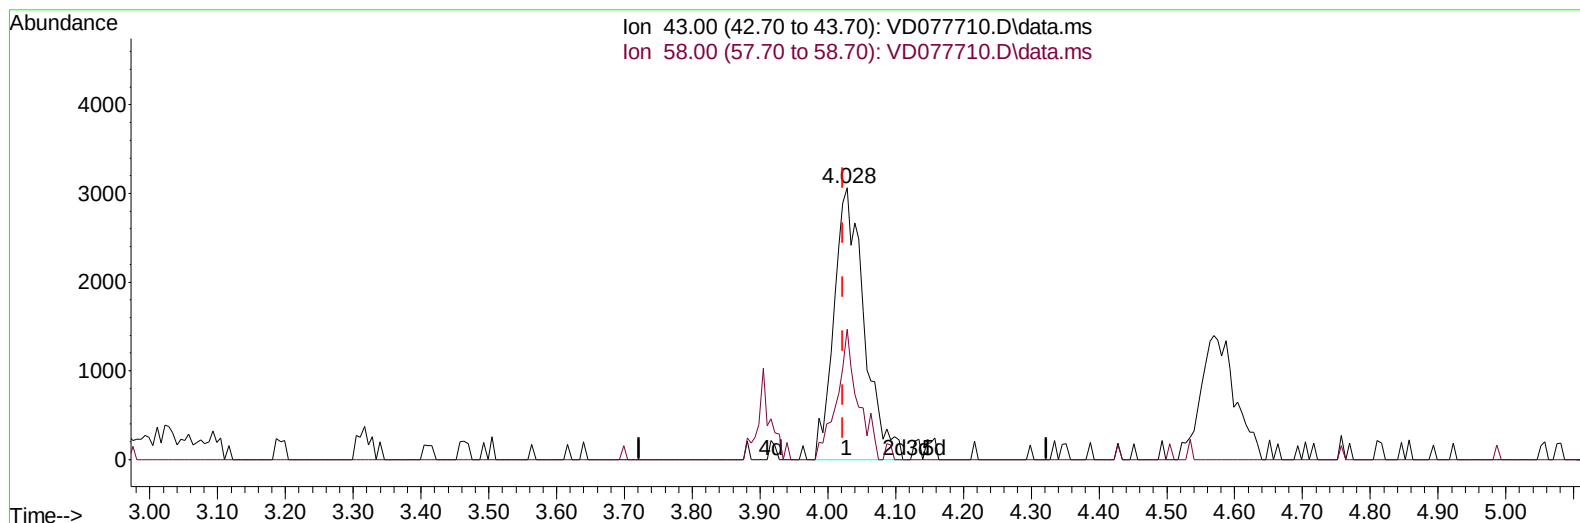

TIC: VD077710.D\data.ms

(13) Acetone (T)

4.028min (+ 0.006) 5.07 ug/L m

response 9433

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	30.79
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD113023\
 Data File : VD077710.D
 Acq On : 30 Nov 2023 16:55
 Operator : JC/SY
 Sample : 04929-05
 Misc : 3.41G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0AQ3

Manual IntegrationsAPPROVED

Quant Time: Nov 30 23:01:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 30 23:00:23 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/01/2023
 Supervised By :Semsettin Yesilyurt 12/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	421640	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	361138	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	124027	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.281	65	241952	21.042	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.160%	
7) Chloroethane-d5	2.805	69	194991	21.276	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.120%	
11) 1,1-Dichloroethene-d2	3.922	65	60029	20.135	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	80.520%	
21) 2-Butanone-d5	6.987	46	66669	45.877	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.760%	
24) Chloroform-d	7.575	84	239606	21.085	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	84.320%	
26) 1,2-Dichloroethane-d4	8.234	65	131298	22.804	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.200%	
32) Benzene-d6	8.204	84	504279	23.185	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.760%	
36) 1,2-Dichloropropane-d6	9.210	67	158327	23.858	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.440%	
41) Toluene-d8	10.269	98	446476	22.302	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.200%	
43) trans-1,3-Dichloroprop...	10.522	79	65824	22.430	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.720%	
47) 2-Hexanone-d5	10.881	63	59434	51.973	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.940%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84	108369	22.598	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	90.400%	
66) 1,2-Dichlorobenzene-d4	13.816	152	96312	21.707	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	86.840%	
Target Compounds						
					Qvalue	
13) Acetone	4.028	43	9433m	5.066	ug/L	
51) Chlorobenzene	11.604	112	47037	3.038	ug/L	92
65) 1,4-Dichlorobenzene	13.539	146	2858	0.344	ug/L #	73
67) 1,2-Dichlorobenzene	13.833	146	2843	0.395	ug/L #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD113023\
Data File : VD077710.D
Acq On : 30 Nov 2023 16:55
Operator : JC/SY
Sample : 04929-05
Misc : 3.41G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0AQ3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/01/2023
Supervised By :Semsettin Yesilyurt 12/01/2023

Quant Time: Nov 30 23:01:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 30 23:00:23 2023
Response via : Initial Calibration

