




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077722.D
 Acq On : 01 Dec 2023 14:26
 Operator : JC/SY
 Sample : 04929-11
 Misc : 4.36G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B62

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:10:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

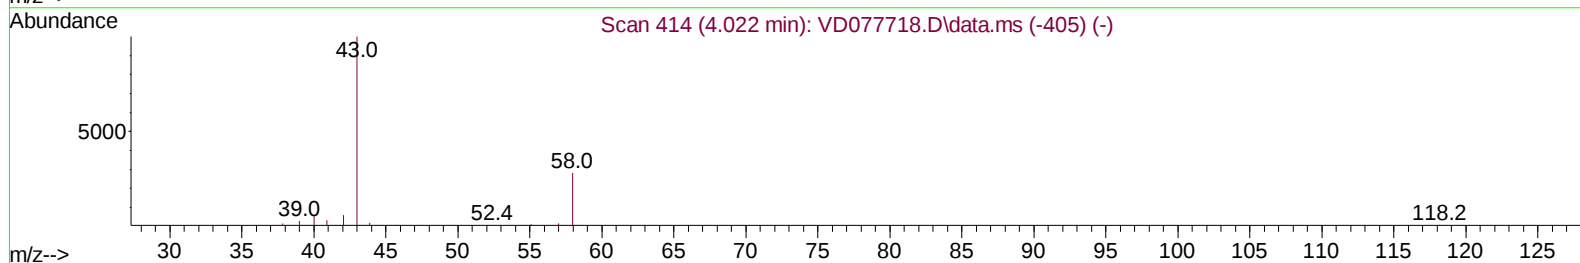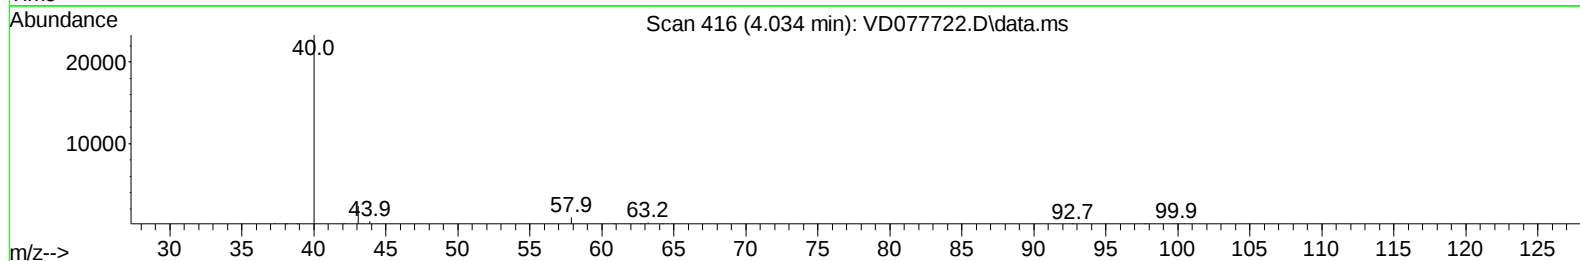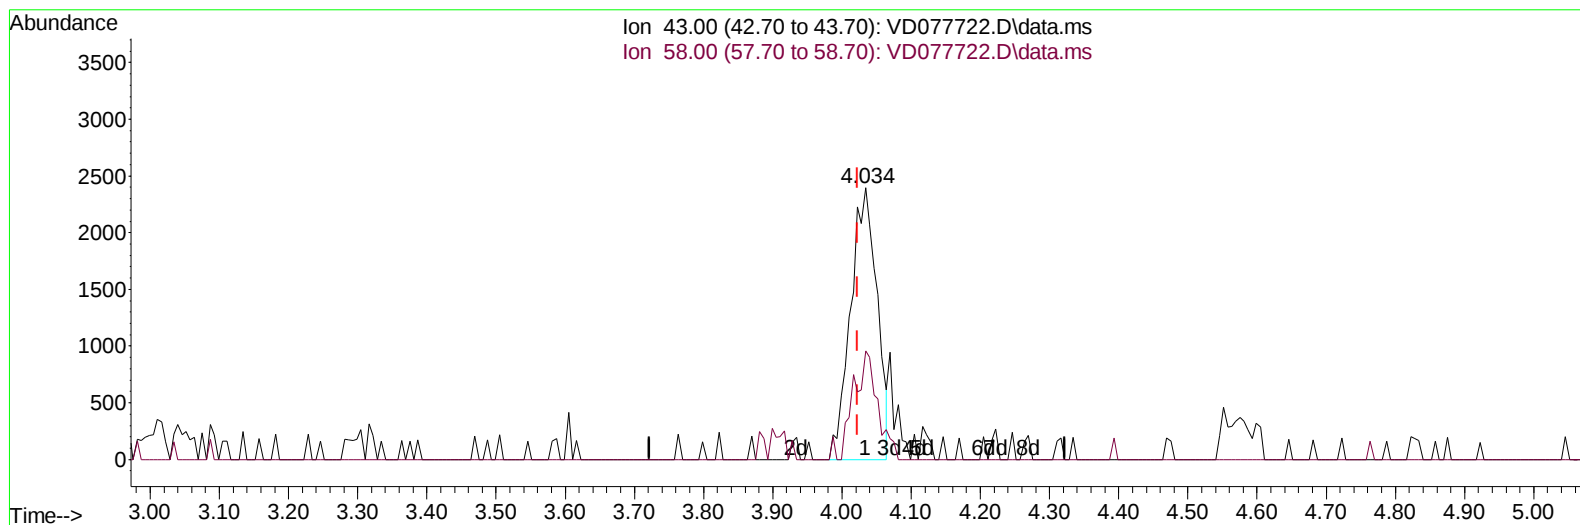

TIC: VD077722.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 3.14 ug/L

response 6333

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	16.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077722.D
 Acq On : 01 Dec 2023 14:26
 Operator : JC/SY
 Sample : 04929-11
 Misc : 4.36G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B62

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:10:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

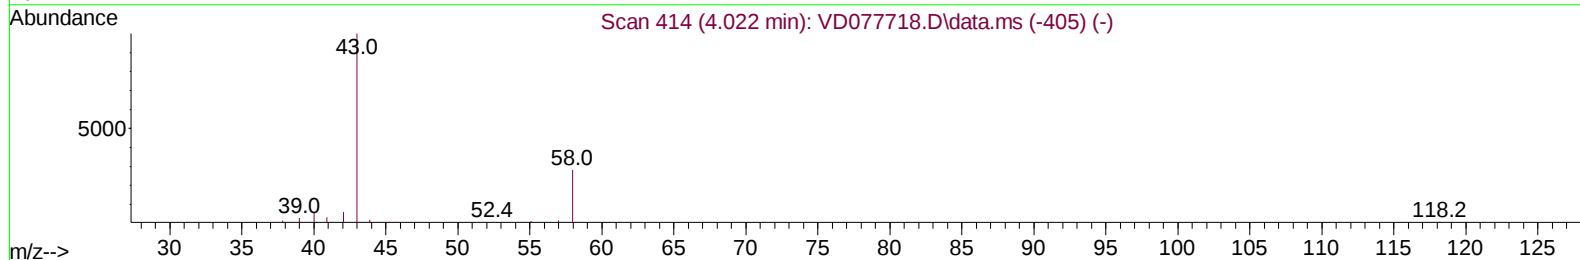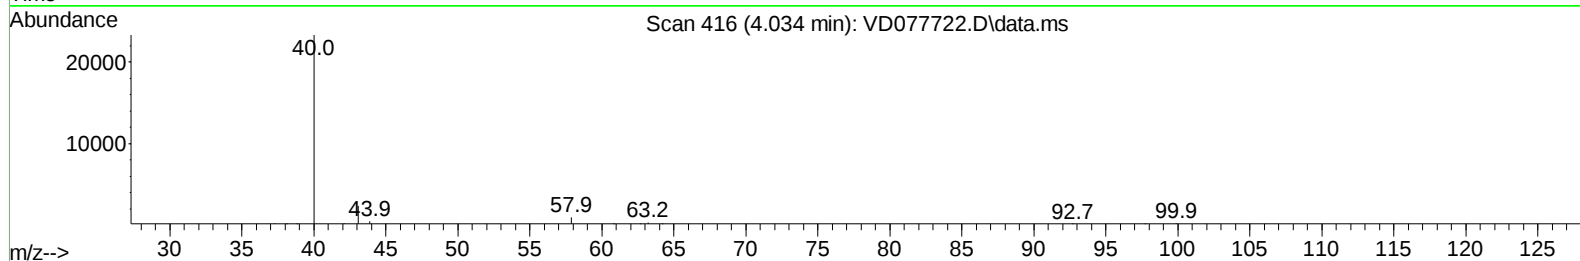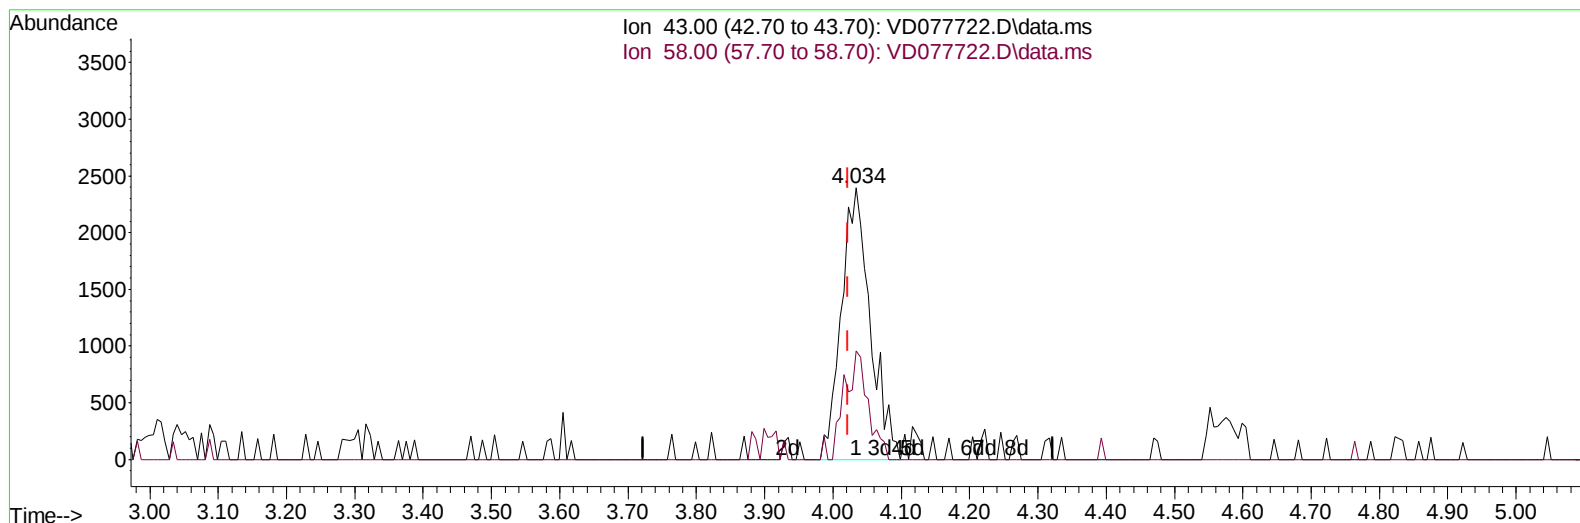

TIC: VD077722.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 3.50 ug/L m

response 7046

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	14.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077722.D
 Acq On : 01 Dec 2023 14:26
 Operator : JC/SY
 Sample : 04929-11
 Misc : 4.36G/10ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B62

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:10:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		456089	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		352477	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		104951	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.287	65		285229	22.933	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	91.720%	
7) Chloroethane-d5	2.811	69		235907	23.796	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.200%	
11) 1,1-Dichloroethene-d2	3.928	65		74123	22.984	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	91.920%	
21) 2-Butanone-d5	6.987	46		64143	40.805	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	81.600%	
24) Chloroform-d	7.575	84		297351	24.190	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	96.760%	
26) 1,2-Dichloroethane-d4	8.240	65		146379	23.503	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	94.000%	
32) Benzene-d6	8.204	84		632472	29.794	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	119.160%	
36) 1,2-Dichloropropane-d6	9.216	67		190466	29.406	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	117.640%	
41) Toluene-d8	10.275	98		538166	27.542	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	110.160%	
43) trans-1,3-Dichloroprop...	10.528	79		73223	25.564	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	102.240%	
47) 2-Hexanone-d5	10.881	63		57699	51.696	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	103.400%	
56) 1,1,2,2-Tetrachloroeth...	12.657	84		104938	22.420	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	89.680%	
66) 1,2-Dichlorobenzene-d4	13.822	152		92465	24.627	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	98.520%	
Target Compounds							
13) Acetone	4.034	43		7046m	3.498	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077722.D
Acq On : 01 Dec 2023 14:26
Operator : JC/SY
Sample : 04929-11
Misc : 4.36G/10ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B62

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

Quant Time: Dec 04 03:10:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

