




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077725.D
Acq On : 01 Dec 2023 15:46
Operator : JC/SY
Sample : 04929-14
Misc : 3.60G/10ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B65

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

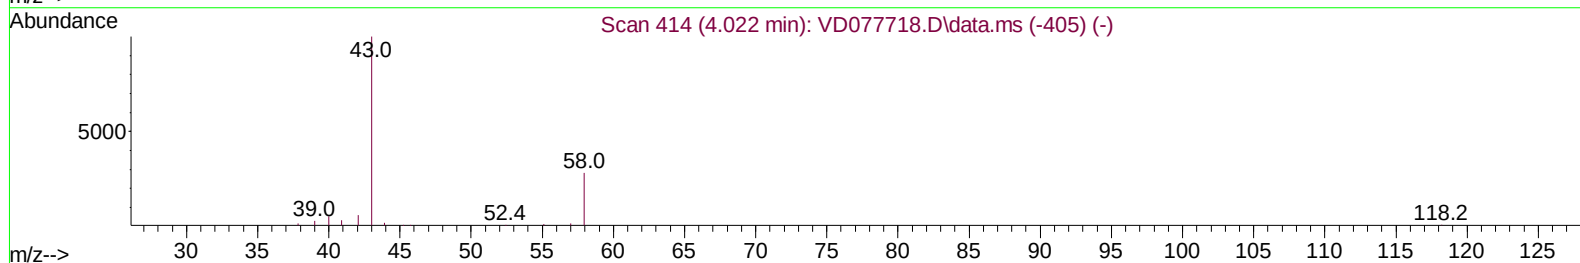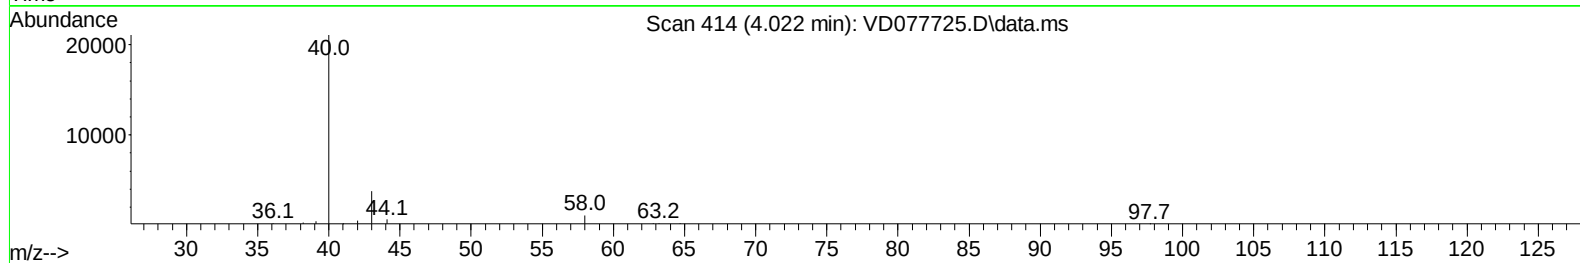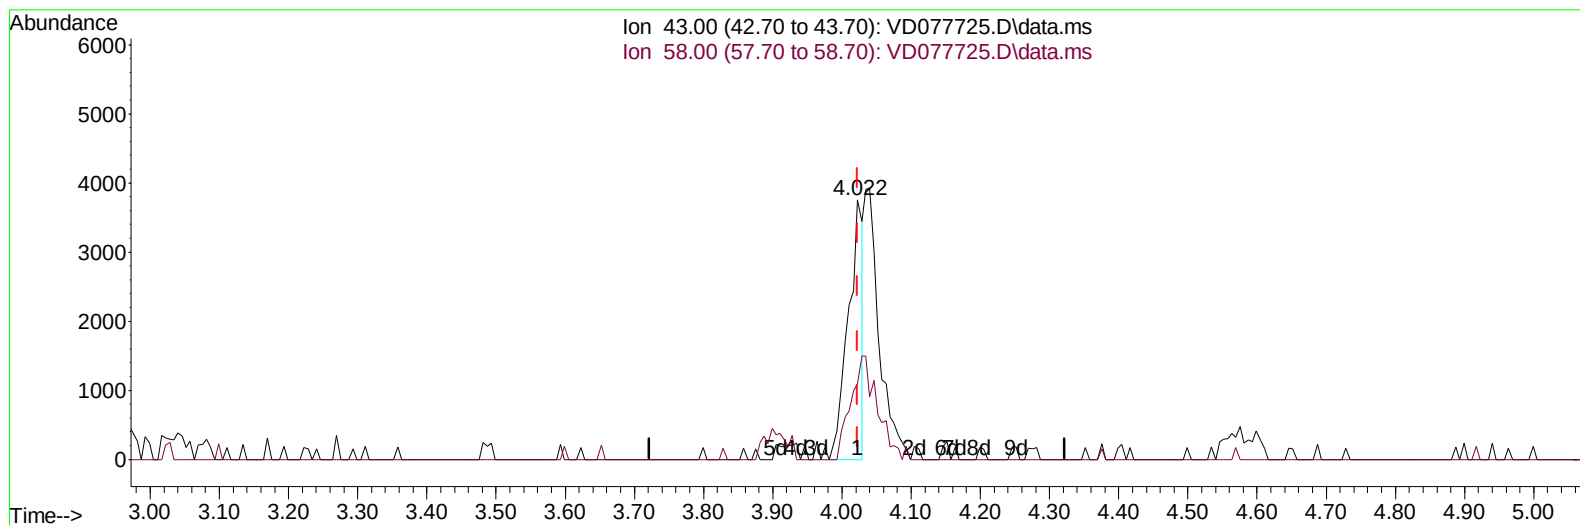

TIC: VD077725.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 5.23 ug/L

response 5395

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	65.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077725.D
Acq On : 01 Dec 2023 15:46
Operator : JC/SY
Sample : 04929-14
Misc : 3.60G/10ml/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B65

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

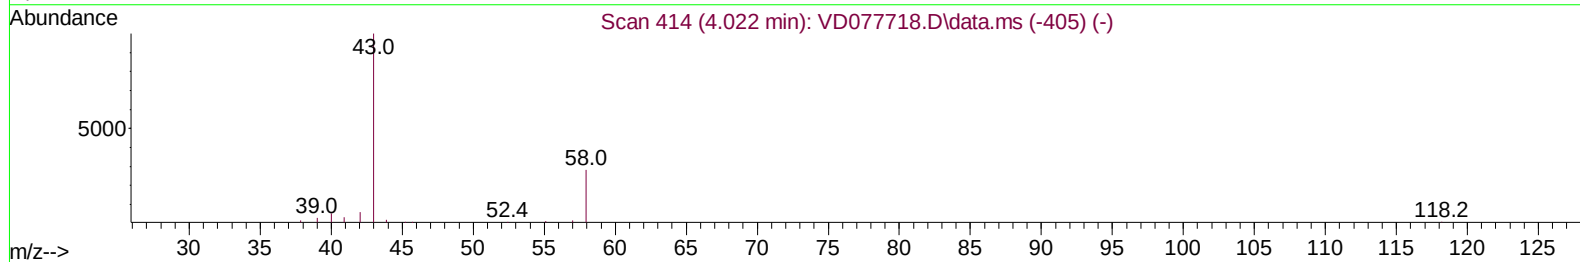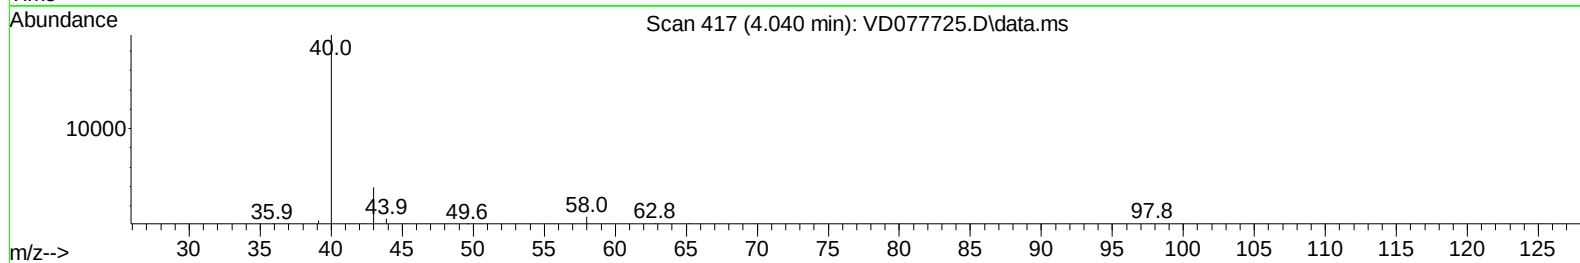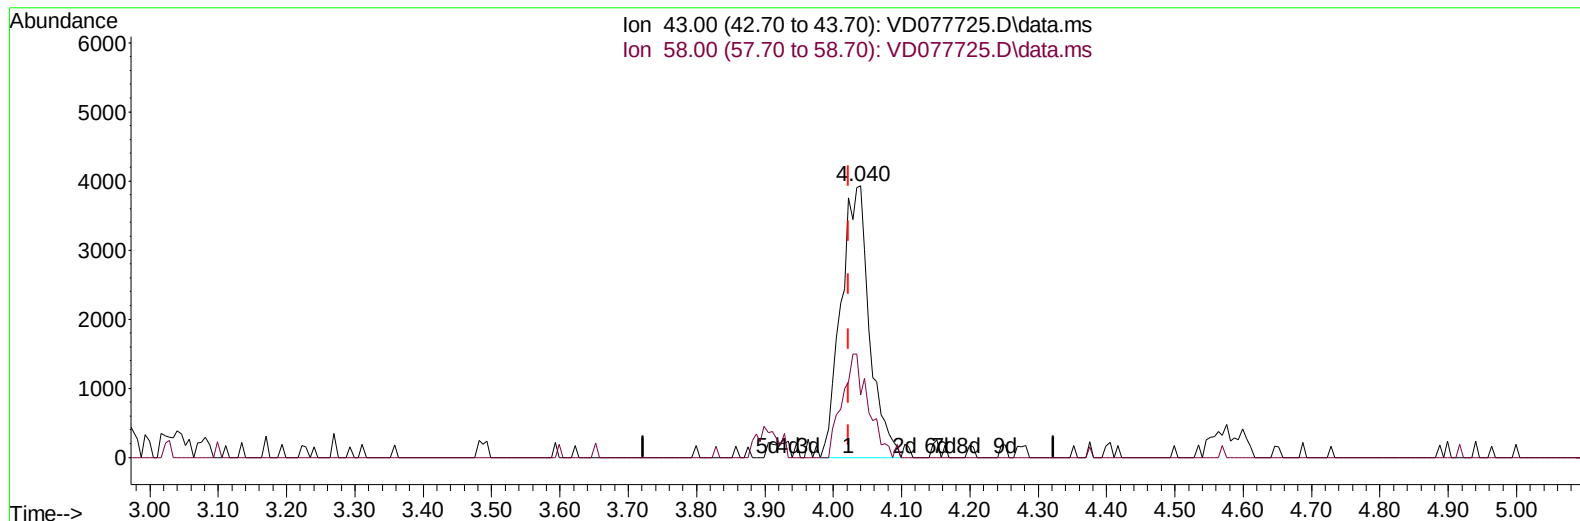

TIC: VD077725.D\data.ms

(13) Acetone (T)

4.040min (+ 0.018) 10.98 ug/L m

response 11323

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	31.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077725.D
 Acq On : 01 Dec 2023 15:46
 Operator : JC/SY
 Sample : 04929-14
 Misc : 3.60G/10ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B65

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		233500	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		123509	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		20816	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.281	65		217842	34.211	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	136.840%	
7) Chloroethane-d5	2.811	69		184985	36.447	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	145.800%	
11) 1,1-Dichloroethene-d2	3.922	65		47336	28.670	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	114.680%#	
21) 2-Butanone-d5	6.987	46		61881	76.892	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	153.780%#	
24) Chloroform-d	7.575	84		202105	32.115	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	128.440%	
26) 1,2-Dichloroethane-d4	8.234	65		119286	37.411	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	149.640%#	
32) Benzene-d6	8.205	84		388153	52.181	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	208.720%#	
36) 1,2-Dichloropropane-d6	9.216	67		126613	55.786	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	223.160%#	
41) Toluene-d8	10.275	98		238675	34.860	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	139.440%#	
43) trans-1,3-Dichloroprop...	10.528	79		45297	45.133	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	180.520%#	
47) 2-Hexanone-d5	10.881	63		48157	123.134	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	246.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		54266	33.087	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	132.360%#	
66) 1,2-Dichlorobenzene-d4	13.822	152		17546	23.562	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	94.240%	
Target Compounds							
13) Acetone	4.040	43		11323m	10.981	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077725.D
Acq On : 01 Dec 2023 15:46
Operator : JC/SY
Sample : 04929-14
Misc : 3.60G/10ml/MSVOA_D/SoIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B65

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

Quant Time: Dec 04 03:11:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

