




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077726.D
Acq On : 01 Dec 2023 16:13
Operator : JC/SY
Sample : 04929-15
Misc : 4.23G/10ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B68

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

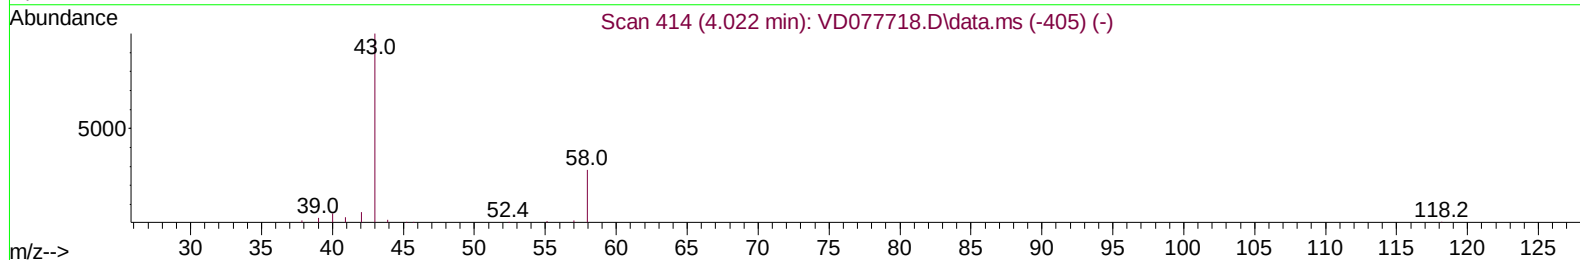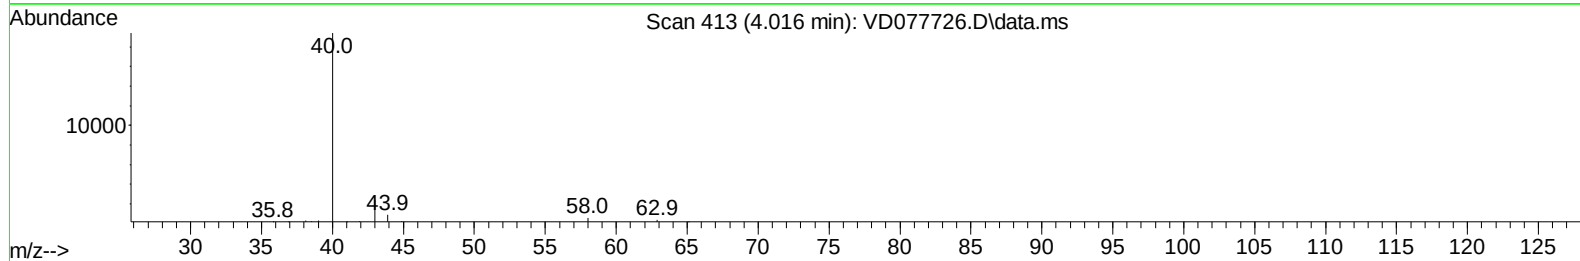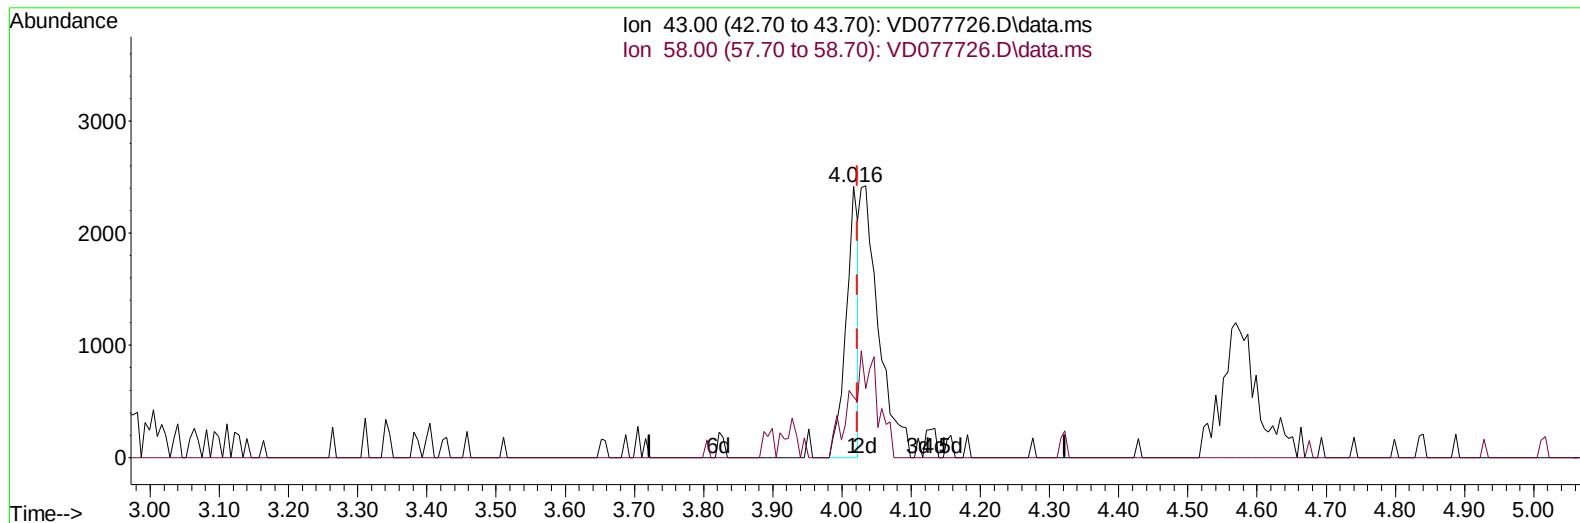

TIC: VD077726.D\data.ms

(13) Acetone (T)

4.016min (-0.006) 1.80 ug/L

response 2944

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	23.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077726.D
 Acq On : 01 Dec 2023 16:13
 Operator : JC/SY
 Sample : 04929-15
 Misc : 4.23G/10ml/MSVOA_D/SoIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B68

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

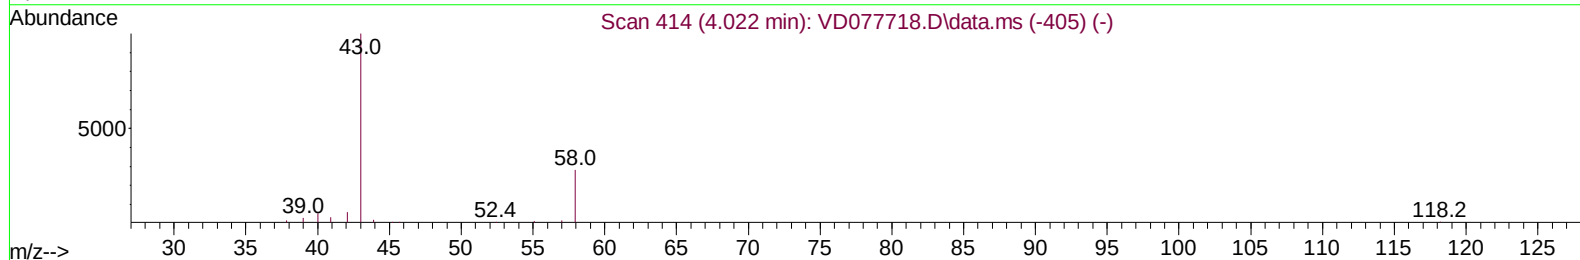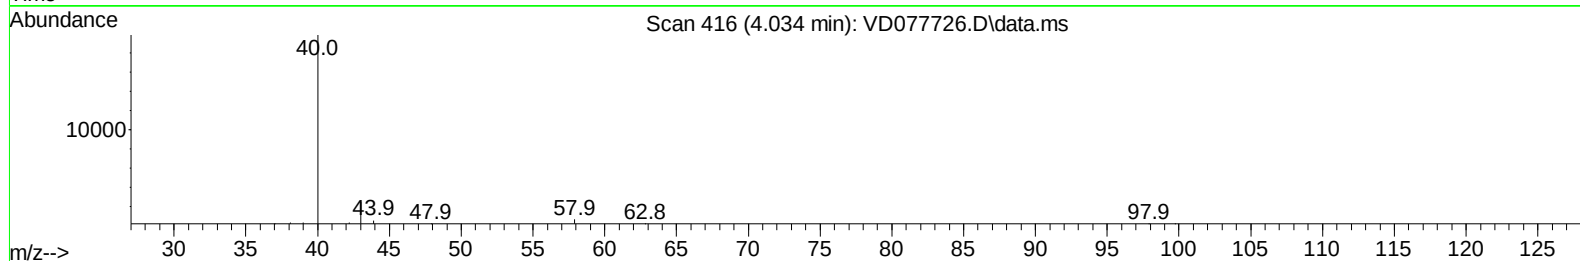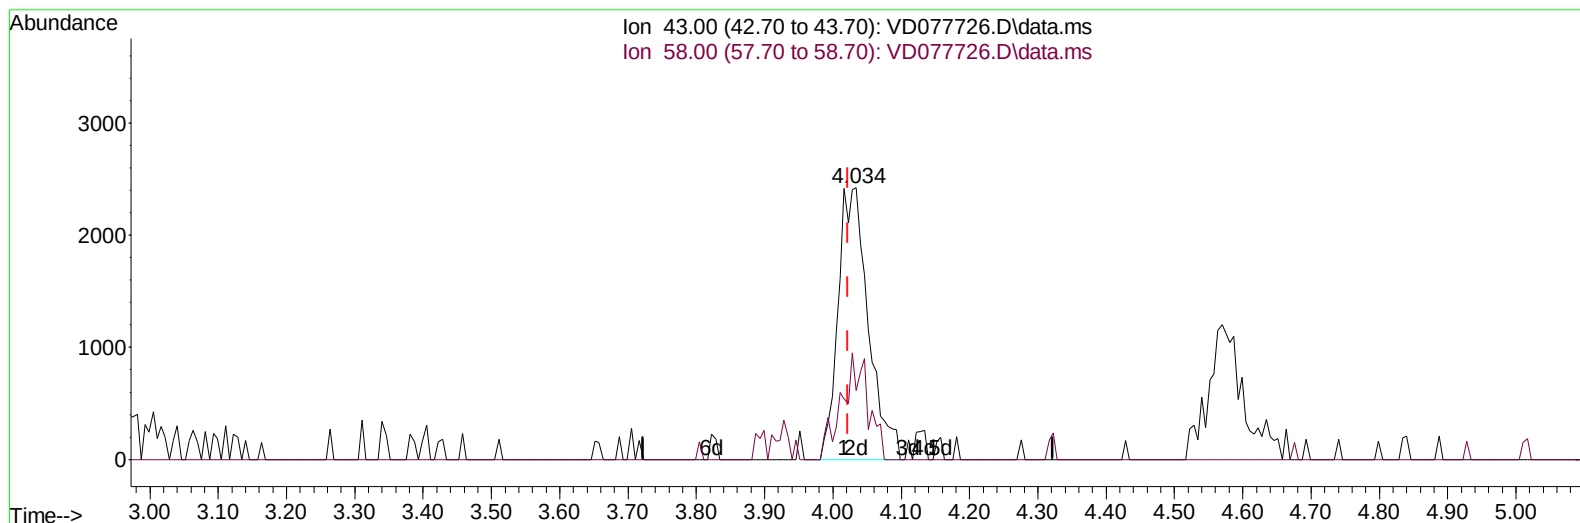

TIC: VD077726.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 4.56 ug/L m

response 7448

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	9.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
 Data File : VD077726.D
 Acq On : 01 Dec 2023 16:13
 Operator : JC/SY
 Sample : 04929-15
 Misc : 4.23G/10ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B68

Manual IntegrationsAPPROVED

Quant Time: Dec 04 03:11:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Dec 04 03:09:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/04/2023
 Supervised By :Semsettin Yesilyurt 12/04/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		369591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		254229	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		53622	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.281	65		217331	21.563	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	86.240%	
7) Chloroethane-d5	2.805	69		188504	23.464	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	93.840%	
11) 1,1-Dichloroethene-d2	3.928	65		52888	20.238	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	80.960%	
21) 2-Butanone-d5	6.993	46		59146	46.432	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	92.860%	
24) Chloroform-d	7.575	84		220647	22.151	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	88.600%	
26) 1,2-Dichloroethane-d4	8.234	65		123032	24.377	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	97.520%	
32) Benzene-d6	8.204	84		454123	29.659	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	118.640%	
36) 1,2-Dichloropropane-d6	9.216	67		145427	31.129	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	124.520%#	
41) Toluene-d8	10.275	98		349935	24.830	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.320%	
43) trans-1,3-Dichloroprop...	10.528	79		53701	25.994	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	103.960%	
47) 2-Hexanone-d5	10.881	63		48613	60.387	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.780%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		77742	23.028	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	92.120%	
66) 1,2-Dichlorobenzene-d4	13.816	152		38070	19.846	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	79.400%	
Target Compounds							
13) Acetone	4.034	43		7448m	4.563	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120123\
Data File : VD077726.D
Acq On : 01 Dec 2023 16:13
Operator : JC/SY
Sample : 04929-15
Misc : 4.23G/10ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B68

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/04/2023
Supervised By :Semsettin Yesilyurt 12/04/2023

Quant Time: Dec 04 03:11:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Dec 04 03:09:24 2023
Response via : Initial Calibration

