

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD120318\
 Data File : VD060474.D
 Acq On : 3 Dec 2018 14:46
 Operator : VA/AP
 Sample : J5764-25
 Misc : 6.38g/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JC-02-113018-C

Quant Time: Dec 04 02:44:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 19 16:31:59 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.43	168	1312098	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	7.47	114	1822438	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.29	117	1398993	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.38	152	669933	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.81	65	455379	48.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.94%	
35) Dibromofluoromethane	6.34	113	612085	45.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.08%	
50) Toluene-d8	9.47	98	1495601	37.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	75.20%	
62) 4-Bromofluorobenzene	12.44	95	592203	41.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.18%	
Target Compounds						
16) Acetone	3.19	43	49013	30.076	ug/l	99
20) Methylene Chloride	3.74	84	64000	4.427	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD120318\
Data File : VD060474.D
Acq On : 3 Dec 2018 14:46
Operator : VA/AP
Sample : J5764-25
Misc : 6.38g/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JC-02-113018-C

Quant Time: Dec 04 02:44:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D110618S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 19 16:31:59 2018
Response via : Initial Calibration

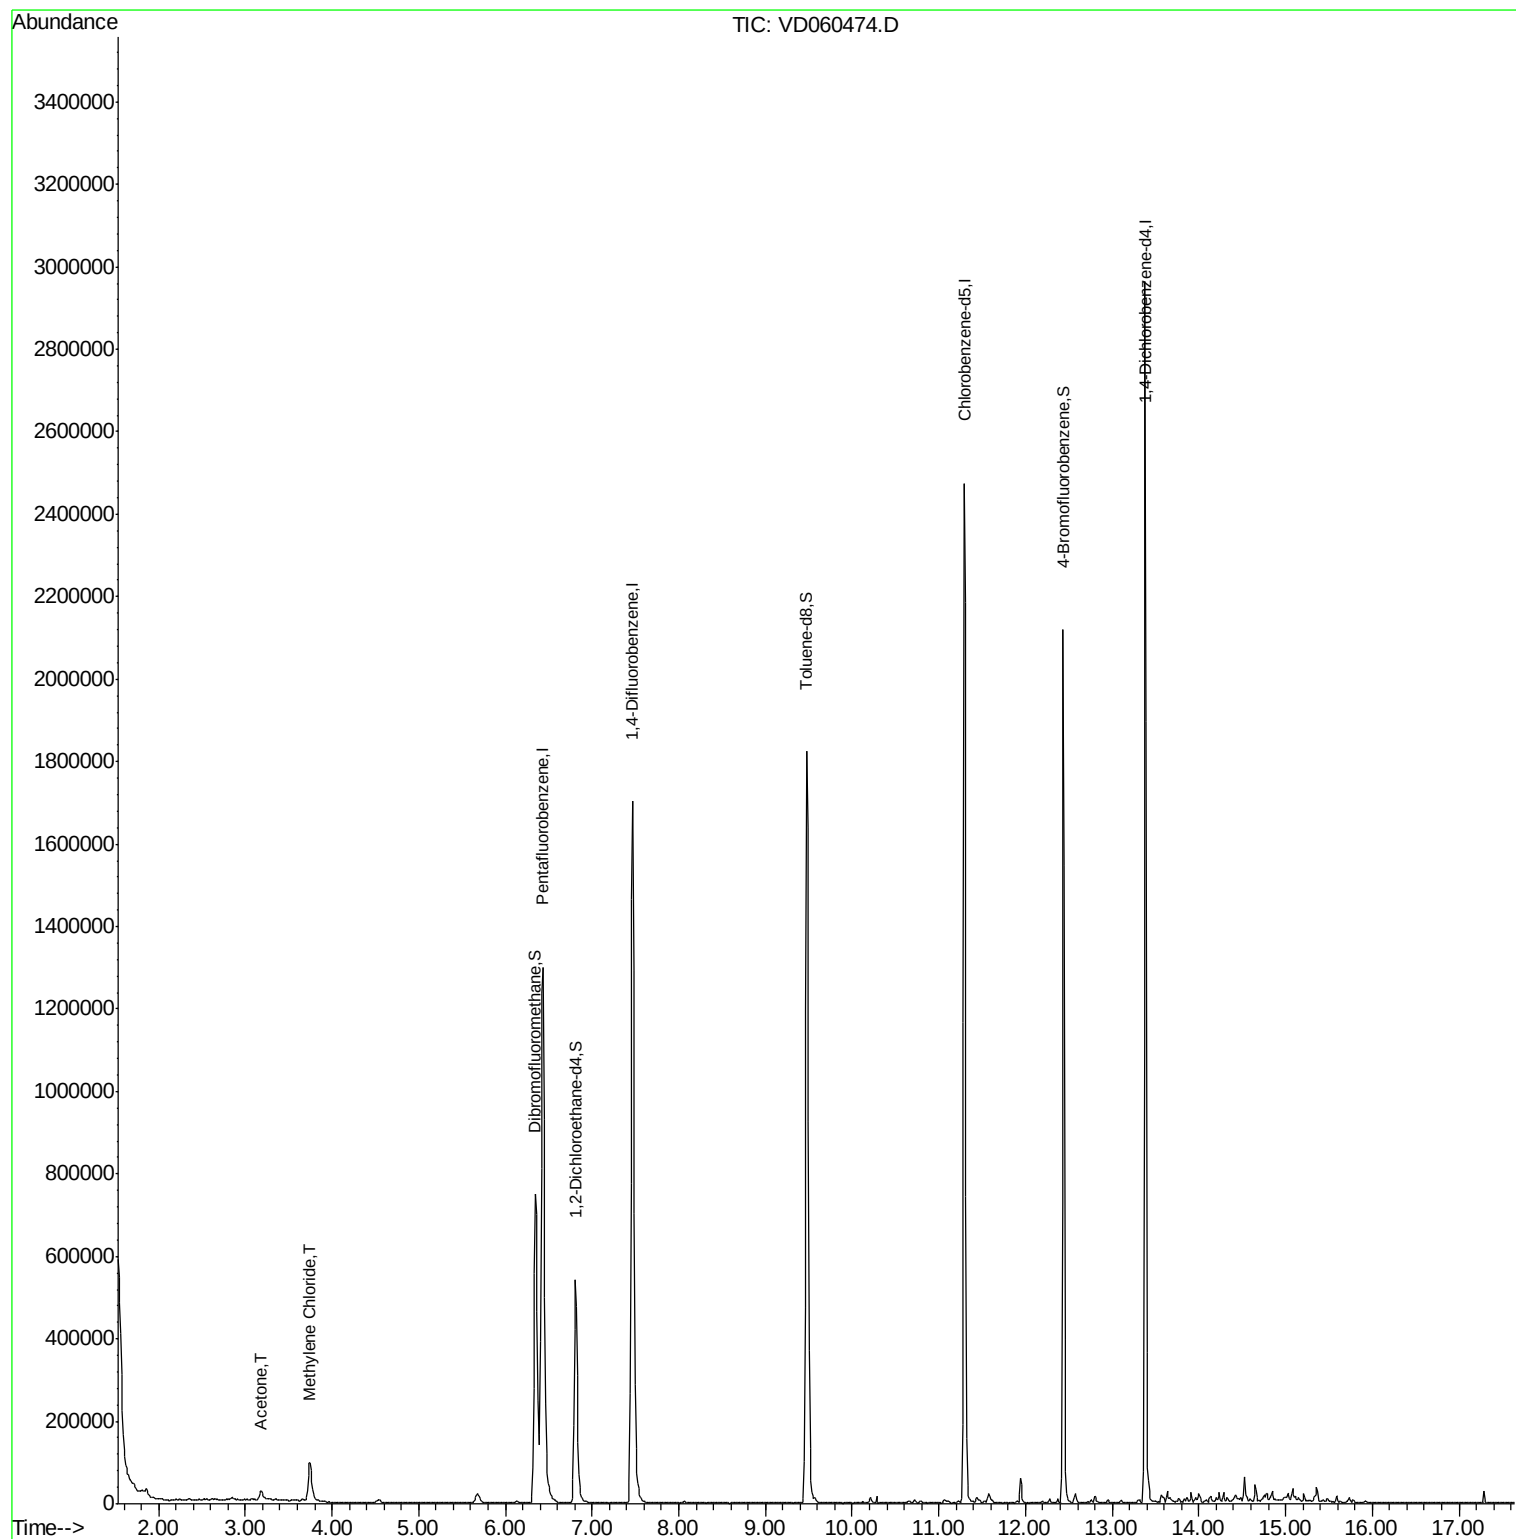

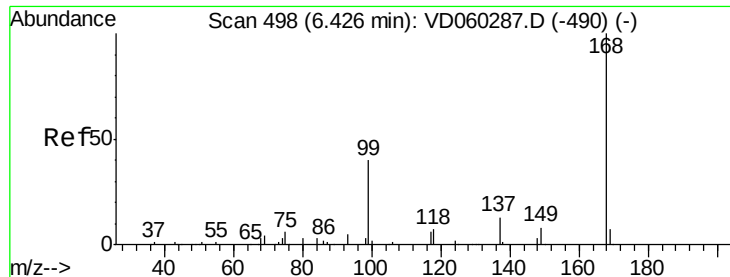

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 6.43 min Scan# 499

Delta R.T. 0.01 min

Lab File: VD060474.D

Acq: 3 Dec 2018 14:46

Instrument :

MSVOA_D

ClientSampleId :


JC-02-113018-C

Tot Ion:168 Resp: 1312098

Ion Ratio Lower Upper

168 100

99 45.2 39.8 59.8

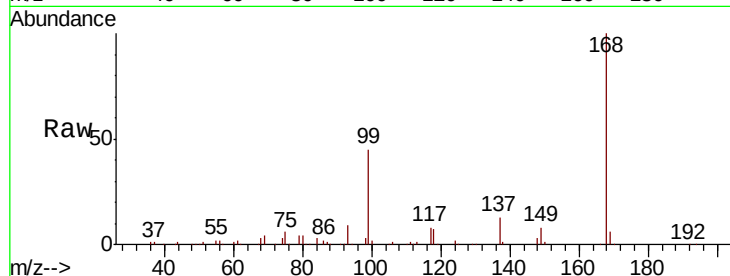

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

6.43

500000

400000



300000

200000

100000

0

Time-->

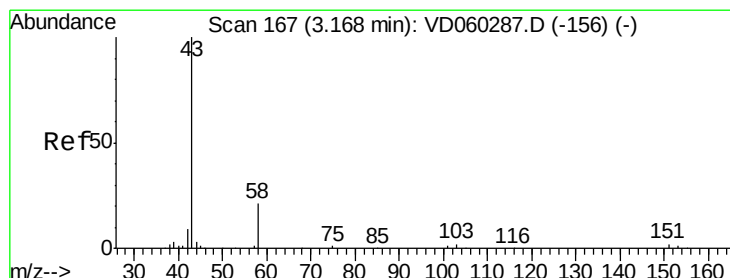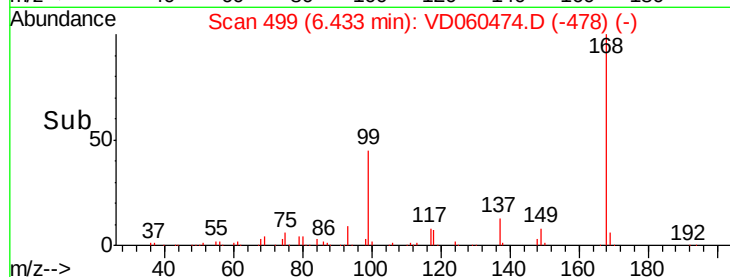

#16

Acetone

Concen: 30.076 ug/l

RT: 3.19 min Scan# 169

Delta R.T. 0.02 min

Lab File: VD060474.D


Acq: 3 Dec 2018 14:46

Tgt Ion: 43 Resp: 49013

Ion Ratio Lower Upper

43 100

58 21.5 16.9 25.3

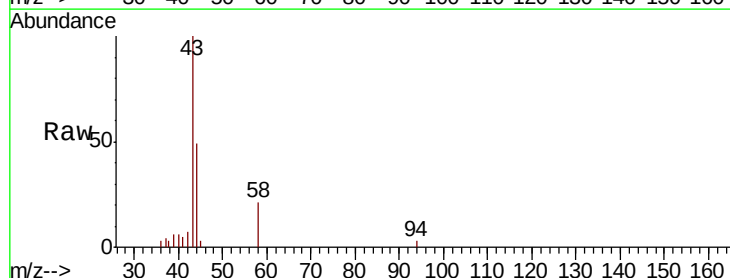

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

3.19


15000


10000

5000

0

Time-->

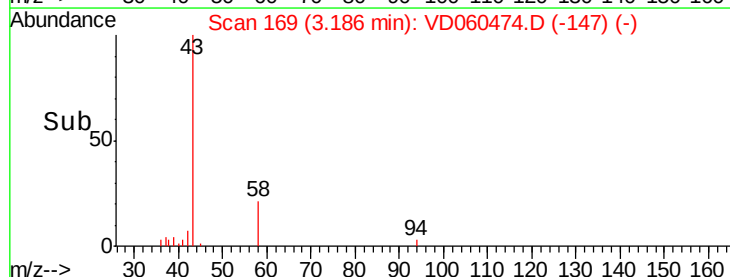


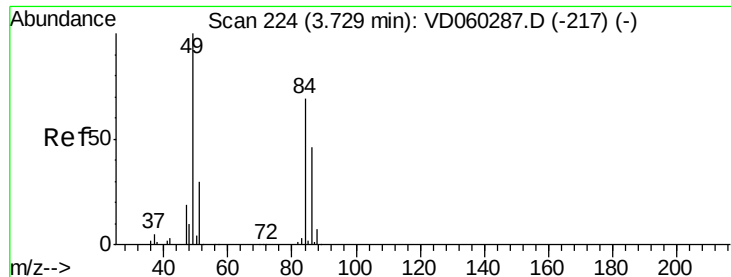




#20
Methylene Chloride
Concen: 4.427 ug/l
RT: 3.74 min Scan# 225
Delta R.T. 0.01 min
Lab File: VD060474.D
Acq: 3 Dec 2018 14:46

Instrument :
MSVOA_D
ClientSampleId :
JC-02-113018-C

Tot Ion: 84 Resp: 64000
Ion Ratio Lower Upper
84 100
49 134.3 115.6 173.4
51 40.2 35.6 53.4
86 62.8 52.3 78.5

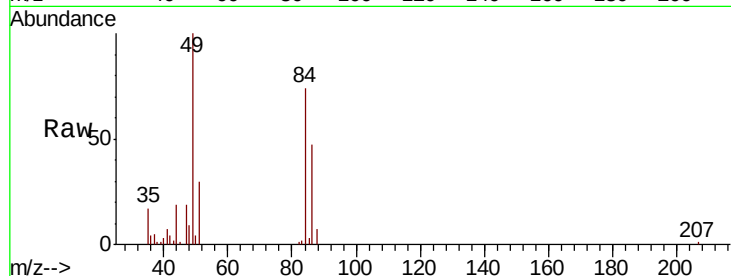


Abundance Ion 83.95 (83.65 to 84.65): VDC
Ion 48.90 (48.60 to 49.60): VDC
Ion 50.90 (50.60 to 51.60): VDC
Ion 85.90 (85.60 to 86.60): VDC

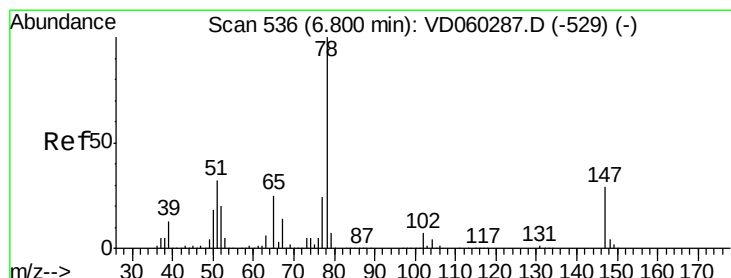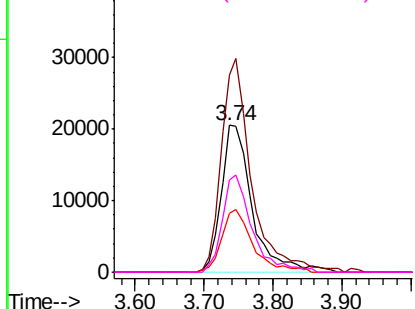
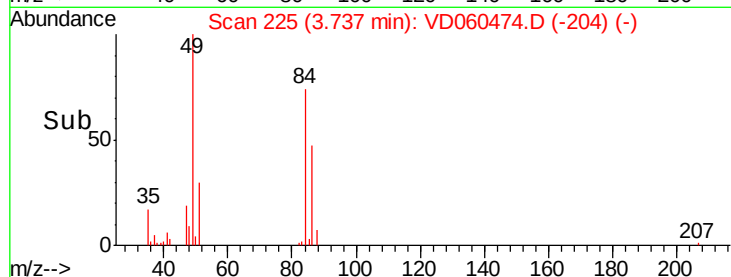



#33
1,2-Dichloroethane-d4
Concen: N.D. ug/l
RT: 6.81 min Scan# 537
Delta R.T. 0.01 min
Lab File: VD060474.D
Acq: 3 Dec 2018 14:46

Tgt Ion: 65 Resp: 455379
Ion Ratio Lower Upper
65 100
67 52.8 0.0 109.8

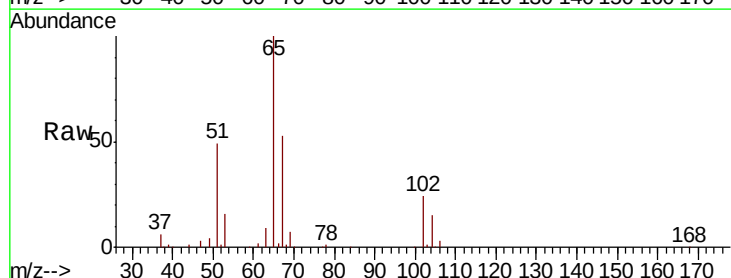

Abundance Ion 64.95 (64.65 to 65.65): VDC
Ion 66.90 (66.60 to 67.60): VDC

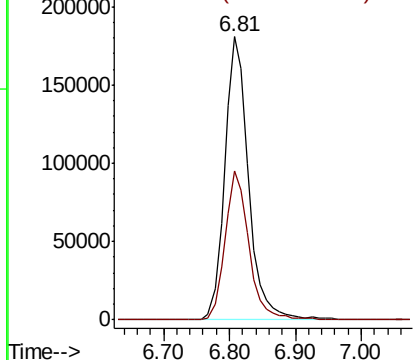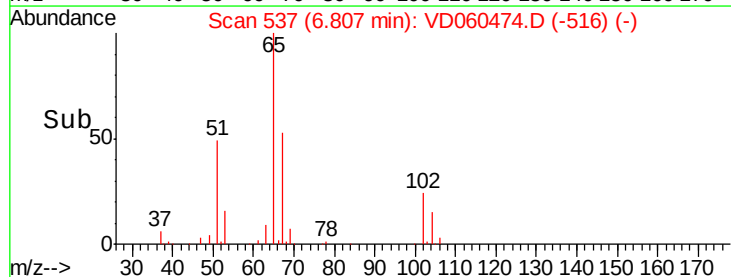


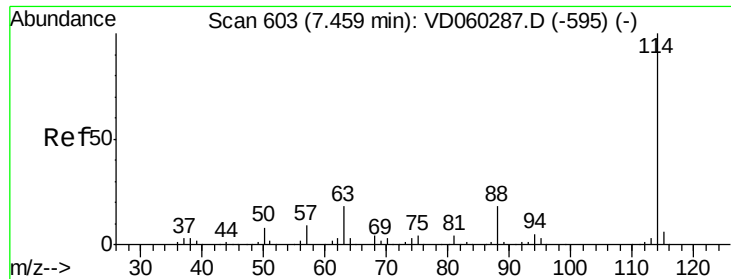




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 7.47 min Scan# 604
 Delta R.T. 0.01 min
 Lab File: VD060474.D
 Acq: 3 Dec 2018 14:46

Instrument :
 MSVOA_D
 ClientSampleId :
 JC-02-113018-C

Tot Ion:114 Resp: 1822438
 Ion Ratio Lower Upper
 114 100
 63 17.7 0.0 34.0
 88 17.7 0.0 35.4

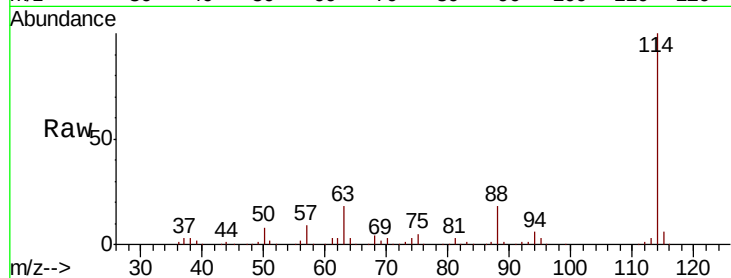


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

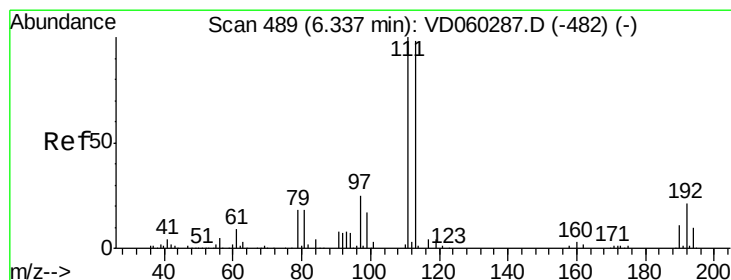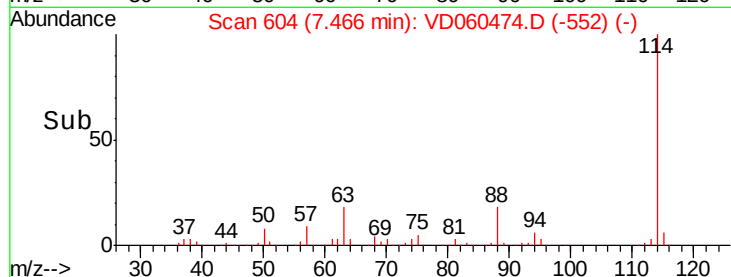
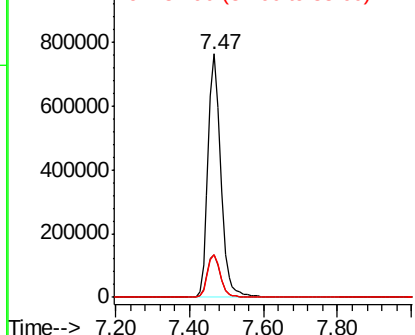



#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.34 min Scan# 490
 Delta R.T. 0.01 min
 Lab File: VD060474.D
 Acq: 3 Dec 2018 14:46

Tgt Ion:113 Resp: 612085
 Ion Ratio Lower Upper
 113 100
 111 102.2 81.6 122.4
 192 20.1 16.5 24.7

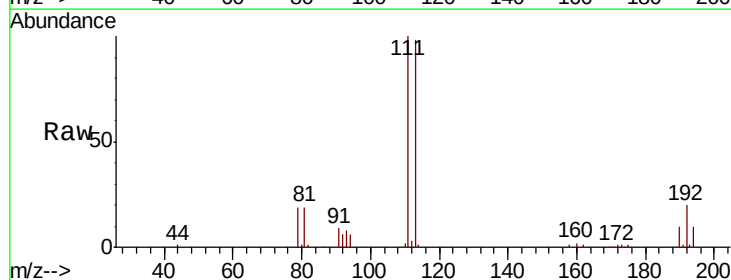

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

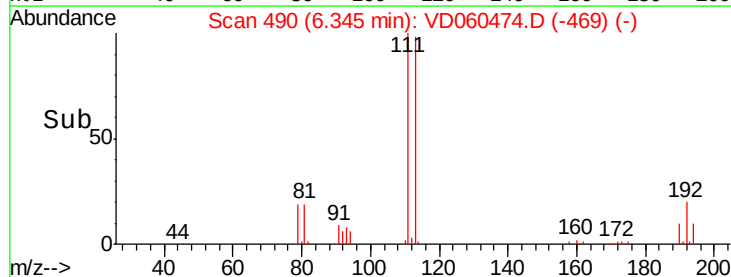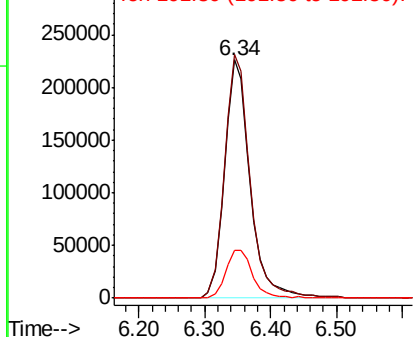

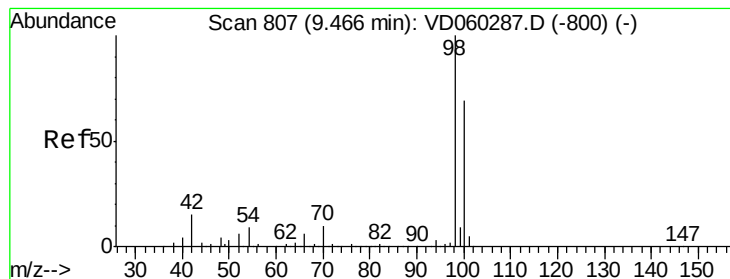

#50

Toluene-d8

Concen: N.D. ug/l

RT: 9.47 min Scan# 808

Delta R.T. 0.01 min

Lab File: VD060474.D

Acq: 3 Dec 2018 14:46

Instrument :

MSVOA_D

ClientSampleId :


JC-02-113018-C

Tot Ion: 98 Resp: 1495601

Ion Ratio Lower Upper




98 100

100 67.8 55.2 82.8

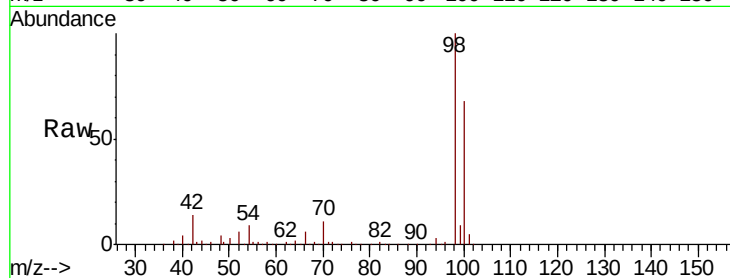

Abundance Ion 98.05 (97.75 to 98.75): VDC

Ion 100.05 (99.75 to 100.75): VDC

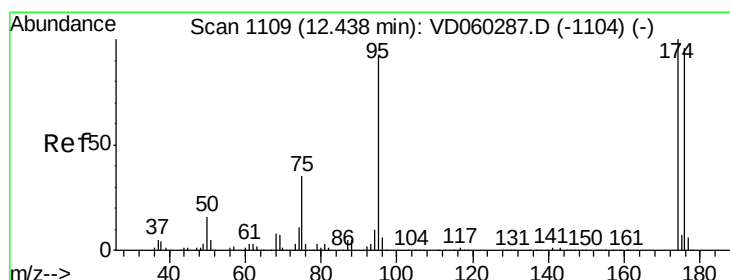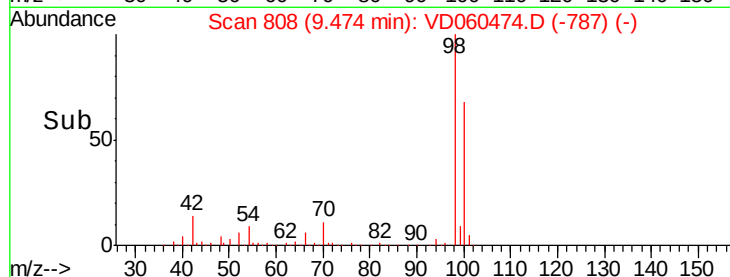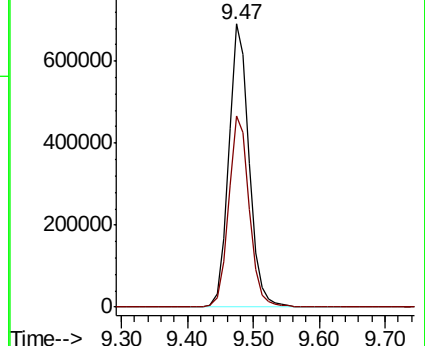

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.44 min Scan# 1109

Delta R.T. -0.00 min

Lab File: VD060474.D

Acq: 3 Dec 2018 14:46


Tgt Ion: 95 Resp: 592203

Ion Ratio Lower Upper

95 100

174 84.5 0.0 160.8



176 80.6 0.0 154.6

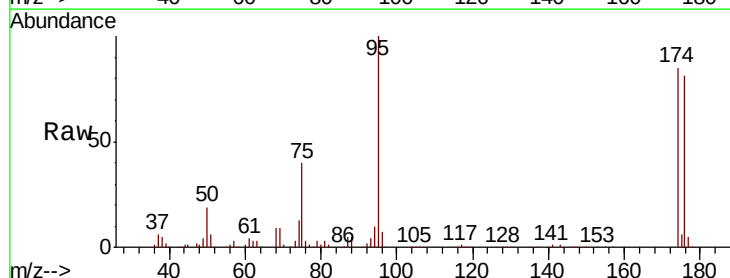


Abundance Ion 95.00 (94.70 to 95.70): VDC

Ion 173.90 (173.60 to 174.60): VDC

Ion 175.90 (175.60 to 176.60): VDC



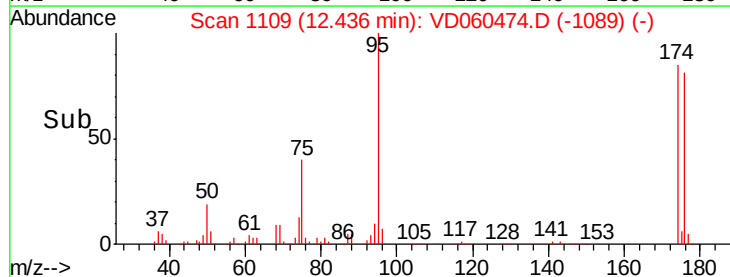
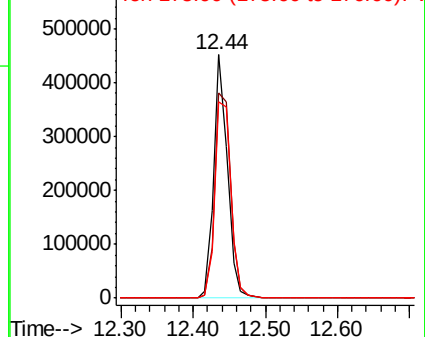


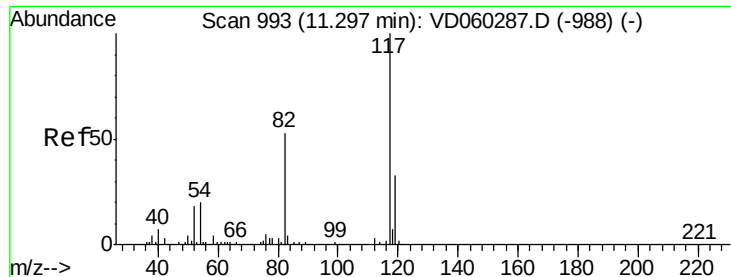

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.29 min Scan# 993
Delta R.T. -0.00 min
Lab File: VD060474.D
Acq: 3 Dec 2018 14:46

Instrument :
MSVOA_D
ClientSampleId :
JC-02-113018-C

Tot Ion:117 Resp: 1398993
Ion Ratio Lower Upper
117 100
82 55.6 43.7 65.5
119 32.5 26.1 39.1

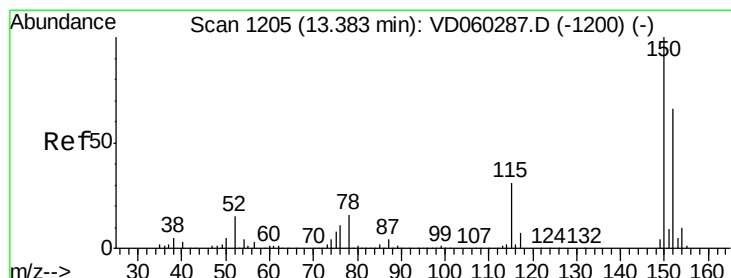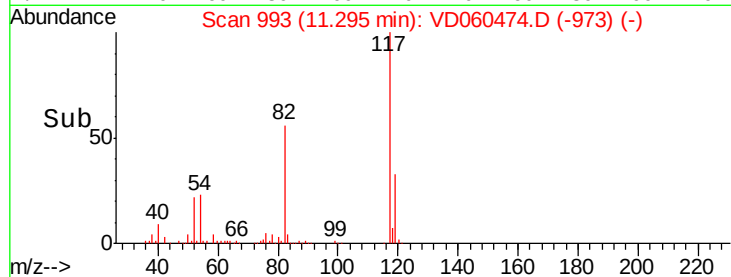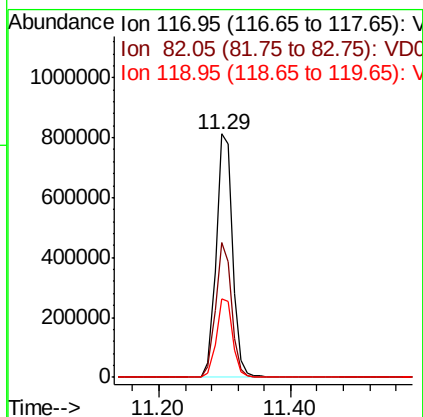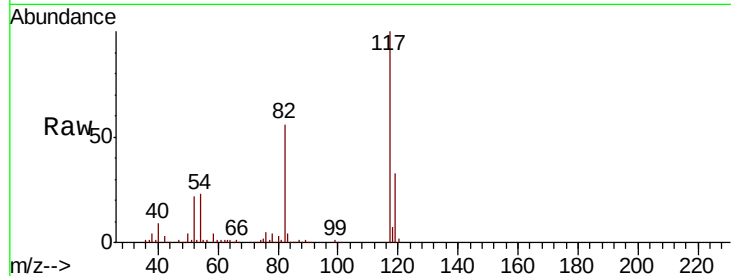

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.38 min Scan# 1205
Delta R.T. -0.00 min
Lab File: VD060474.D
Acq: 3 Dec 2018 14:46

Tgt Ion:152 Resp: 669933
Ion Ratio Lower Upper
152 100
115 54.7 24.1 72.3
150 157.0 0.0 310.6

