

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD120320\
 Data File : VD067858.D
 Acq On : 03 Dec 2020 10:27
 Operator : VA/SY
 Sample : VD1203SBL01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1203SBL01

Quant Time: Dec 03 14:30:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120120S.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 02 08:05:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	246856	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	361940	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	325319	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	156531	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.33	65	121166	45.72	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	91.44%
35) Dibromofluoromethane	7.91	113	105740	43.66	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	87.32%
50) Toluene-d8	10.34	98	402145	46.13	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	92.26%
62) 4-Bromofluorobenzene	12.64	95	132778	44.05	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	88.10%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD120320\
Data File : VD067858.D
Acq On : 03 Dec 2020 10:27
Operator : VA/SY
Sample : VD1203SBL01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1203SBL01

Quant Time: Dec 03 14:30:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D120120S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 02 08:05:58 2020
Response via : Initial Calibration

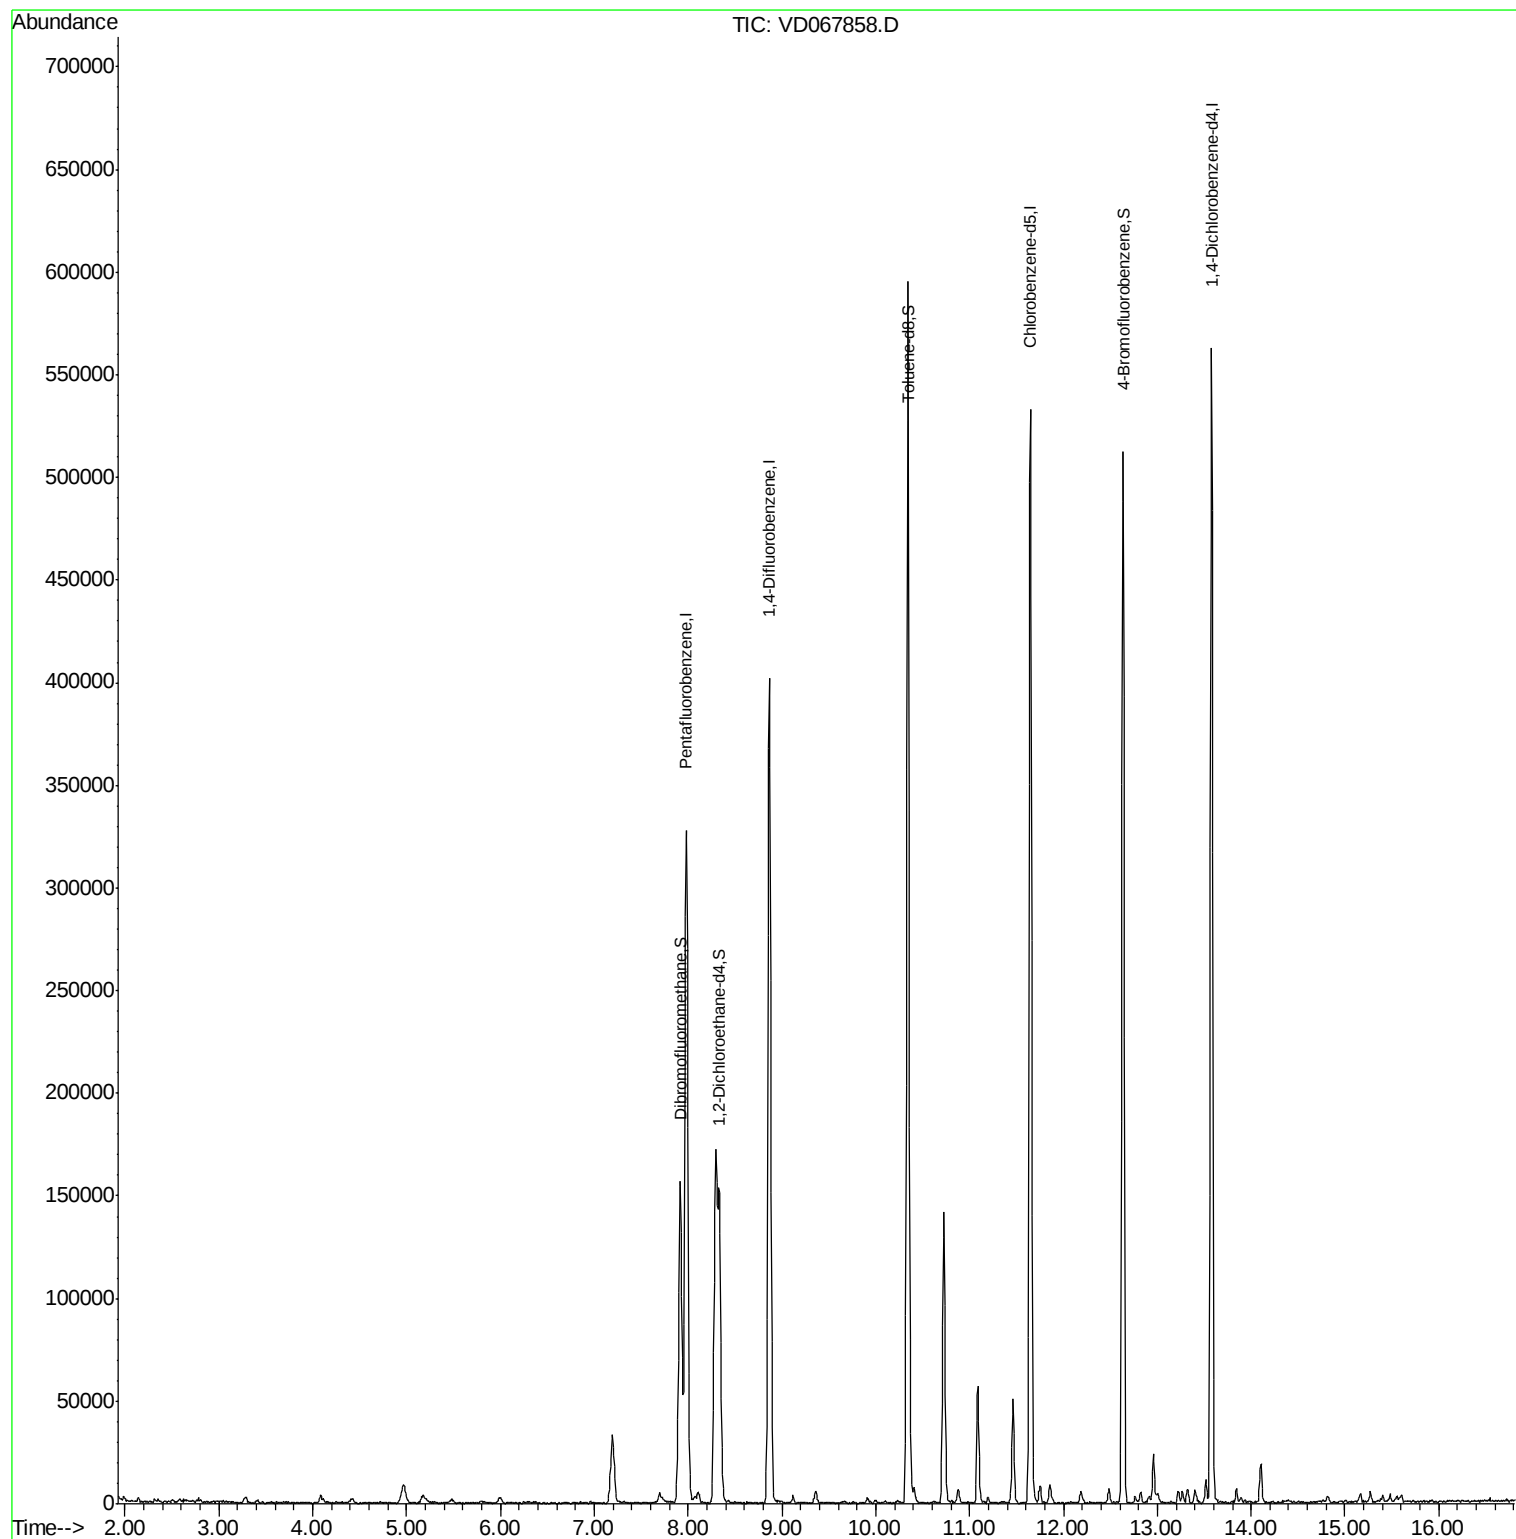

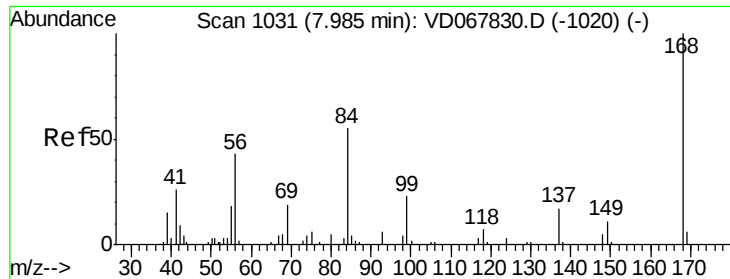

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067858.D

Acq: 03 Dec 2020 10:27

Instrument :

MSVOA_D

ClientSampleId :


VD1203SBL01

Tot Ion:168 Resp: 246856

Ion Ratio Lower Upper




168 100

99 55.6 47.1 70.7

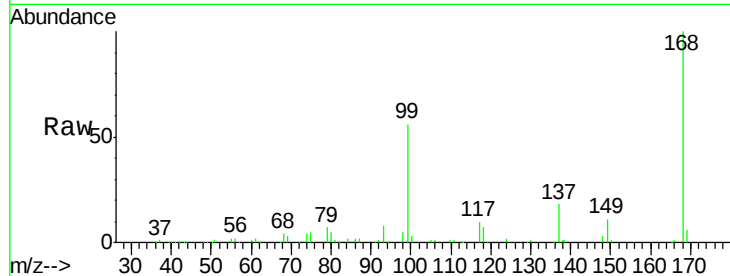

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

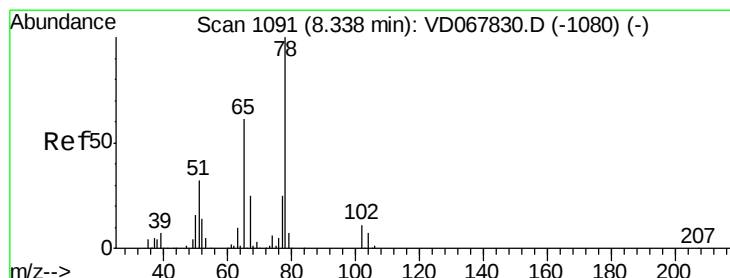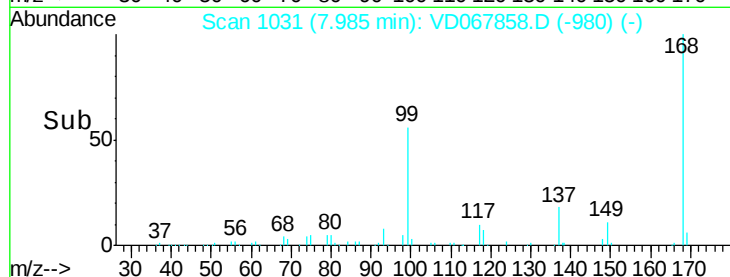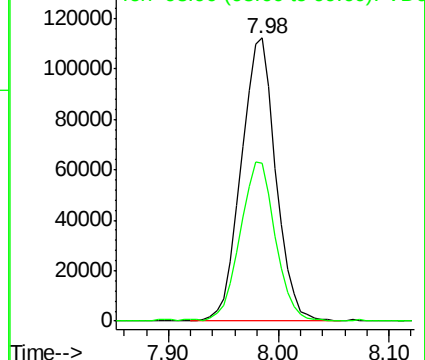

#33

1,2-Dichloroethane-d4

Concen: 45.721 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD067858.D


Acq: 03 Dec 2020 10:27

Tgt Ion: 65 Resp: 121166

Ion Ratio Lower Upper



65 100


67 49.2 0.0 92.0

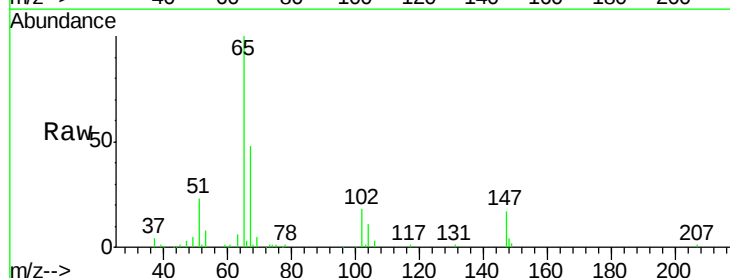

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

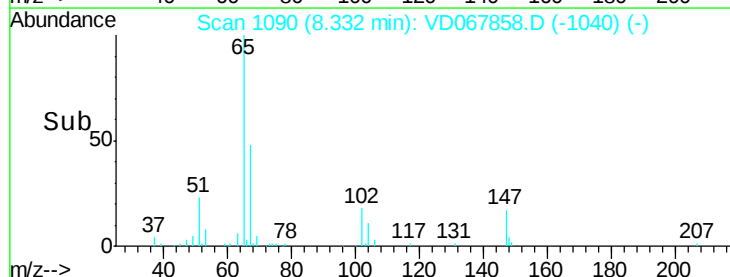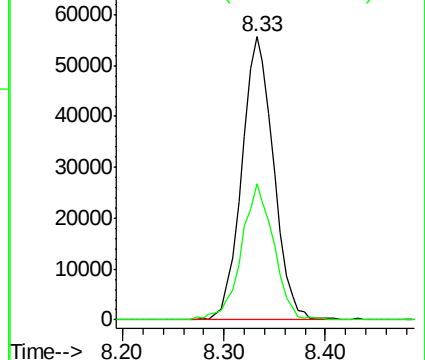

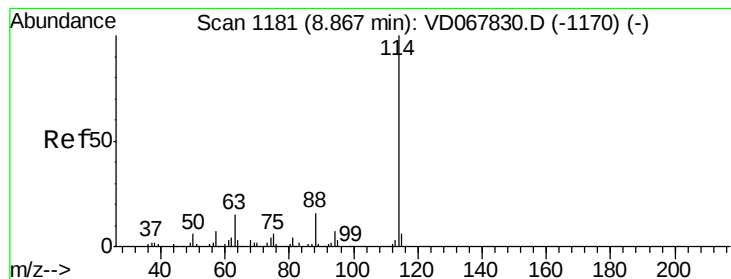

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD067858.D

Acq: 03 Dec 2020 10:27

Instrument :

MSVOA_D

ClientSampleId :

VD1203SBL01


Tot Ion:114 Resp: 361940

Ion Ratio Lower Upper

114 100

63 17.3 0.0 30.8




88 14.3 0.0 31.8

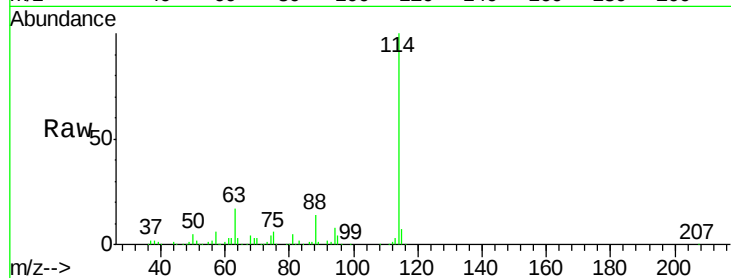

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

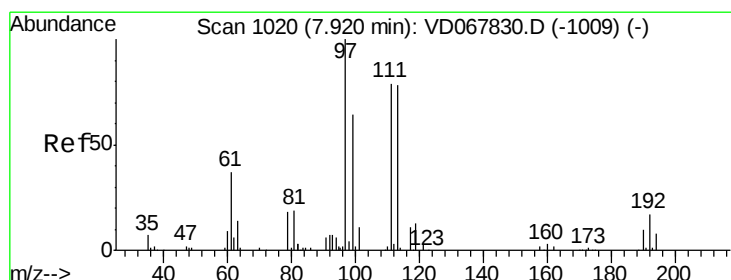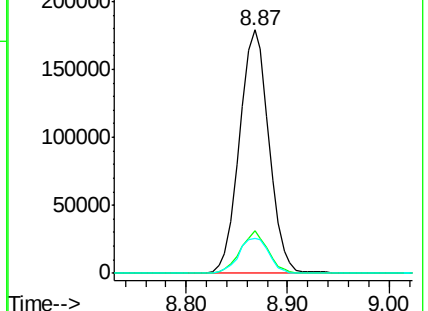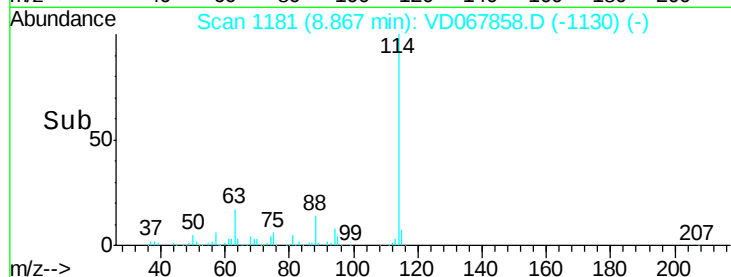

#35

Dibromofluoromethane

Concen: 43.660 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. -0.01 min

Lab File: VD067858.D

Acq: 03 Dec 2020 10:27


Tgt Ion:113 Resp: 105740

Ion Ratio Lower Upper

113 100

111 102.4 81.2 121.8



192 21.9 16.8 25.2

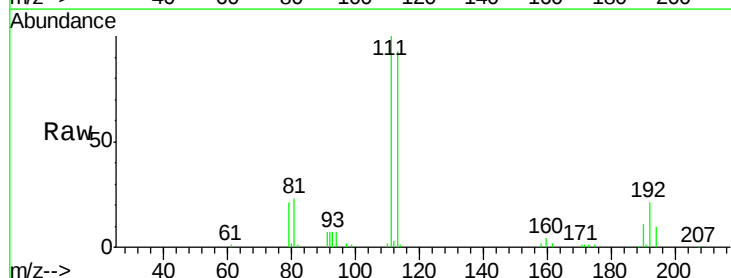


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

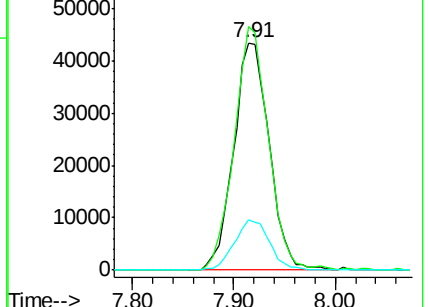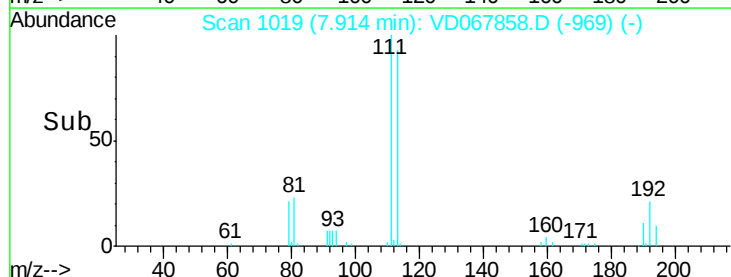

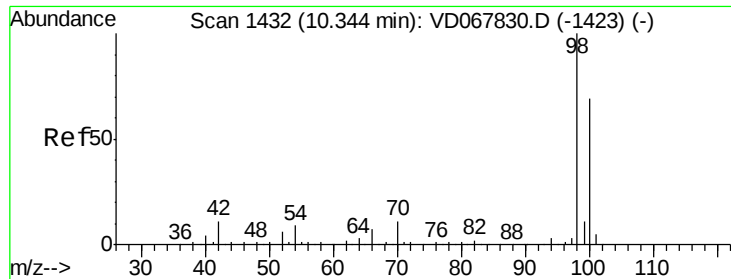

#50

Toluene-d8

Concen: 46.126 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD067858.D

Acq: 03 Dec 2020 10:27

Instrument :

MSVOA_D

ClientSampleId :


VD1203SBL01

Tot Ion: 98 Resp: 402145

Ion Ratio Lower Upper

98 100

100 66.8 52.9 79.3

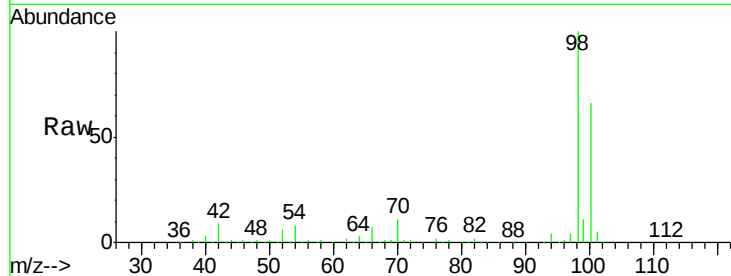

Abundance Ion 98.00 (97.70 to 98.70): VD0

Ion 100.00 (99.70 to 100.70): VD

10.34

250000

200000



150000

100000

50000

0

Time-->

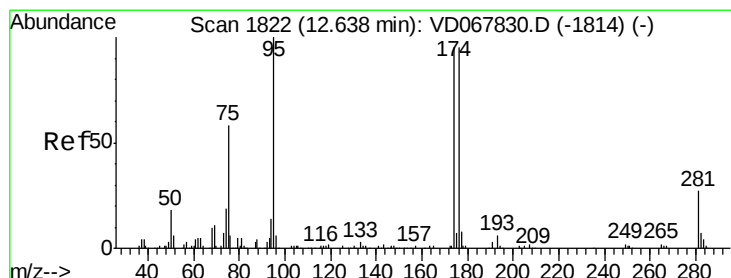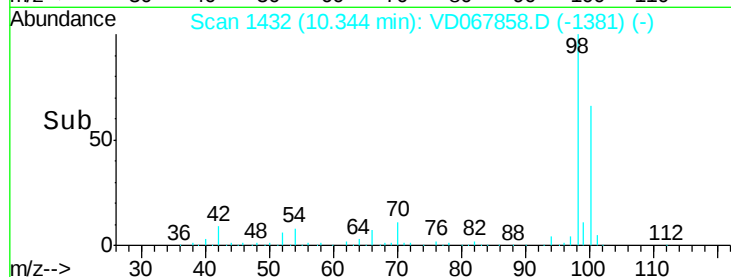

#62

4-Bromofluorobenzene

Concen: 44.051 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD067858.D

Acq: 03 Dec 2020 10:27


Tgt Ion: 95 Resp: 132778

Ion Ratio Lower Upper

95 100

174 93.3 0.0 186.0

176 89.4 0.0 184.2

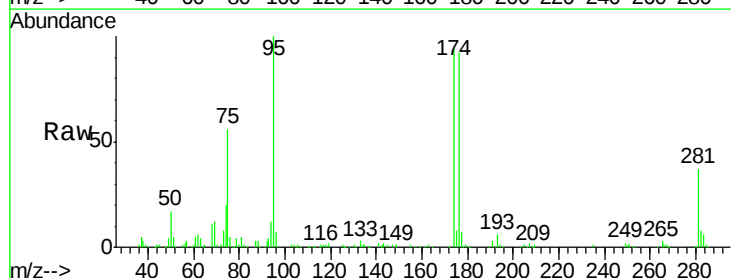

Abundance Ion 94.90 (94.60 to 95.60): VD0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

100000

80000


60000


40000

20000

0

Time-->




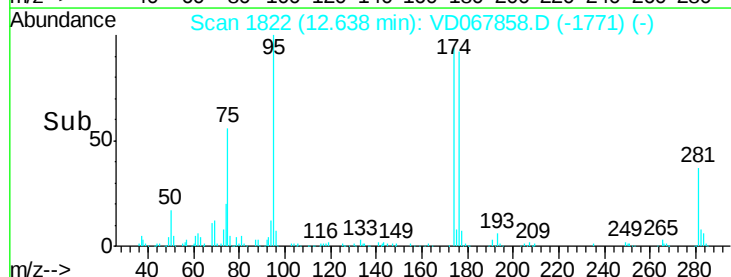


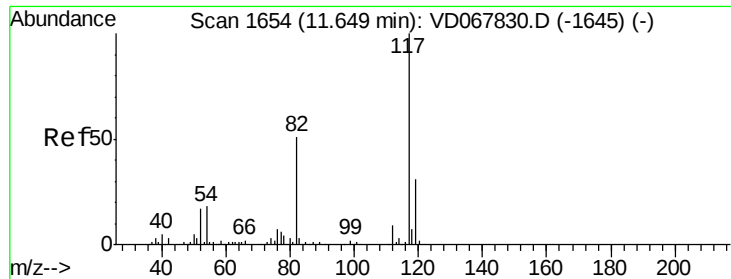

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067858.D
Acq: 03 Dec 2020 10:27

Instrument :
MSVOA_D
ClientSampleId :
VD1203SBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	50.0	40.6	60.8
119	31.9	25.1	37.7

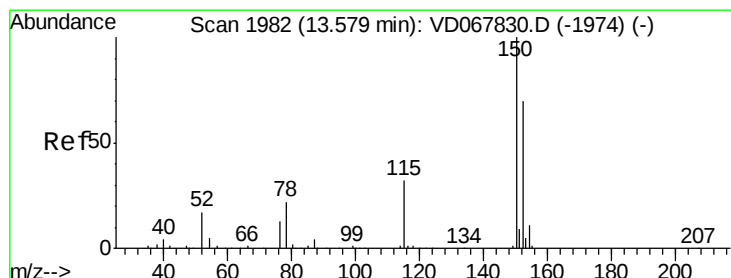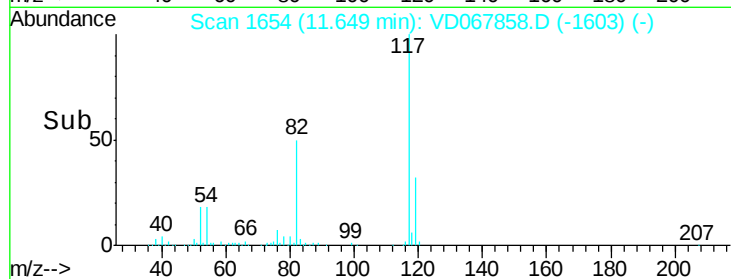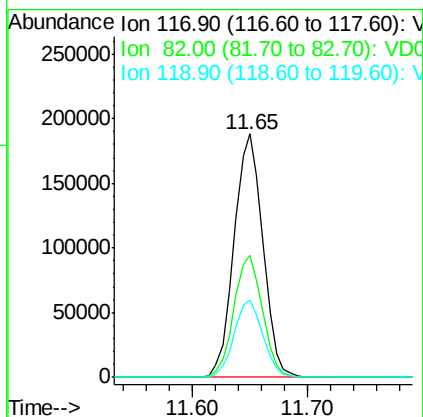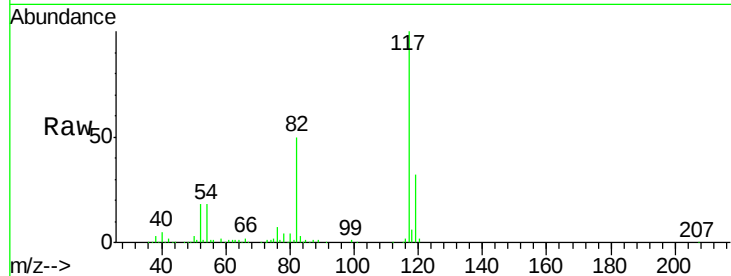

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. 0.00 min
Lab File: VD067858.D
Acq: 03 Dec 2020 10:27

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.3	29.1	87.4
150	161.6	0.0	339.0

