

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120321\
 Data File : VD071137.D
 Acq On : 03 Dec 2021 17:02
 Operator : VA/SY
 Sample : M4939-01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 OR-03-120321

Quant Time: Dec 04 03:51:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 29 17:54:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	40675	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.861	114	74012	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	82749	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	45187	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	36704	76.903	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	153.800%
35) Dibromofluoromethane	7.914	113	27062	57.420	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	114.840%
50) Toluene-d8	10.338	98	93815	52.307	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.620%
62) 4-Bromofluorobenzene	12.626	95	43745	70.363	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	140.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120321\
Data File : VD071137.D
Acq On : 03 Dec 2021 17:02
Operator : VA/SY
Sample : M4939-01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
OR-03-120321

Quant Time: Dec 04 03:51:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 29 17:54:09 2021
Response via : Initial Calibration




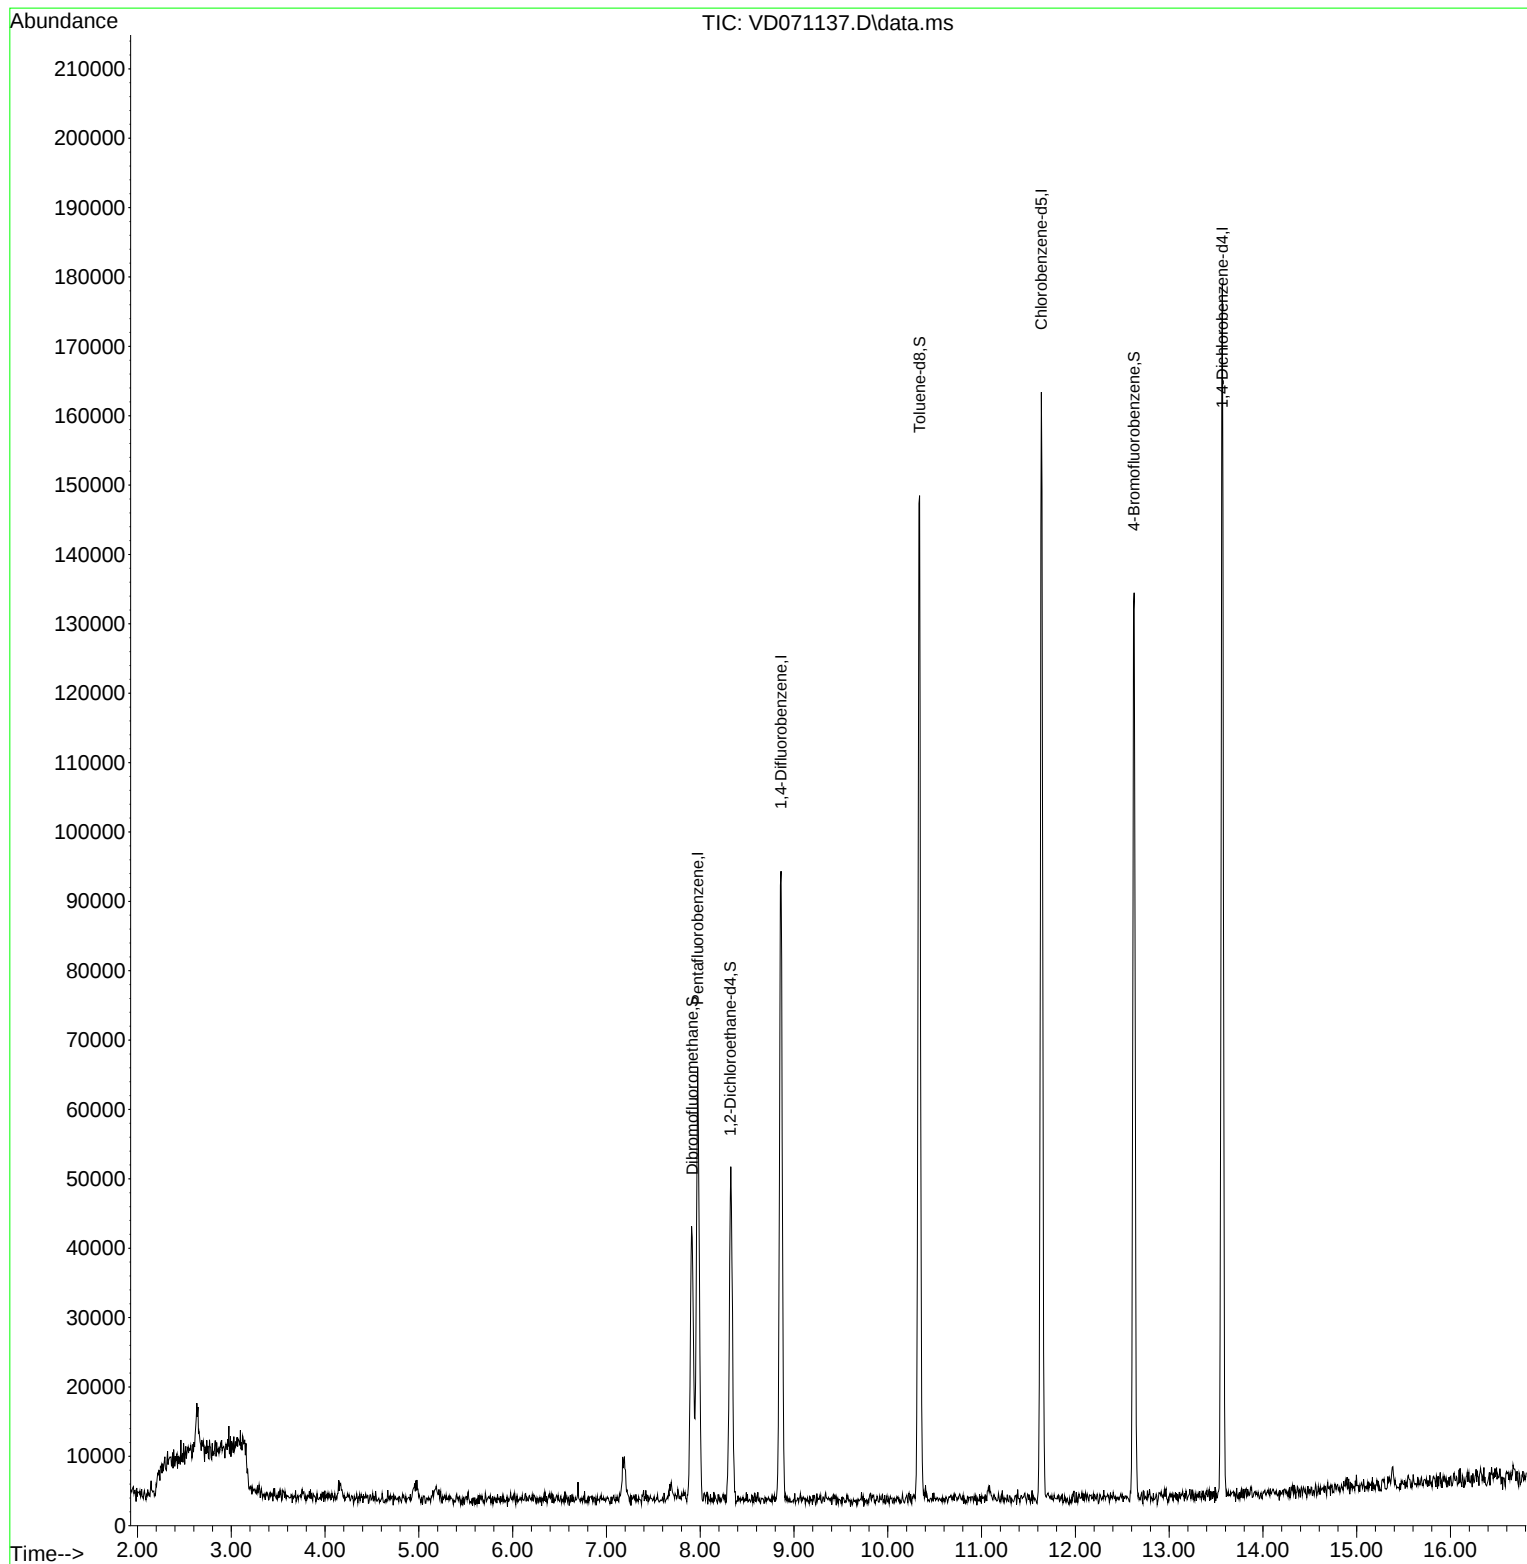


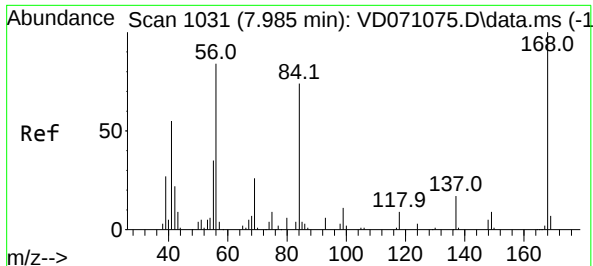

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. -0.012 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02




Instrument :
MSVOA_D
ClientSampleId :
OR-03-120321


Tgt Ion:168 Resp: 40675
Ion Ratio Lower Upper
168 100
99 57.2 46.6 69.8

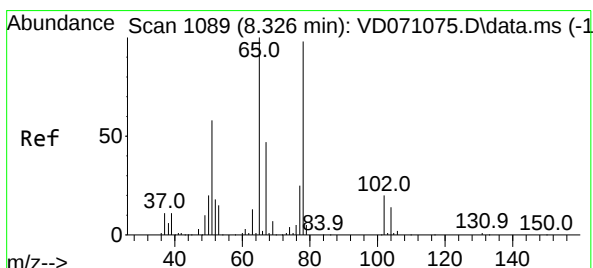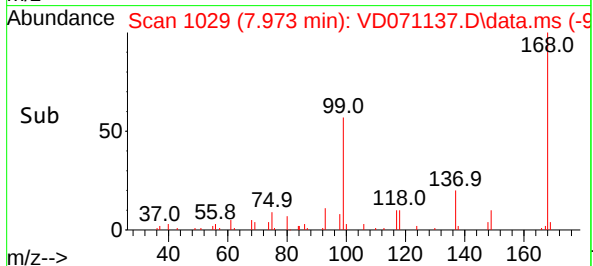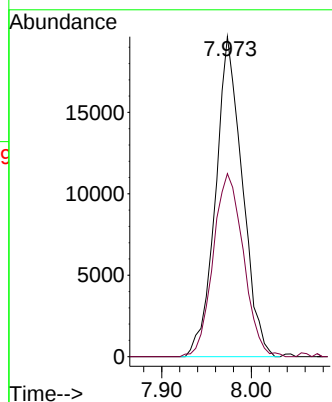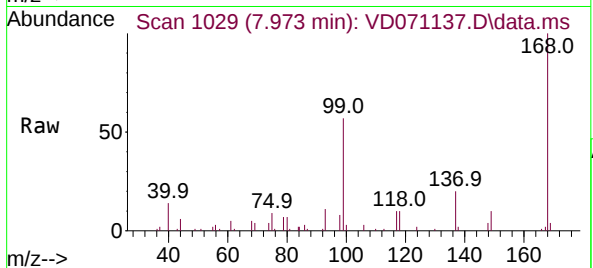

#33
1,2-Dichloroethane-d4
Concen: 76.903 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. -0.006 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02

Tgt Ion: 65 Resp: 36704
Ion Ratio Lower Upper
65 100
67 53.0 0.0 112.2

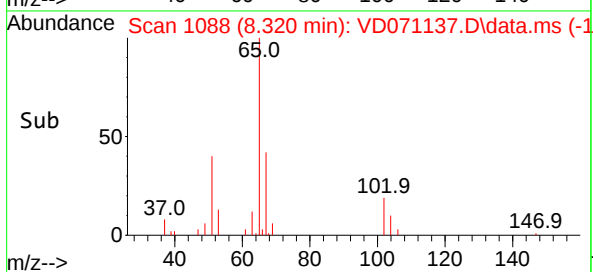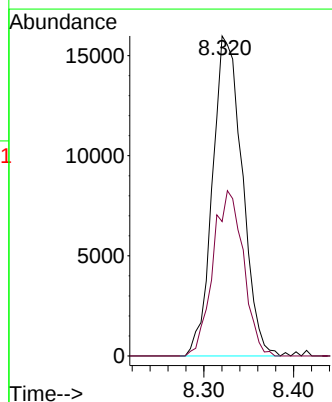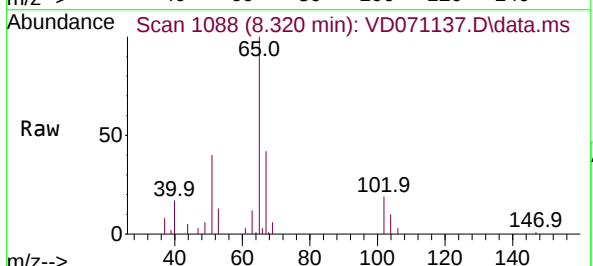

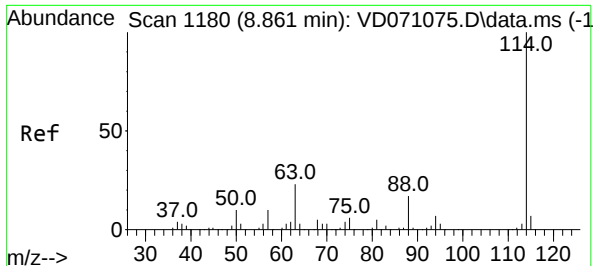

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071137.D

Acq: 03 Dec 2021 17:02

Instrument :

MSVOA_D

ClientSampleId :

OR-03-120321





Tgt Ion:114 Resp: 74012

Ion Ratio Lower Upper

114 100

63 25.1 0.0 41.8

88 15.3 0.0 32.8

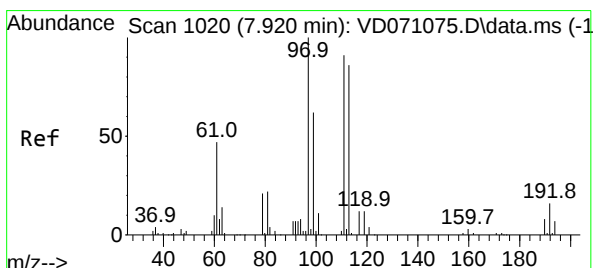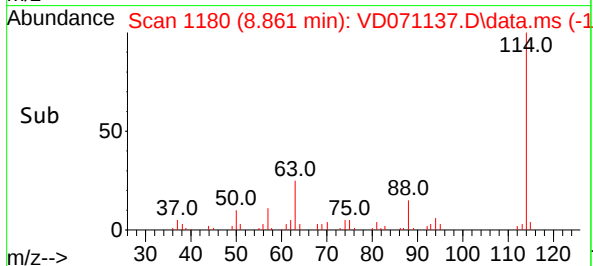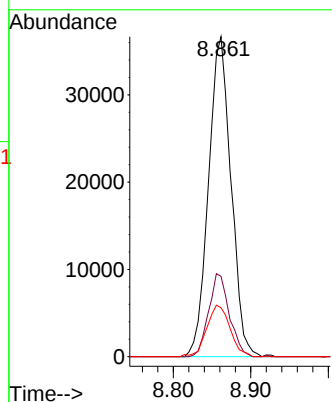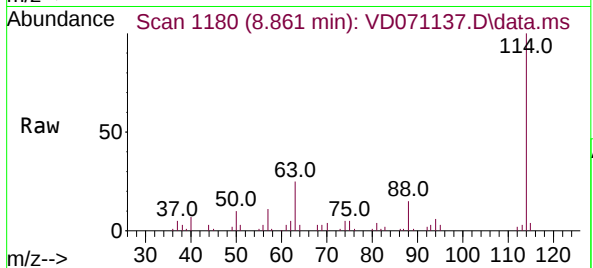

#35

Dibromofluoromethane

Concen: 57.420 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.006 min

Lab File: VD071137.D

Acq: 03 Dec 2021 17:02




Tgt Ion:113 Resp: 27062


Ion Ratio Lower Upper

113 100

111 106.8 82.0 123.0

192 18.3 15.2 22.8


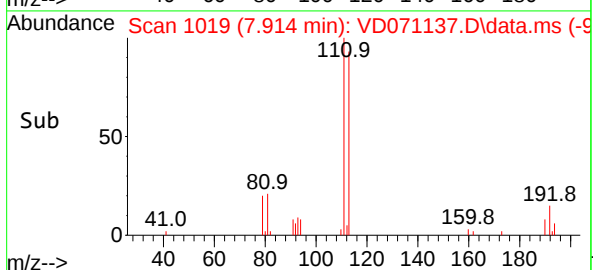
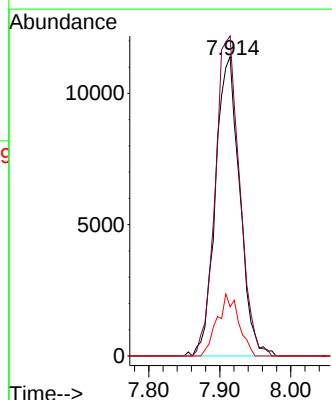
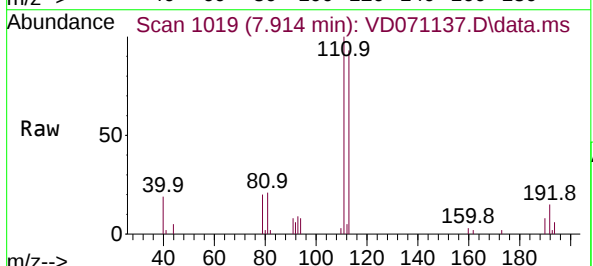


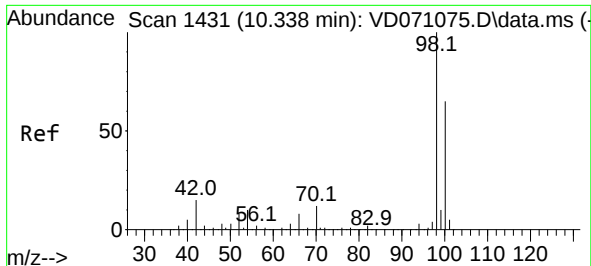

#50
Toluene-d8
Concen: 52.307 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02




Instrument :
MSVOA_D
ClientSampleId :
OR-03-120321


Tgt Ion: 98 Resp: 93815
Ion Ratio Lower Upper
98 100
100 65.6 51.8 77.6

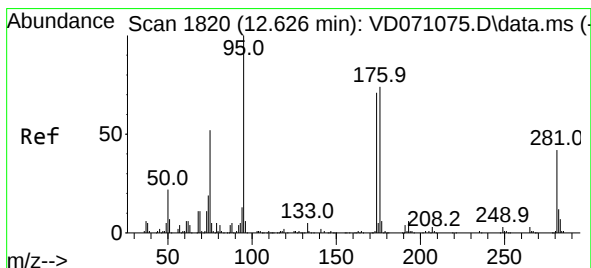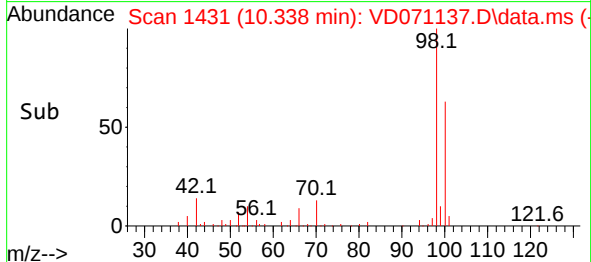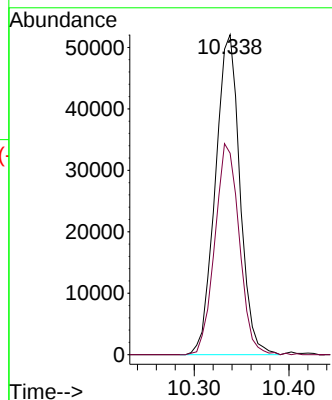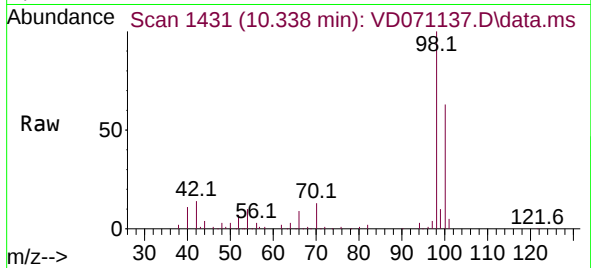

#62
4-Bromofluorobenzene
Concen: 70.363 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02

Tgt Ion: 95 Resp: 43745
Ion Ratio Lower Upper
95 100
174 74.5 0.0 159.4
176 70.4 0.0 154.0


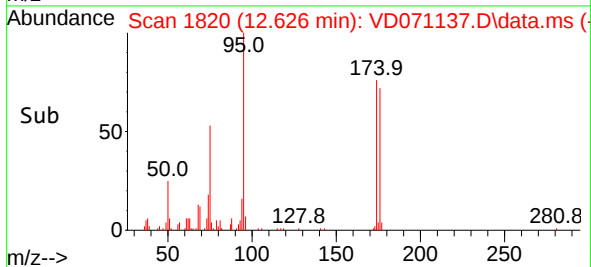
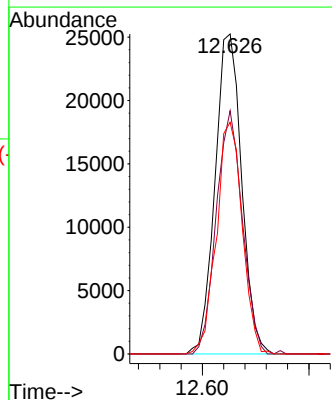
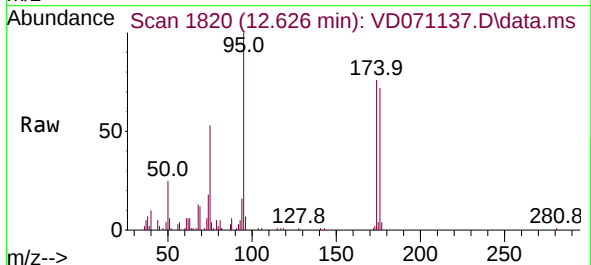


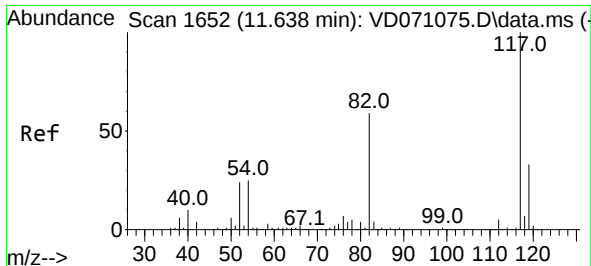

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02

Instrument :
MSVOA_D
ClientSampleId :
OR-03-120321

Tgt Ion:117 Resp: 82749
Ion Ratio Lower Upper
117 100
82 59.3 44.7 67.1
119 29.9 26.2 39.4

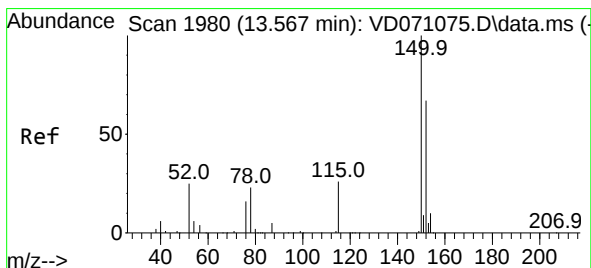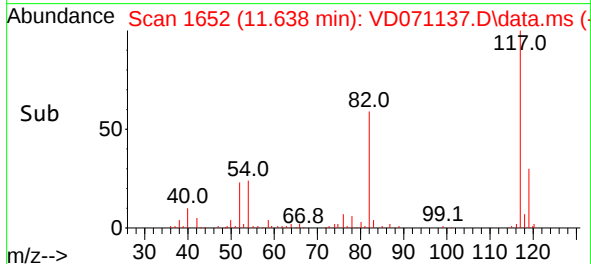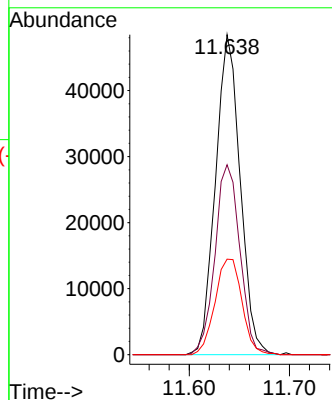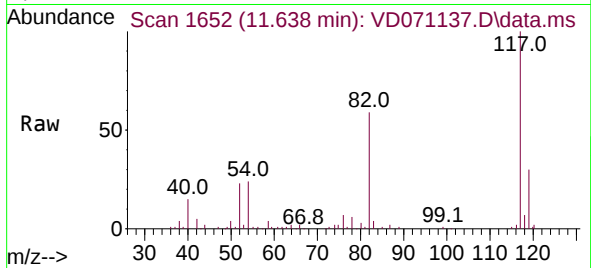

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.000 min
Lab File: VD071137.D
Acq: 03 Dec 2021 17:02

Tgt Ion:152 Resp: 45187
Ion Ratio Lower Upper
152 100
115 56.2 29.8 89.3
150 155.9 0.0 349.2

