




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
Data File : VD077734.D
Acq On : 04 Dec 2023 10:33
Operator : JC/SY
Sample : 04929-12RE
Misc : 2.84G/10ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B63RE

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:04:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 05 00:04:05 2023
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/05/2023
Supervised By :Semsettin Yesilyurt 12/05/2023

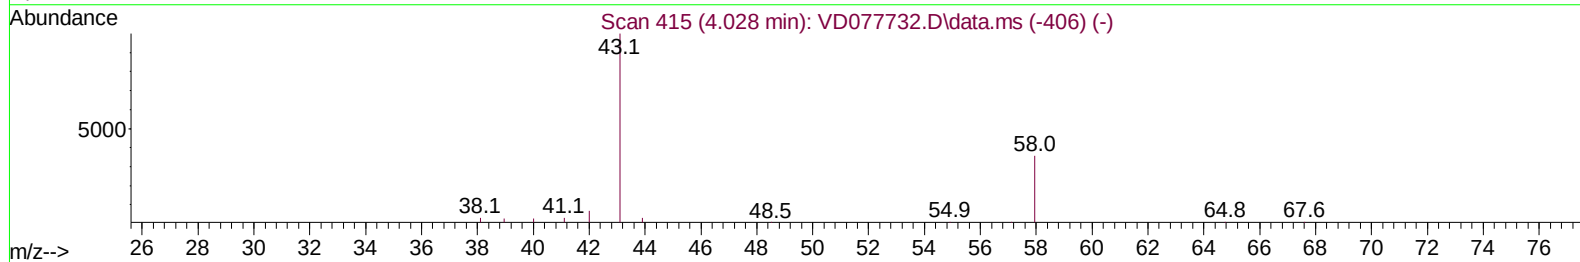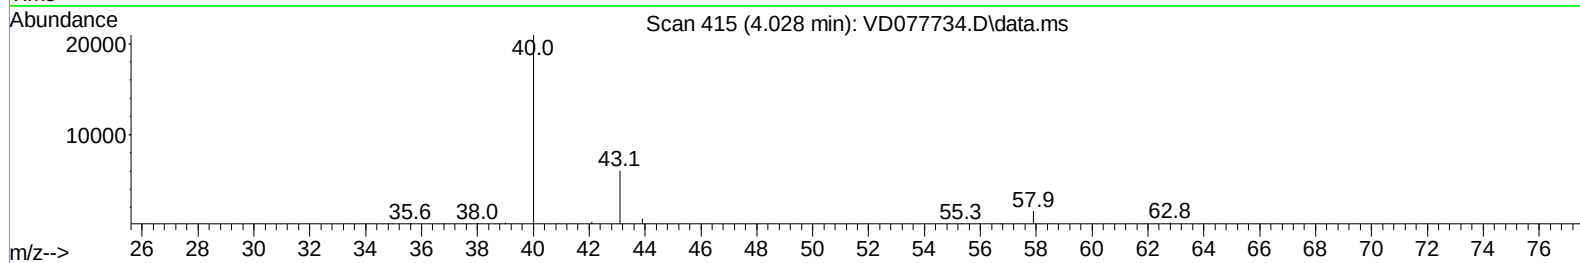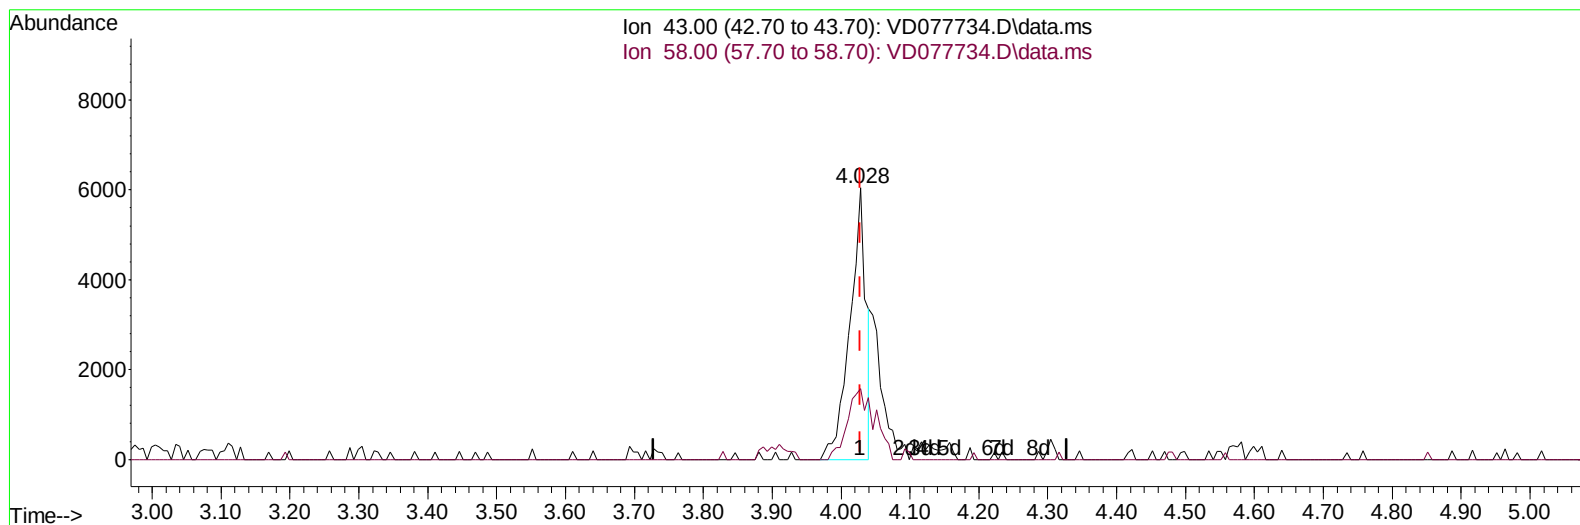

TIC: VD077734.D\data.ms

(13) Acetone (T)

4.028min (+ 0.000) 8.39 ug/L

response 9834

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	34.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
 Data File : VD077734.D
 Acq On : 04 Dec 2023 10:33
 Operator : JC/SY
 Sample : 04929-12RE
 Misc : 2.84G/10ml/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B63RE

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:04:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 05 00:04:05 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/05/2023
 Supervised By :Semsettin Yesilyurt 12/05/2023

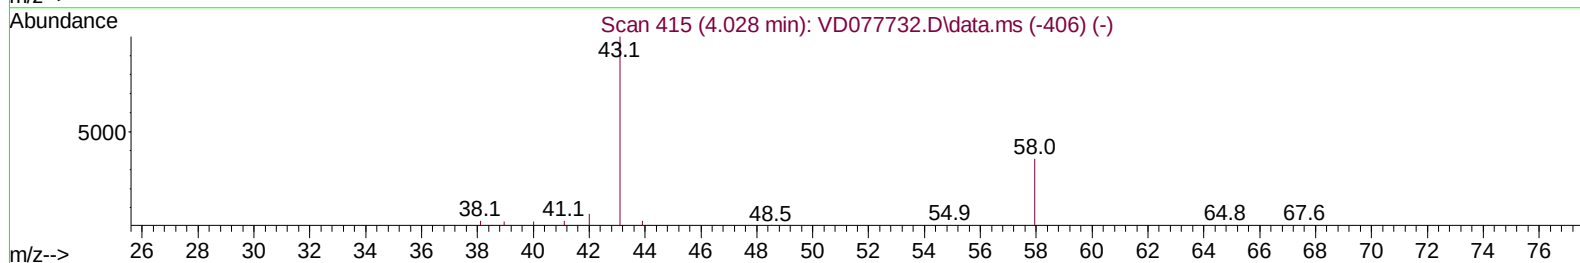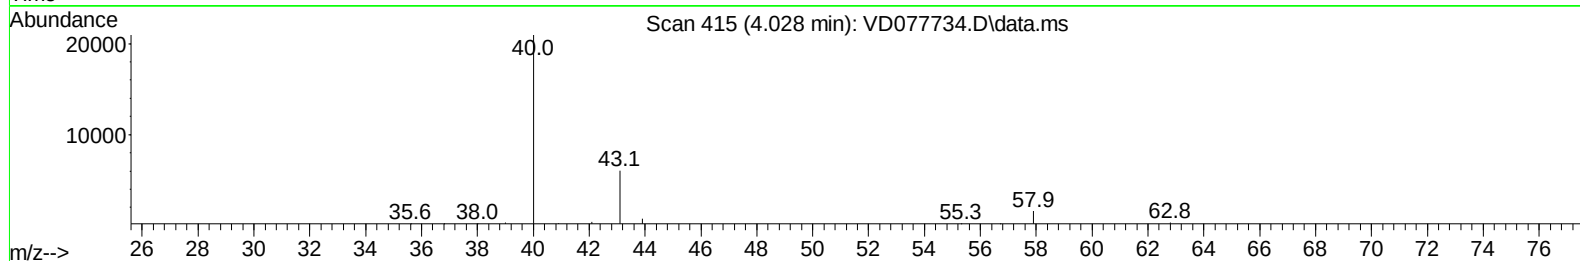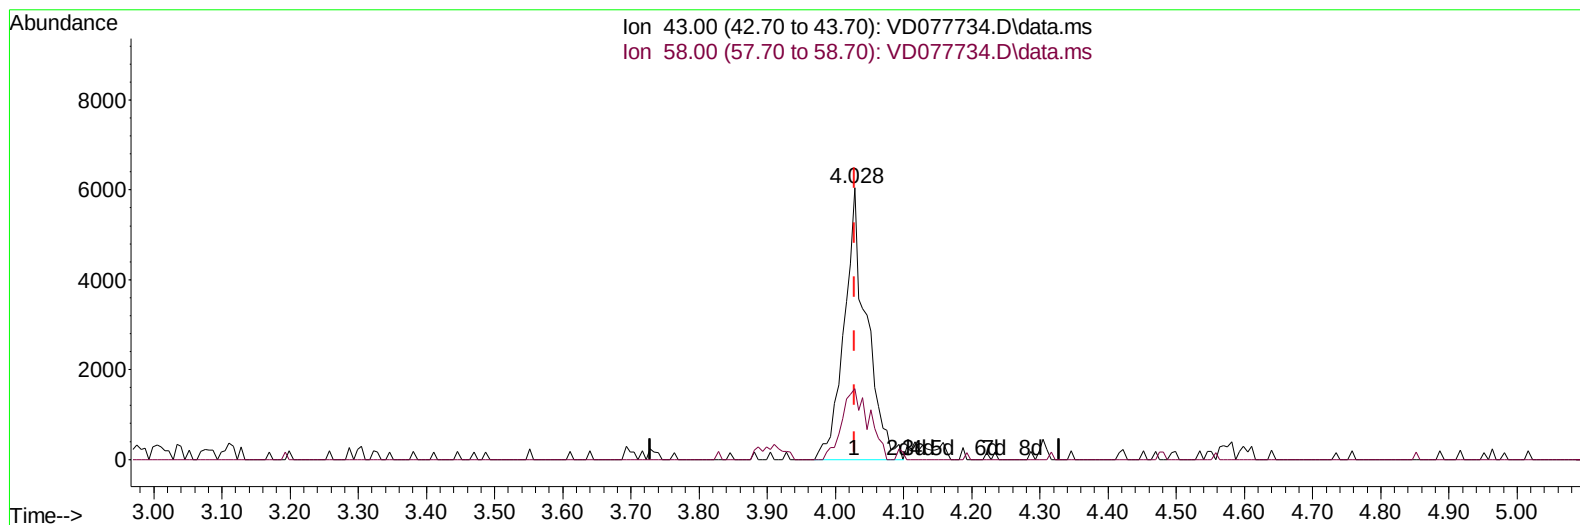

TIC: VD077734.D\data.ms

(13) Acetone (T)

4.028min (+ 0.000) 11.71 ug/L m

response 13716

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.60	24.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
 Data File : VD077734.D
 Acq On : 04 Dec 2023 10:33
 Operator : JC/SY
 Sample : 04929-12RE
 Misc : 2.84G/10mL/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0B63RE

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:04:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 05 00:04:05 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/05/2023
 Supervised By :Semsettin Yesilyurt 12/05/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		265294	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		142249	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		25840	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.281	65		223753	30.928	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	123.720%	
7) Chloroethane-d5	2.811	69		193015	33.471	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	133.880%	
11) 1,1-Dichloroethene-d2	3.928	65		51573	27.493	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	109.960%	
21) 2-Butanone-d5	6.987	46		55322	60.504	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	121.000%	
24) Chloroform-d	7.575	84		217452	30.412	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	121.640%	
26) 1,2-Dichloroethane-d4	8.234	65		113278	31.269	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	125.080%	
32) Benzene-d6	8.210	84		417303	48.710	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	194.840%#	
36) 1,2-Dichloropropane-d6	9.216	67		133172	50.946	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	203.800%#	
41) Toluene-d8	10.275	98		274008	34.748	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	139.000%#	
43) trans-1,3-Dichloroprop...	10.528	79		41024	35.490	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	141.960%#	
47) 2-Hexanone-d5	10.881	63		39417	87.509	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	175.020%#	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		52276	27.675	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	110.680%	
66) 1,2-Dichlorobenzene-d4	13.816	152		20830	22.533	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.120%	
Target Compounds							
13) Acetone	4.028	43		13716m	11.708	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
Data File : VD077734.D
Acq On : 04 Dec 2023 10:33
Operator : JC/SY
Sample : 04929-12RE
Misc : 2.84G/10ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0B63RE

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/05/2023
Supervised By :Semsettin Yesilyurt 12/05/2023

Quant Time: Dec 05 00:04:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 05 00:04:05 2023
Response via : Initial Calibration

