




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
Data File : VD077743.D
Acq On : 04 Dec 2023 16:37
Operator : JC/SY
Sample : 04929-03
Misc : 5.02G/10ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/05/2023
Supervised By :Semsettin Yesilyurt 12/05/2023

Quant Time: Dec 05 00:07:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 05 00:04:05 2023
Response via : Initial Calibration

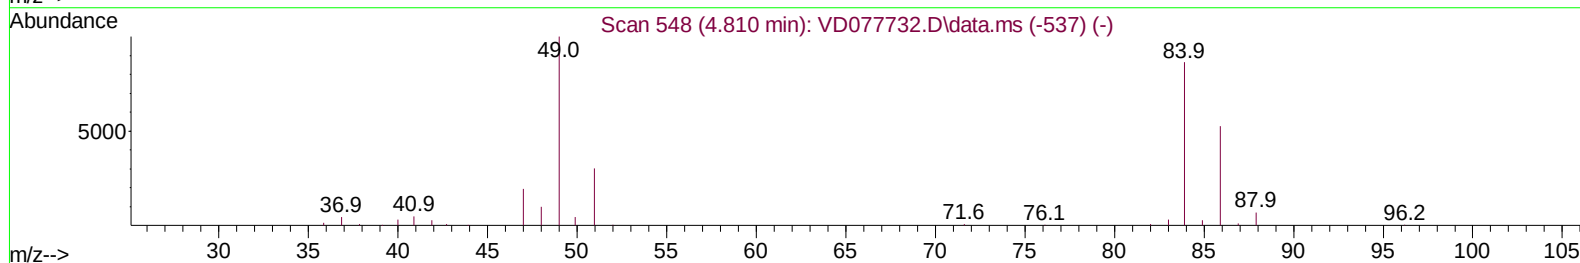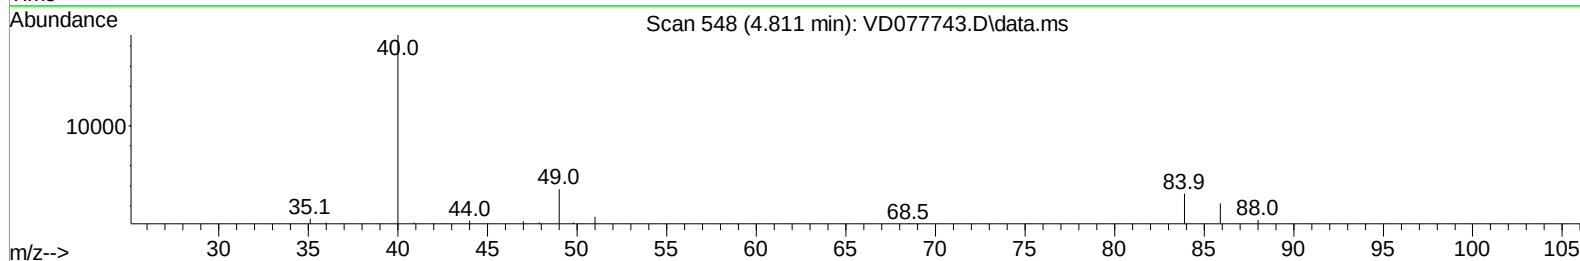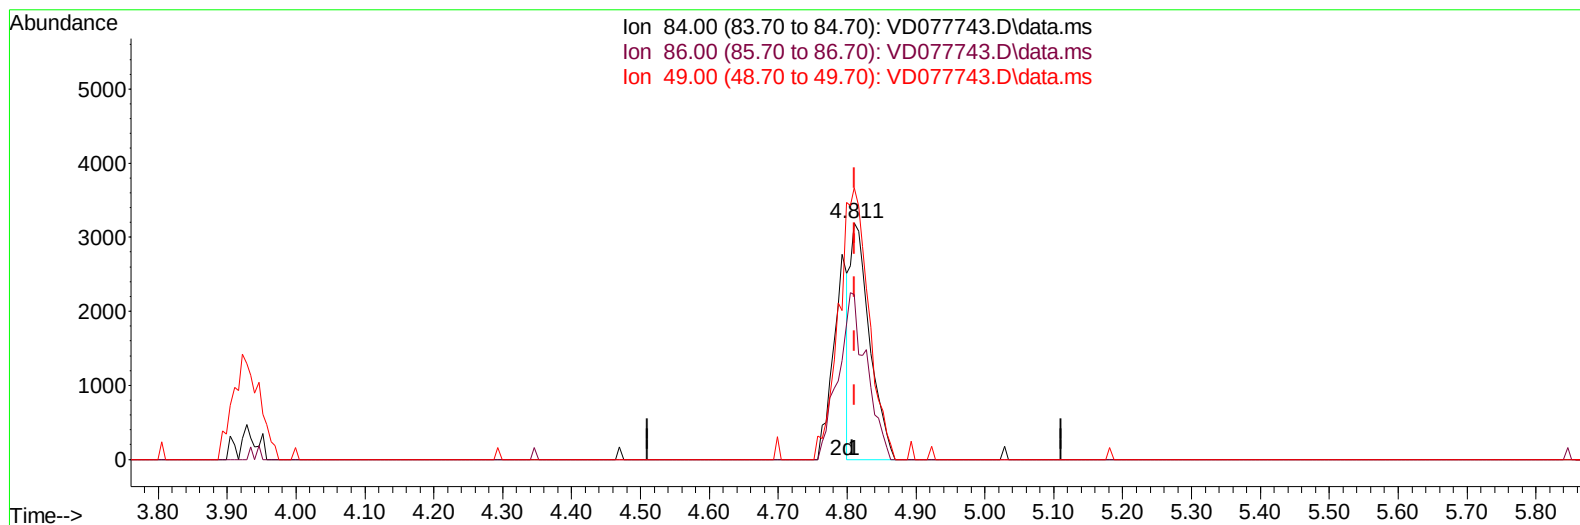

TIC: VD077743.D\data.ms

(16) Methylene chloride (T)

4.811min (+ 0.000) 1.24 ug/L

response 6351

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	57.30	69.58
49.00	118.90	114.71
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
 Data File : VD077743.D
 Acq On : 04 Dec 2023 16:37
 Operator : JC/SY
 Sample : 04929-03
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Dec 05 00:07:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 05 00:04:05 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/05/2023
 Supervised By :Semsettin Yesilyurt 12/05/2023

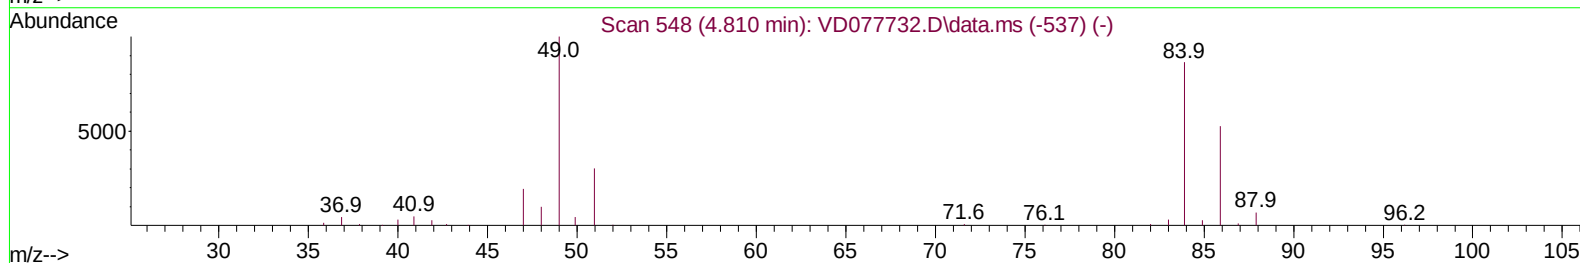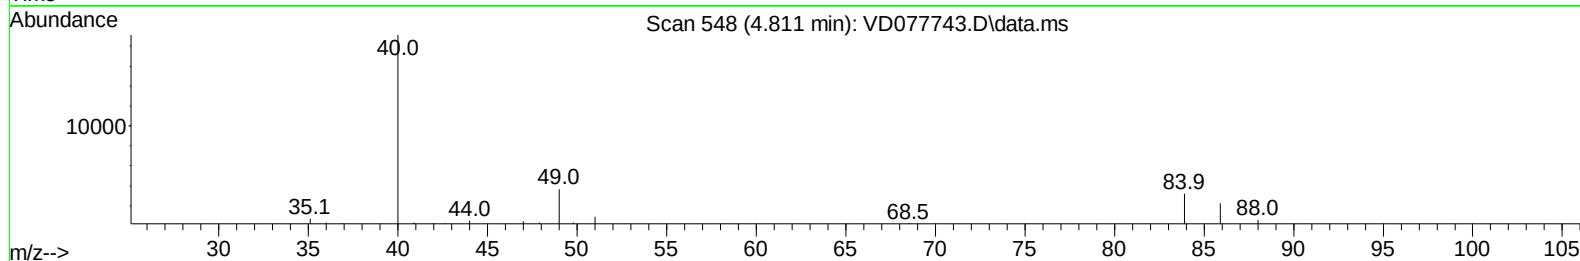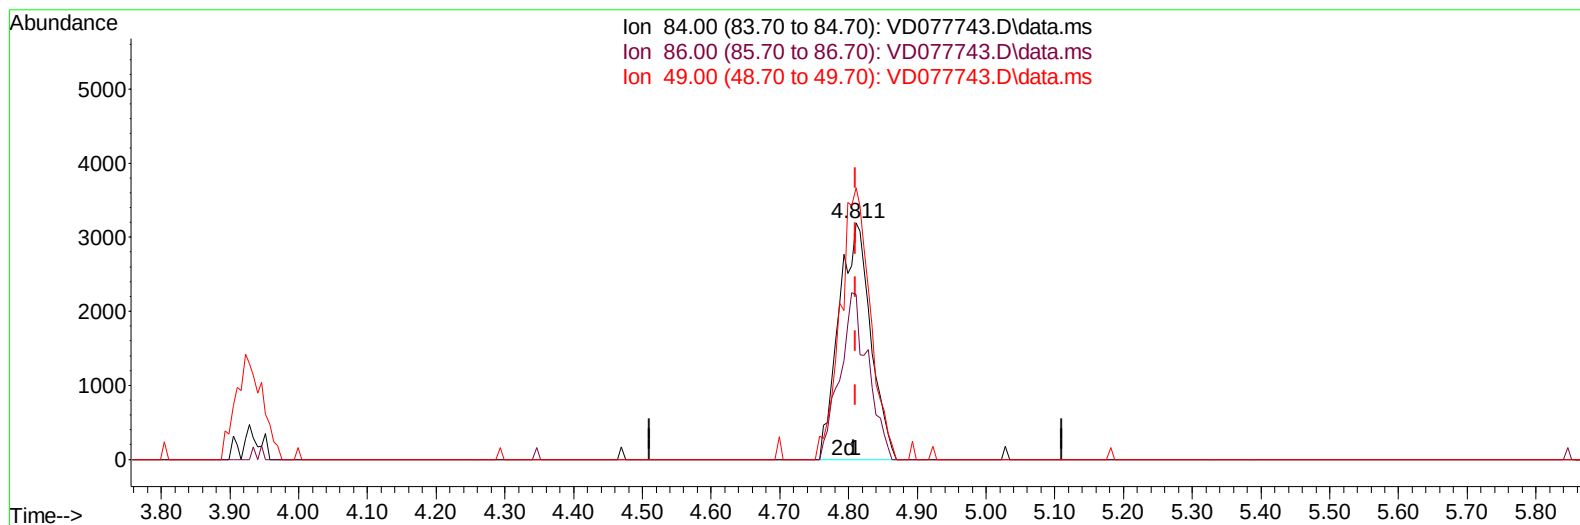

TIC: VD077743.D\data.ms

(16) Methylene chloride (T)

4.811min (+ 0.000) 1.99 ug/L m

response 10240

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	57.30	69.58
49.00	118.90	114.71
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
 Data File : VD077743.D
 Acq On : 04 Dec 2023 16:37
 Operator : JC/SY
 Sample : 04929-03
 Misc : 5.02G/10ml/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/05/2023
 Supervised By :Semsettin Yesilyurt 12/05/2023

Quant Time: Dec 05 00:07:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 05 00:04:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		289160	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		264668	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		117709	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.281	65		134649	17.075	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.320%		
7) Chloroethane-d5	2.811	69		123932	19.718	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	78.880%		
11) 1,1-Dichloroethene-d2	3.922	65		38776	18.965	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	75.840%		
21) 2-Butanone-d5	6.993	46		39901	40.036	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	80.080%		
24) Chloroform-d	7.569	84		166277	21.336	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	85.360%		
26) 1,2-Dichloroethane-d4	8.228	65		84883	21.497	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	86.000%		
32) Benzene-d6	8.205	84		350325	21.978	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	87.920%		
36) 1,2-Dichloropropane-d6	9.210	67		107739	22.152	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	88.600%		
41) Toluene-d8	10.269	98		322075	21.952	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	87.800%		
43) trans-1,3-Dichloroprop...	10.522	79		44869	20.862	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	83.440%		
47) 2-Hexanone-d5	10.875	63		34701	41.405	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	82.820%		
56) 1,1,2,2-Tetrachloroeth...	12.657	84		72188	20.540	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	82.160%		
66) 1,2-Dichlorobenzene-d4	13.816	152		96811	22.990	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	91.960%		
Target Compounds							
16) Methylene chloride	4.811	84		10240m	1.994	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120423\
Data File : VD077743.D
Acq On : 04 Dec 2023 16:37
Operator : JC/SY
Sample : 04929-03
Misc : 5.02G/10ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 12/05/2023
Supervised By :Semsettin Yesilyurt 12/05/2023

Quant Time: Dec 05 00:07:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 05 00:04:05 2023
Response via : Initial Calibration

