



Dichlorodifluoromethane

Response Ratio

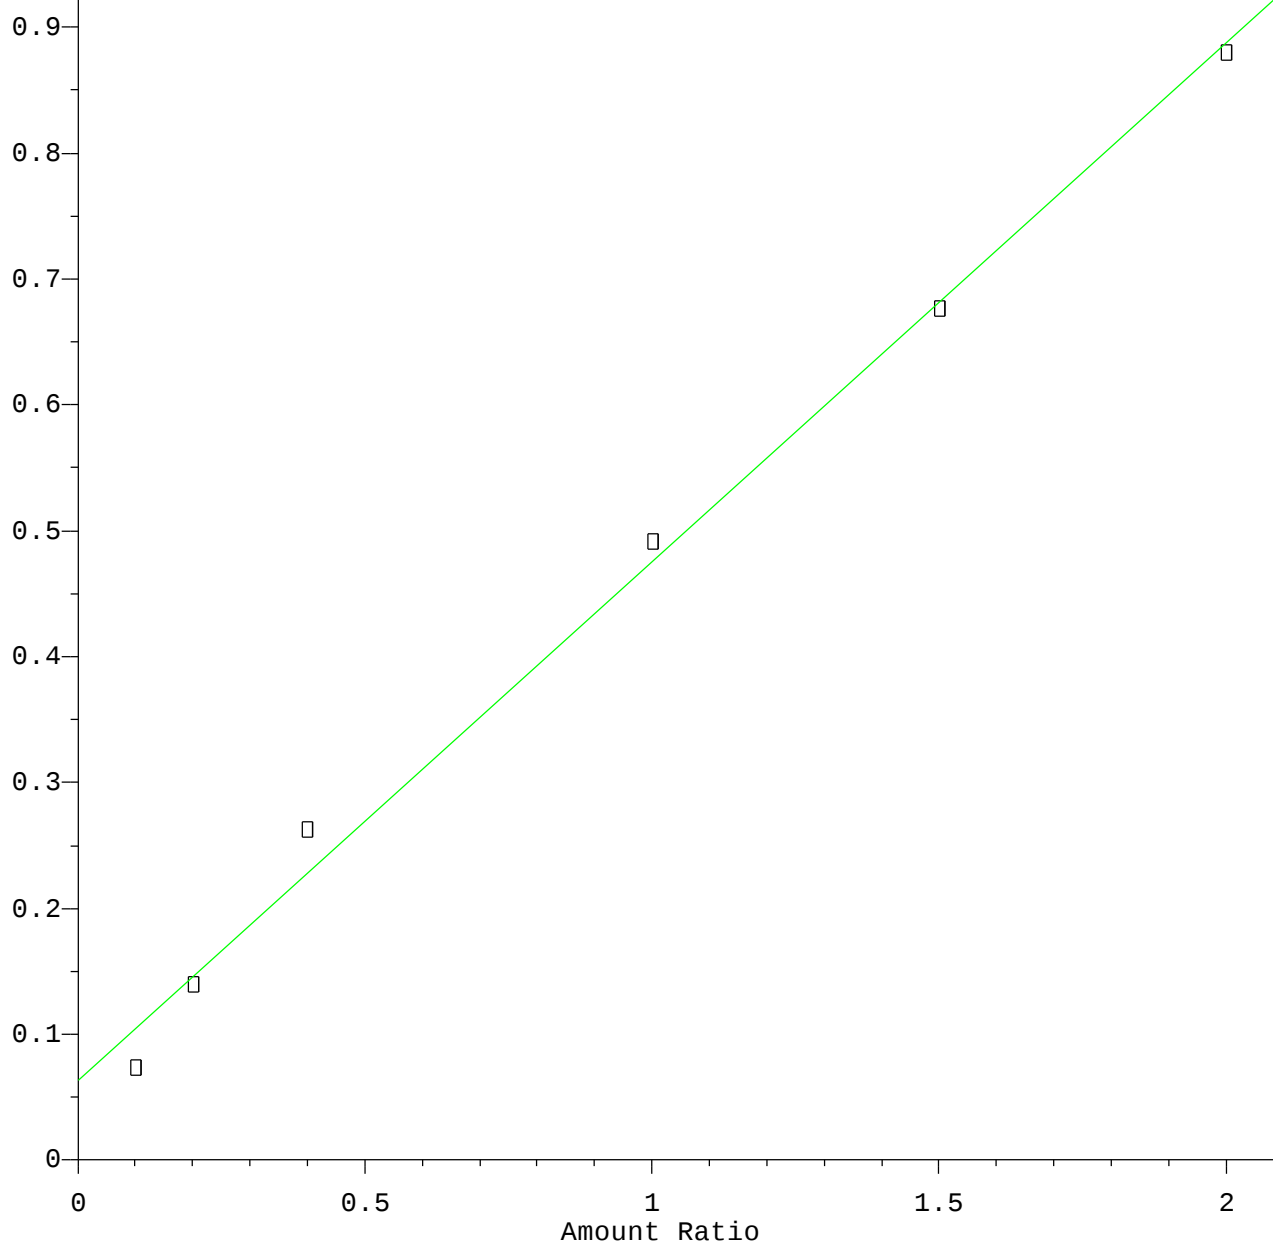


Resp Ratio = $4.13 \times 10^{-1} \times \text{Amt} + 6.29 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Calibration Table Last Updated: Thu Dec 06 01:49:20 2018

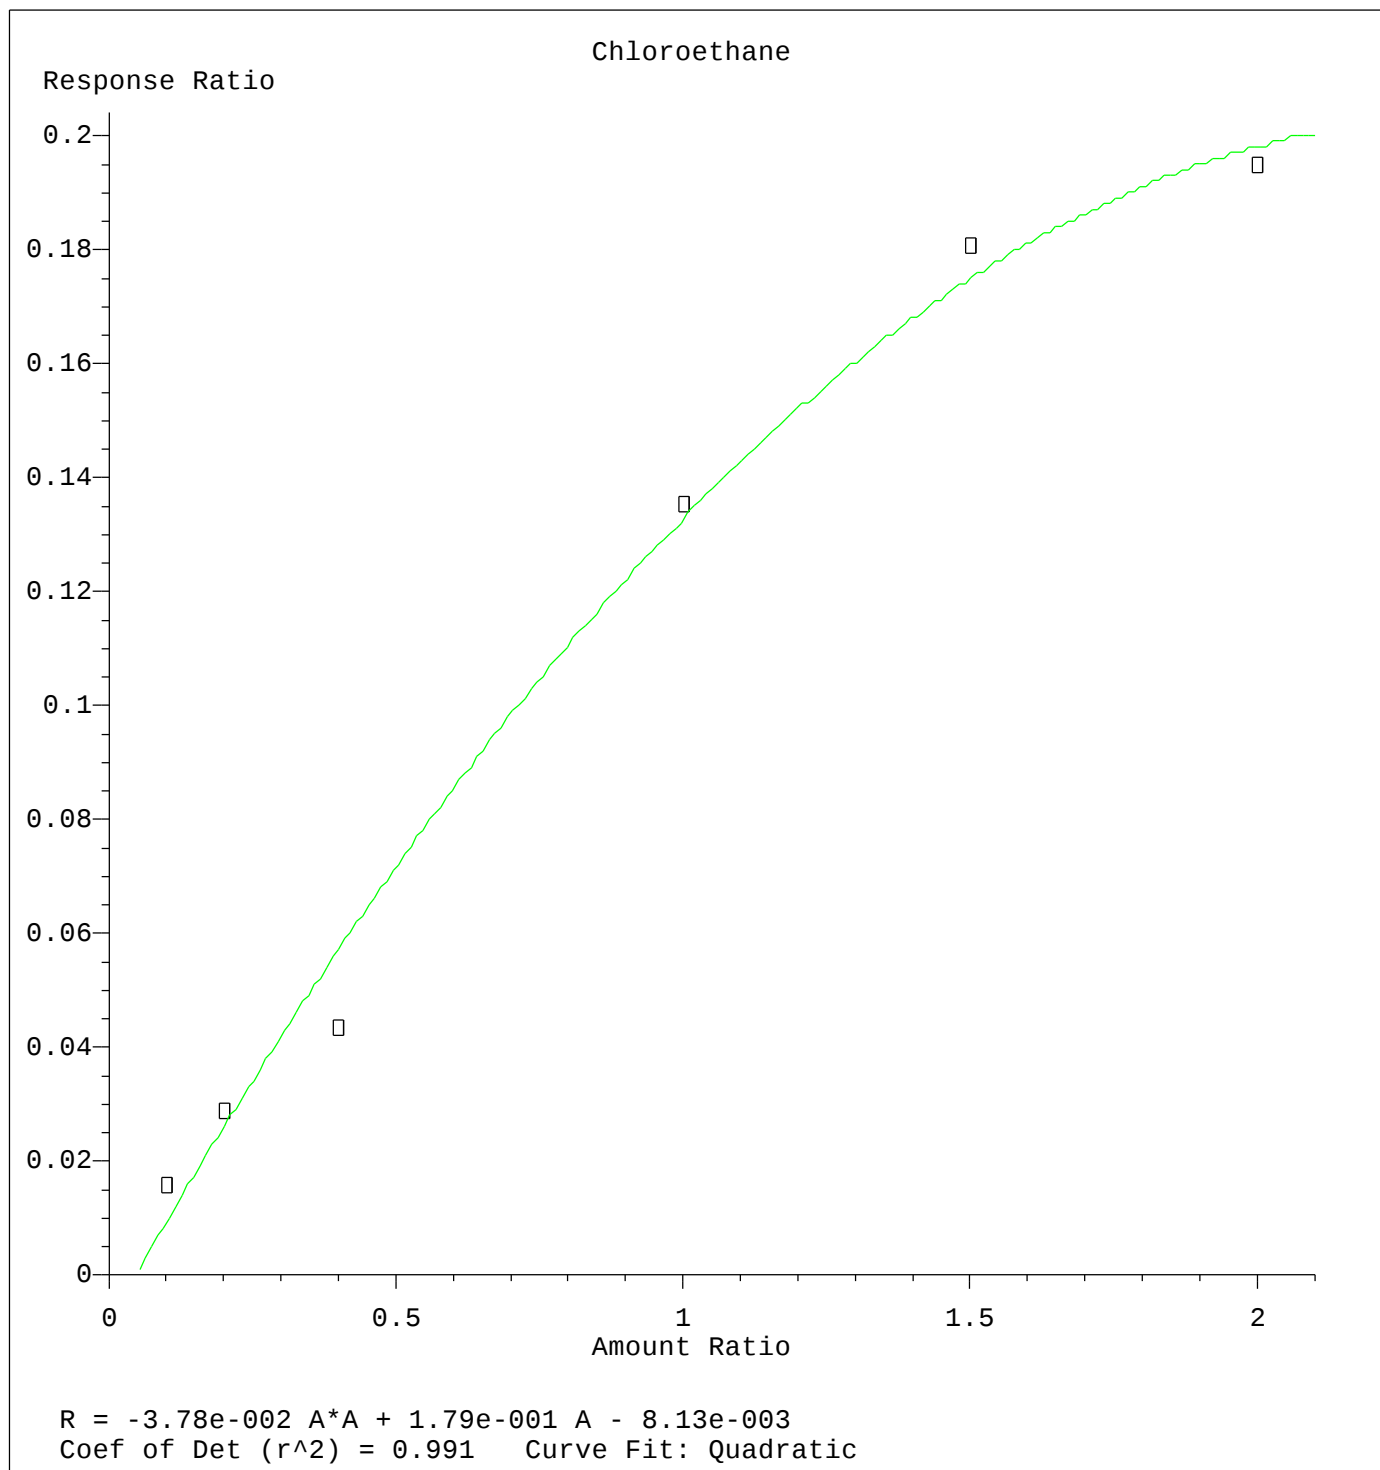


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Calibration Table Last Updated: Thu Dec 06 01:49:20 2018

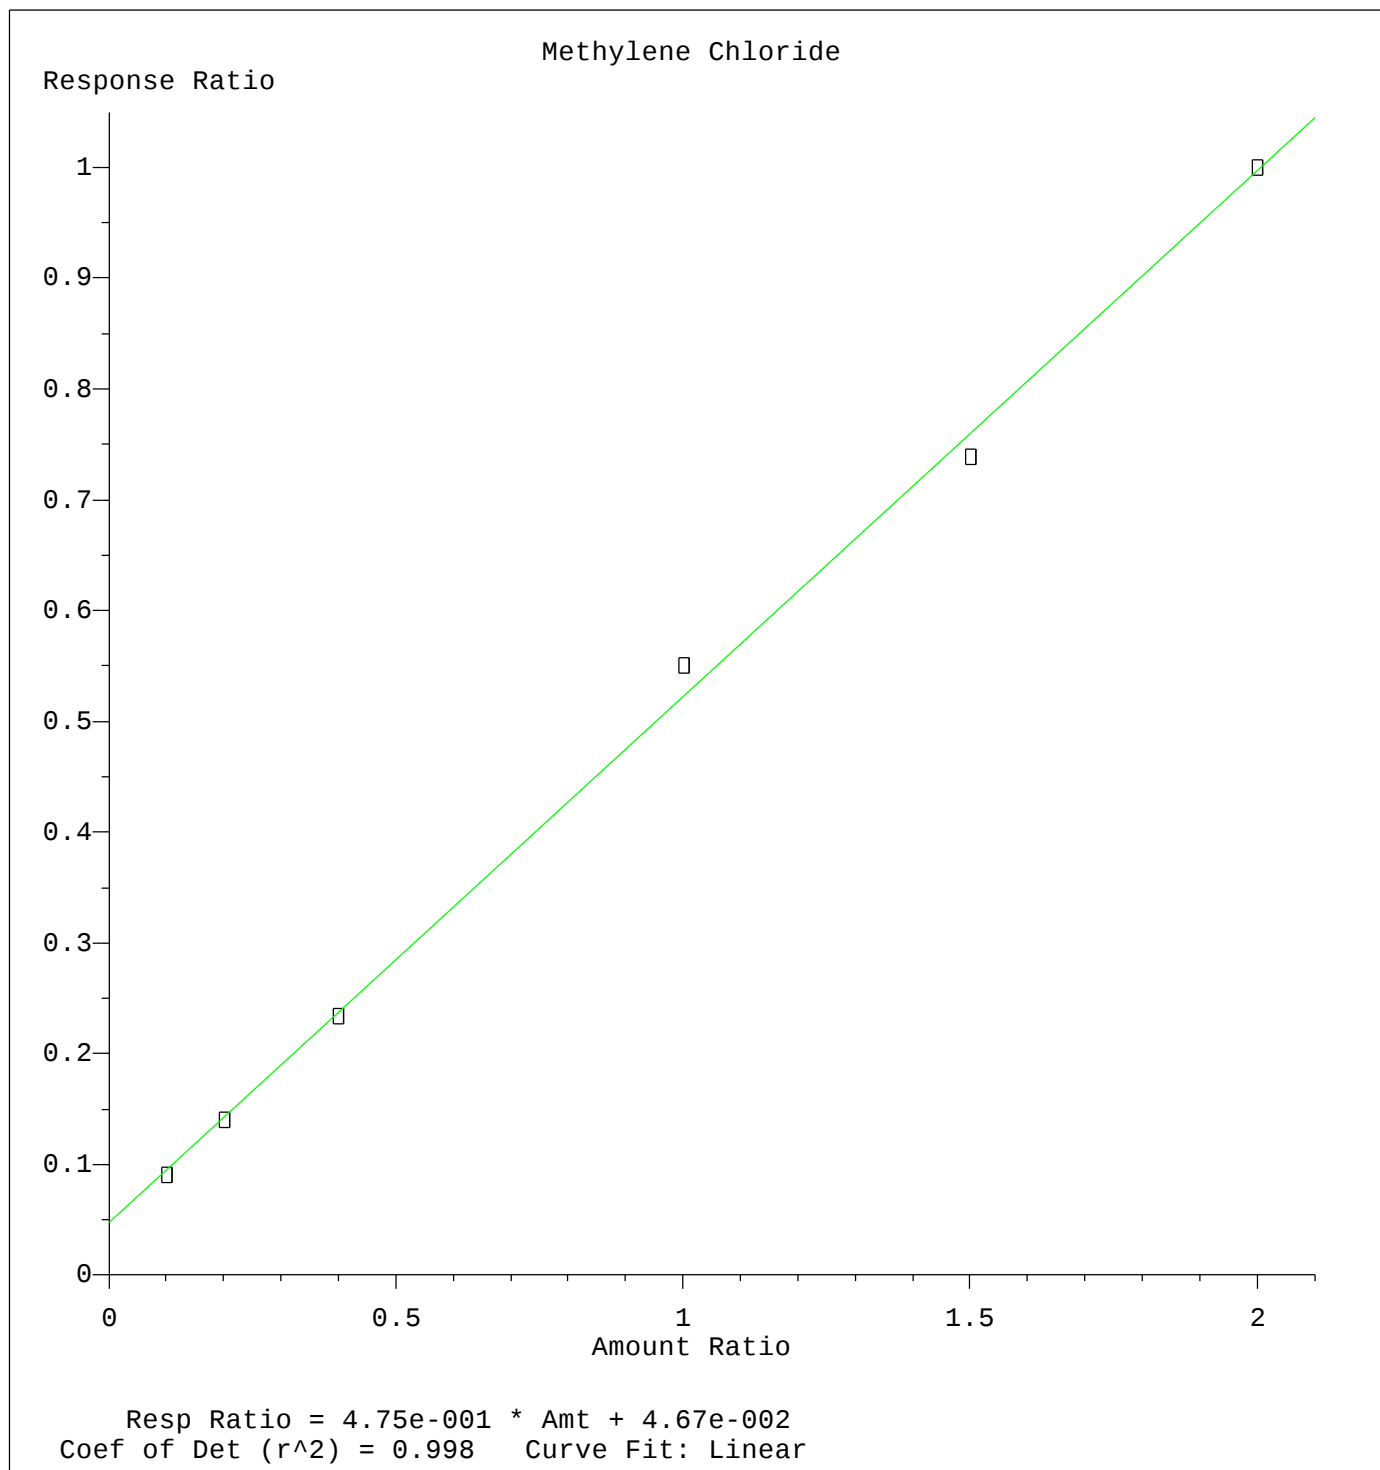

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Calibration Table Last Updated: Thu Dec 06 01:49:20 2018

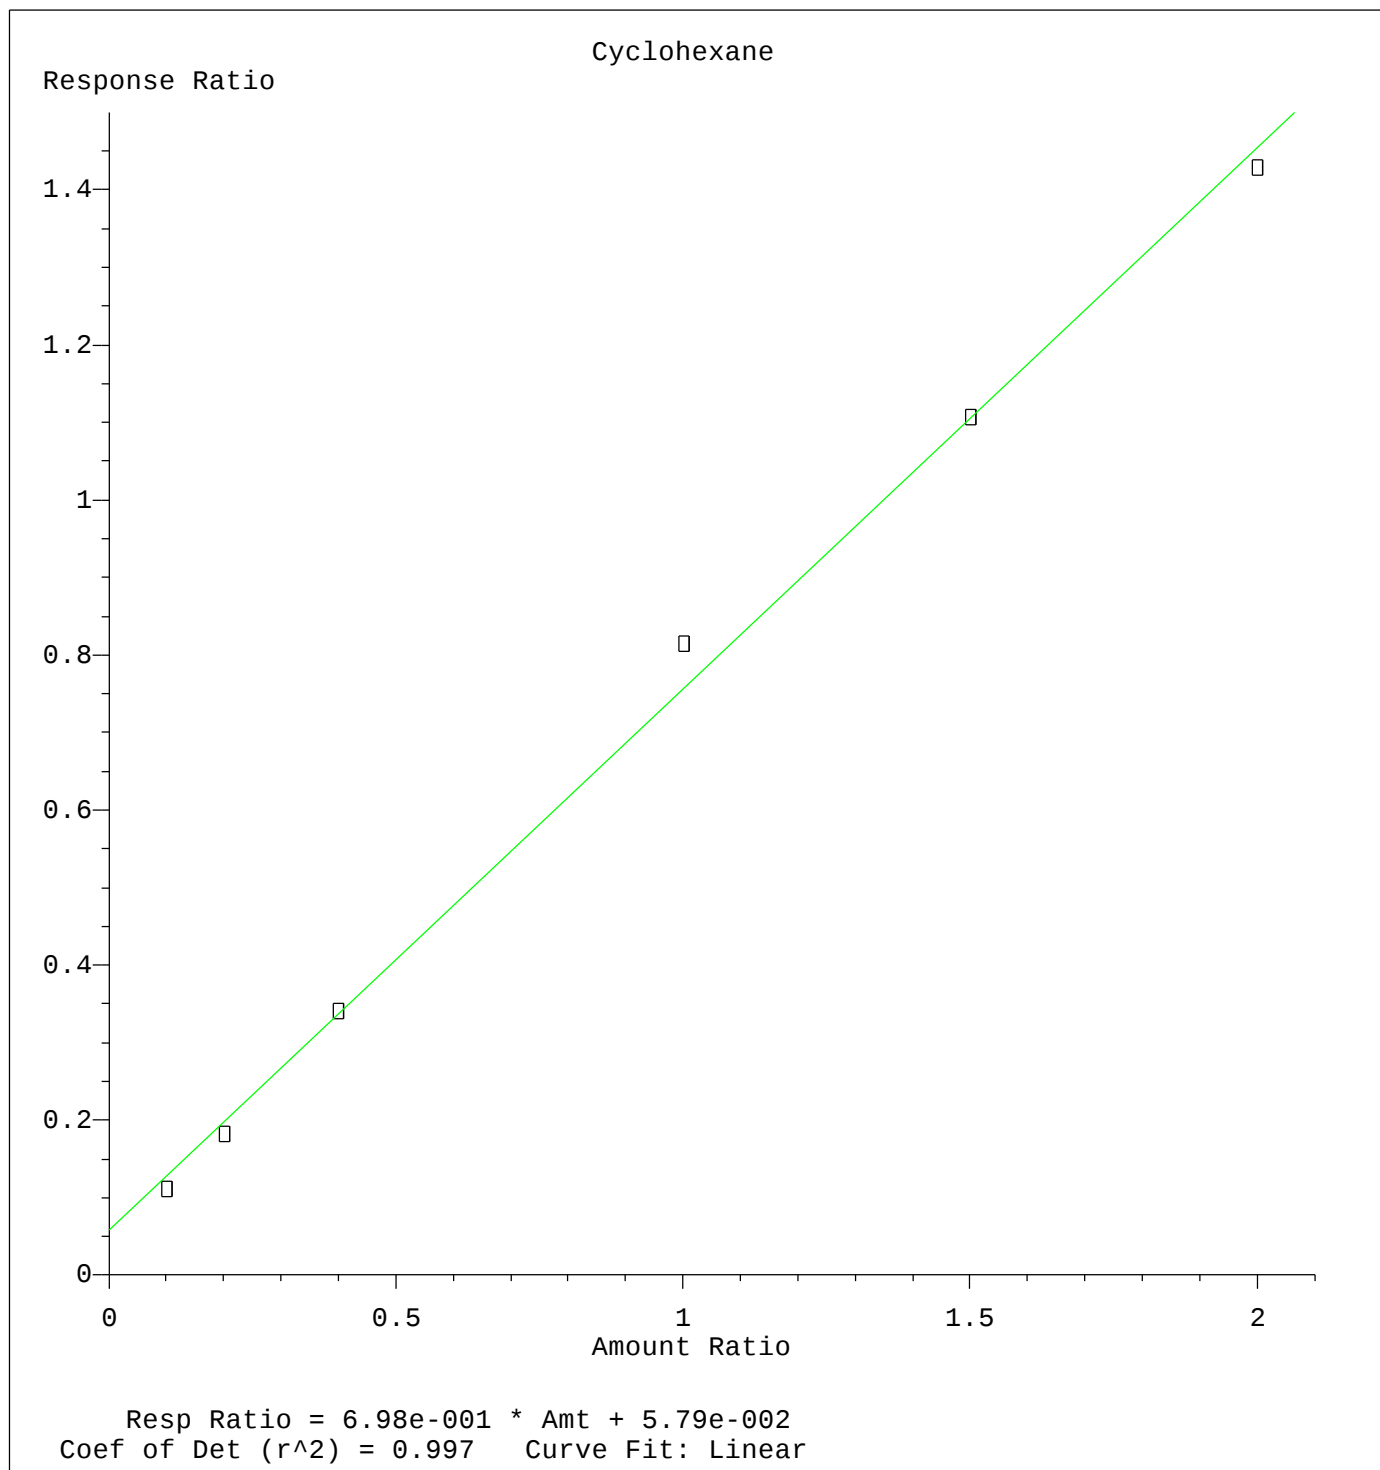

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Calibration Table Last Updated: Thu Dec 06 01:49:20 2018

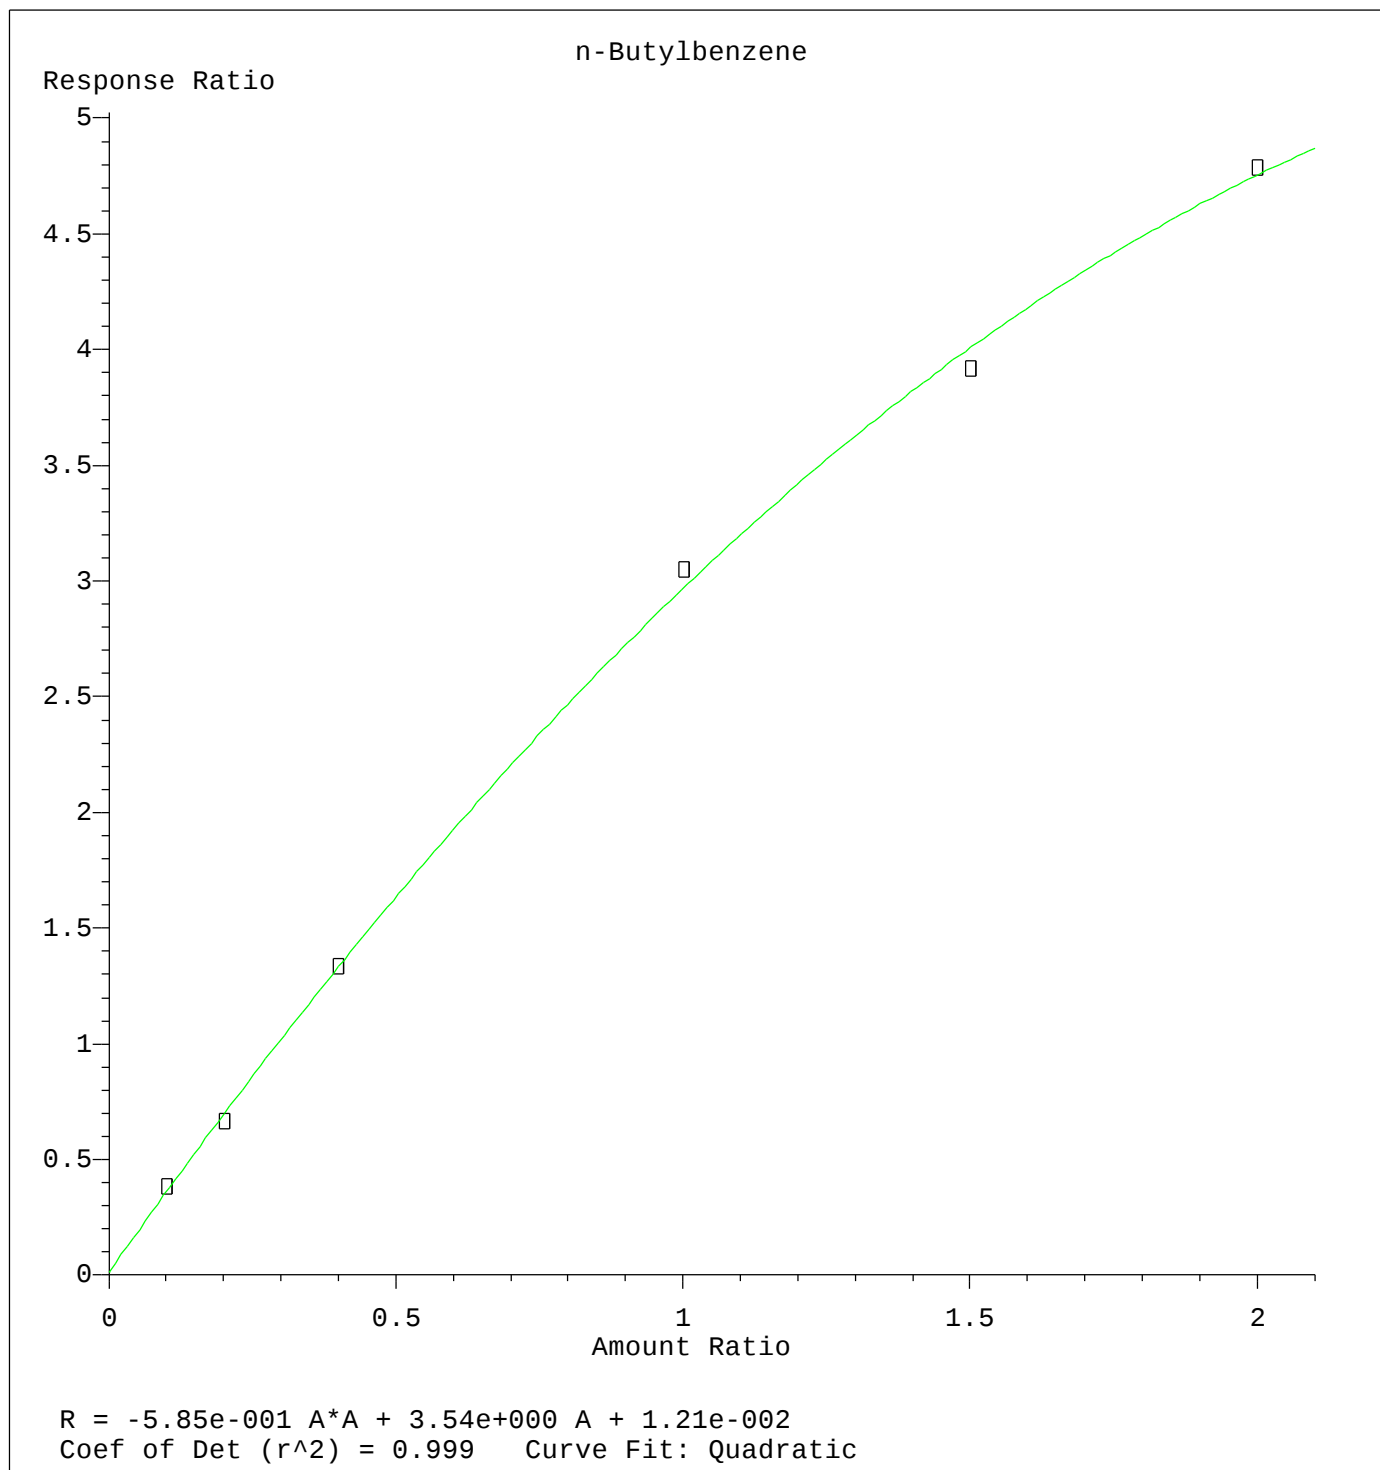

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Calibration Table Last Updated: Thu Dec 06 01:49:20 2018