


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD120518\
Data File : VD060488.D
Acq On : 5 Dec 2018 11:45
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Title : SW846 8260
Last Update : Thu Dec 06 01:49:20 2018

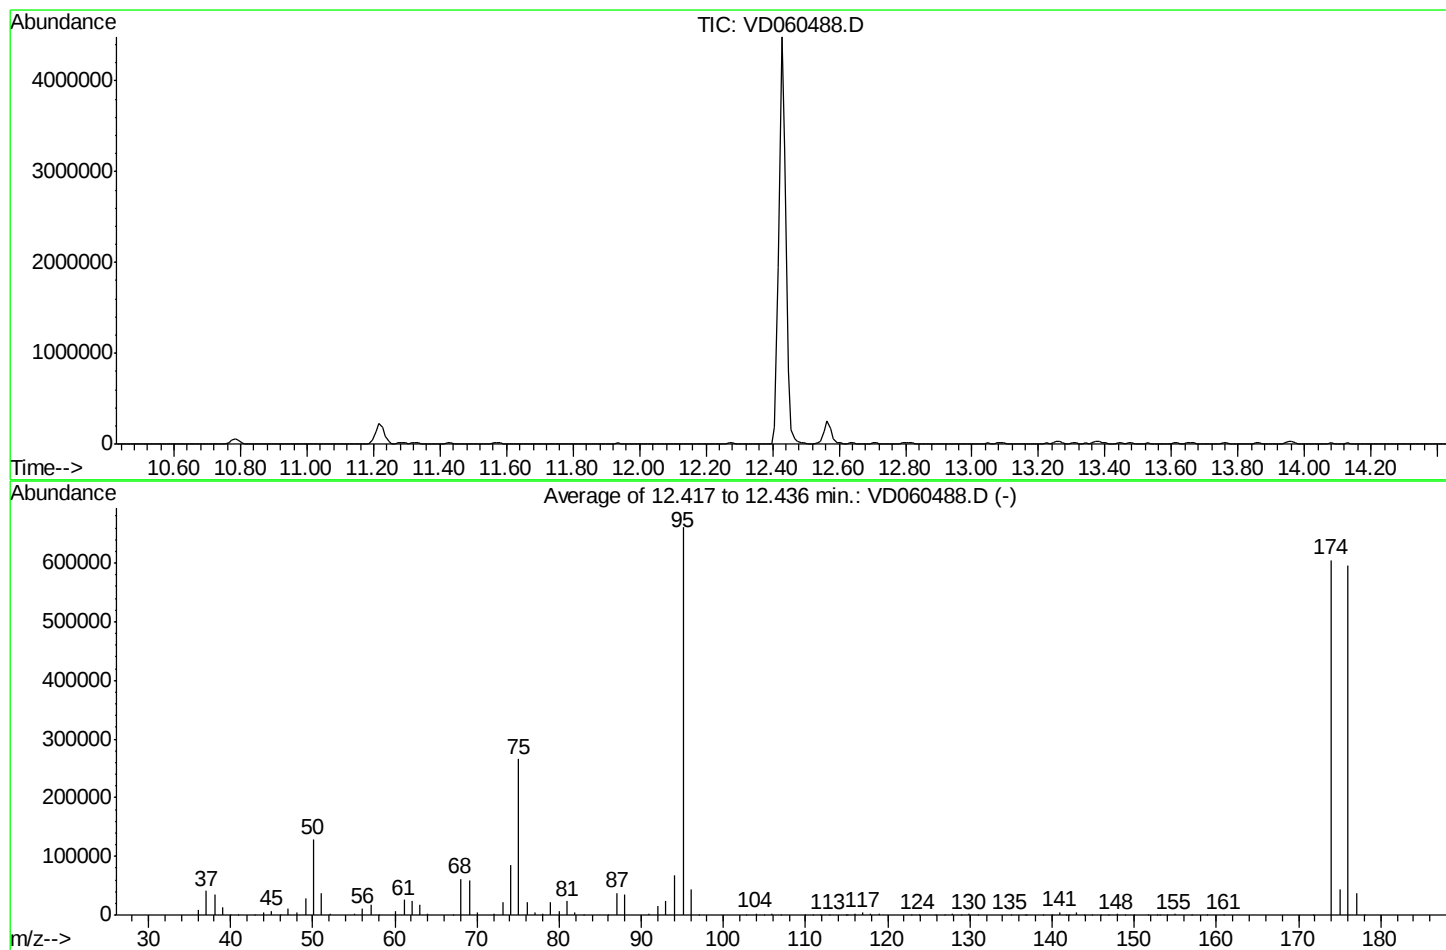

AutoFind: Scans 1107, 1108, 1109; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	127906	PASS
75	95	30	60	40.2	265813	PASS
95	95	100	100	100.0	660864	PASS
96	95	5	9	6.7	43989	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.5	604608	PASS
175	174	5	9	7.4	44693	PASS
176	174	95	101	98.7	596608	PASS
177	176	5	9	6.4	37976	PASS