
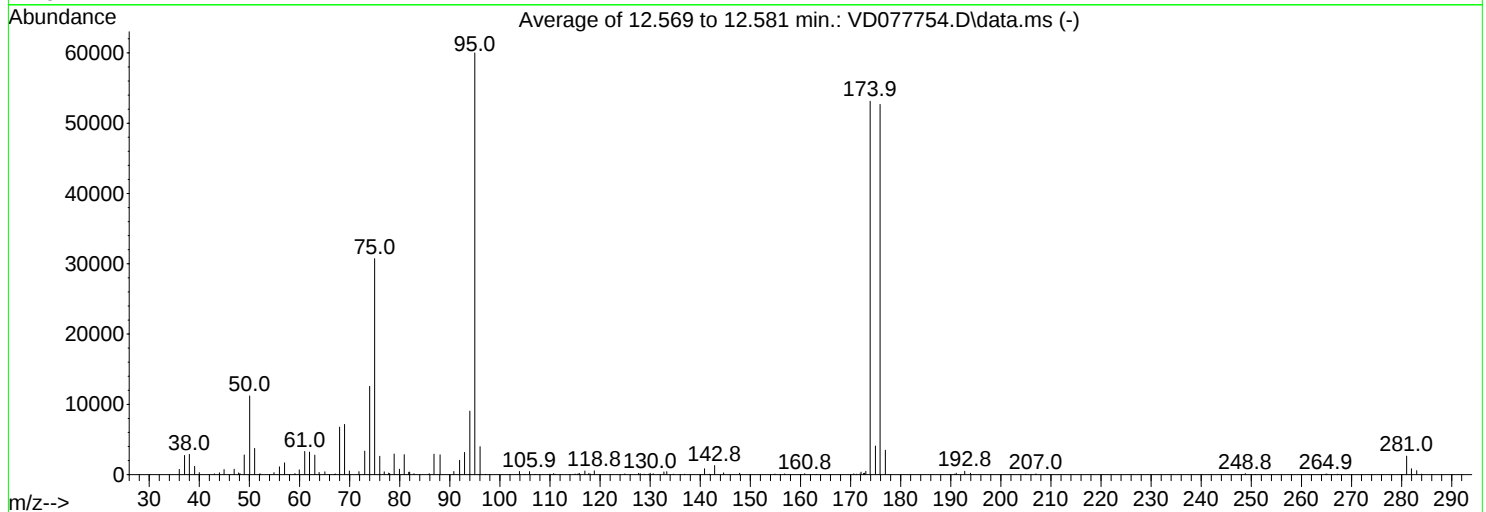


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120623\
Data File : VD077754.D
Acq On : 06 Dec 2023 09:01
Operator : JC/SY
Sample : BFB190
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB190

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Title : SFAM01.0
Last Update : Wed Dec 06 00:24:24 2023

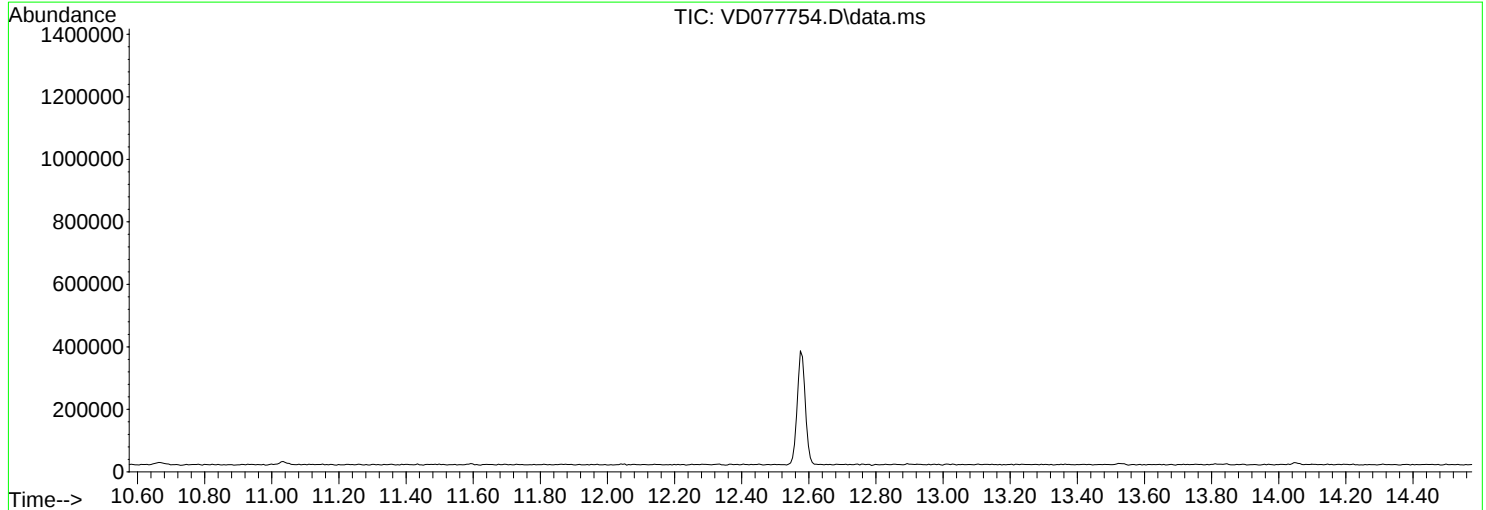

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11198	PASS
75	95	30	80	51.2	30728	PASS
95	95	100	100	100.0	60011	PASS
96	95	5	9	6.6	3977	PASS
173	174	0.00	2	0.9	488	PASS
174	95	50	120	88.5	53131	PASS
175	174	5	9	7.7	4067	PASS
176	174	95	105	99.1	52677	PASS
177	176	5	10	6.6	3489	PASS

Scan 1860 (12.528 min): VD077754.D\data.ms
BFB190

m/z	Abundance
39.20	196.0
40.00	21816.0
44.00	638.0
207.10	234.0

Instrument :
MSVOA_D
ClientSampleId :
BFB190

m/z	Abundance
36.10	697.0
37.00	2646.0
38.00	2494.0
39.10	1409.0
40.00	22600.0
44.00	870.0
44.90	584.0
47.00	658.0
47.80	482.0
48.90	2303.0
50.00	10021.0
51.00	3182.0
52.00	310.0
54.90	241.0
56.00	784.0
57.10	1590.0
59.20	181.0
60.00	561.0
61.00	3146.0
62.00	2774.0
63.00	2207.0
63.90	252.0
65.10	359.0
68.00	6070.0
69.00	6214.0
69.90	582.0
71.90	413.0
73.00	3291.0
74.00	11074.0
75.00	27640.0
76.00	2589.0
77.00	313.0
77.80	190.0
78.90	2381.0
79.90	637.0
80.90	2388.0
81.80	1020.0
86.00	191.0
86.90	2140.0
88.00	1975.0
90.90	368.0
92.00	1478.0
93.00	2614.0
94.00	7025.0
95.00	51048.0
96.00	3119.0
104.00	266.0
106.00	438.0
110.70	176.0
116.00	171.0
117.00	605.0
117.70	211.0
118.90	432.0
127.70	231.0
129.70	198.0
130.70	214.0
132.70	196.0
133.40	372.0
134.70	183.0
140.90	754.0
142.90	984.0
144.60	218.0
147.80	225.0
156.80	202.0
171.90	357.0
172.60	582.0
173.90	41752.0
174.90	3366.0
175.90	42272.0
176.90	2615.0
191.10	316.0
192.80	271.0
207.00	177.0
248.80	252.0
250.80	164.0
281.00	1609.0
282.00	549.0
283.10	523.0

Instrument :
MSVOA_D
ClientSampleId :
BFB190

m/z	Abundance
35.90	744.0
37.10	2726.0
38.00	3104.0
39.00	1817.0
40.00	21048.0
43.10	175.0
44.10	1115.0
45.00	861.0
47.00	1114.0
48.10	488.0
49.00	3294.0
50.00	13034.0
51.10	4000.0
52.20	260.0
54.90	358.0
56.00	1349.0
57.00	1994.0
59.00	283.0
60.00	936.0
61.10	3871.0
62.00	3715.0
63.00	3862.0
63.90	510.0
65.00	512.0
67.00	244.0
68.00	7486.0
69.00	8234.0
69.90	468.0
71.90	491.0
73.00	3775.0
74.00	12598.0
75.00	35384.0
76.00	3023.0
76.90	236.0
77.80	514.0
78.90	3101.0
80.00	812.0
80.90	3107.0
82.00	494.0
82.90	169.0
86.90	3338.0
88.10	3767.0
90.70	563.0
91.90	2624.0
93.00	3949.0
94.00	10063.0
95.00	65744.0
96.10	4451.0
97.10	156.0
103.80	449.0
105.90	359.0
107.00	166.0
110.00	174.0
110.70	261.0
115.00	262.0
115.80	376.0
116.90	493.0
118.00	274.0
118.80	610.0
124.90	180.0
127.70	353.0
130.10	300.0
130.50	203.0
132.80	442.0
133.20	484.0
136.90	232.0
140.80	936.0
142.80	1463.0
144.70	283.0
147.80	208.0
154.90	253.0
160.90	159.0
163.10	157.0
170.70	181.0
171.20	204.0
172.10	581.0
172.80	605.0
173.00	769.0
173.90	58520.0
174.90	4366.0
175.90	57032.0
177.00	4092.0
191.10	295.0
192.80	547.0
193.90	297.0
205.00	180.0
206.80	307.0
264.90	292.0
267.20	194.0
281.00	2705.0
281.80	709.0
283.00	398.0

Instrument :
MSVOA_D
ClientSampleId :
BFB190

m/z	Abundance
36.00	818.0
37.10	2848.0
38.00	3050.0
39.10	920.0
40.00	22680.0
42.90	194.0
44.00	750.0
44.90	778.0
46.80	536.0
47.90	274.0
49.00	2825.0
50.10	10540.0
51.00	4052.0
54.90	283.0
56.00	1237.0
56.90	1475.0
59.90	556.0
61.00	2858.0
62.00	3146.0
63.10	2238.0
63.80	216.0
65.00	330.0
67.20	252.0
68.00	6717.0
69.00	6998.0
70.00	525.0
71.80	405.0
73.00	2993.0
74.00	14001.0
75.00	29160.0
76.00	2250.0
76.90	688.0
78.00	454.0
78.90	3350.0
80.00	872.0
80.90	3046.0
82.00	569.0
82.80	245.0
85.80	190.0
86.80	3279.0
88.00	2723.0
90.80	419.0
91.90	2018.0
92.90	2947.0
94.00	10032.0
95.00	63240.0
96.00	4362.0
104.00	644.0
105.00	165.0
105.80	498.0
111.00	218.0
115.60	335.0
116.90	486.0
117.80	308.0
118.80	574.0
125.00	169.0
128.00	397.0
128.80	191.0
129.90	334.0
132.80	506.0
133.30	412.0
140.80	867.0
141.90	195.0
142.90	1423.0
144.60	221.0
147.90	159.0
156.90	158.0
160.80	229.0
170.60	175.0
172.10	520.0
173.10	694.0
173.90	59120.0
175.00	4469.0
175.90	58728.0
176.90	3760.0
190.80	235.0
192.80	592.0
194.00	291.0
207.00	536.0
248.80	226.0
265.10	266.0
281.00	3592.0
282.00	1260.0
282.90	787.0
284.00	206.0

Instrument :
MSVOA_D
ClientSampleId :
BFB190