

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120723\
 Data File : VD077775.D
 Acq On : 07 Dec 2023 12:48
 Operator : JC/SY
 Sample : VIBLK131
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK131

Quant Time: Dec 08 00:33:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 06 00:24:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	272093	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	249489	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	109634	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.281	65	131563	17.731	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.920%
7) Chloroethane-d5	2.811	69	120361	20.351	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	3.934	65	36077	18.752	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.000%
21) 2-Butanone-d5	6.993	46	44192	47.123	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.240%
24) Chloroform-d	7.575	84	174198	23.754	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	8.234	65	86505	23.282	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.120%
32) Benzene-d6	8.210	84	353434	23.522	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.080%
36) 1,2-Dichloropropane-d6	9.216	67	107381	23.422	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	10.275	98	320738	23.191	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.760%
43) trans-1,3-Dichloroprop...	10.528	79	45359	22.373	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.480%
47) 2-Hexanone-d5	10.881	63	37596	47.589	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.180%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	79540	24.009	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.040%
66) 1,2-Dichlorobenzene-d4	13.816	152	103194	26.311	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.240%
Target Compounds						Qvalue
51) Chlorobenzene	11.616	112	4577	0.428	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120723\
Data File : VD077775.D
Acq On : 07 Dec 2023 12:48
Operator : JC/SY
Sample : VIBLK131
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK131


Quant Time: Dec 08 00:33:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 06 00:24:24 2023
Response via : Initial Calibration

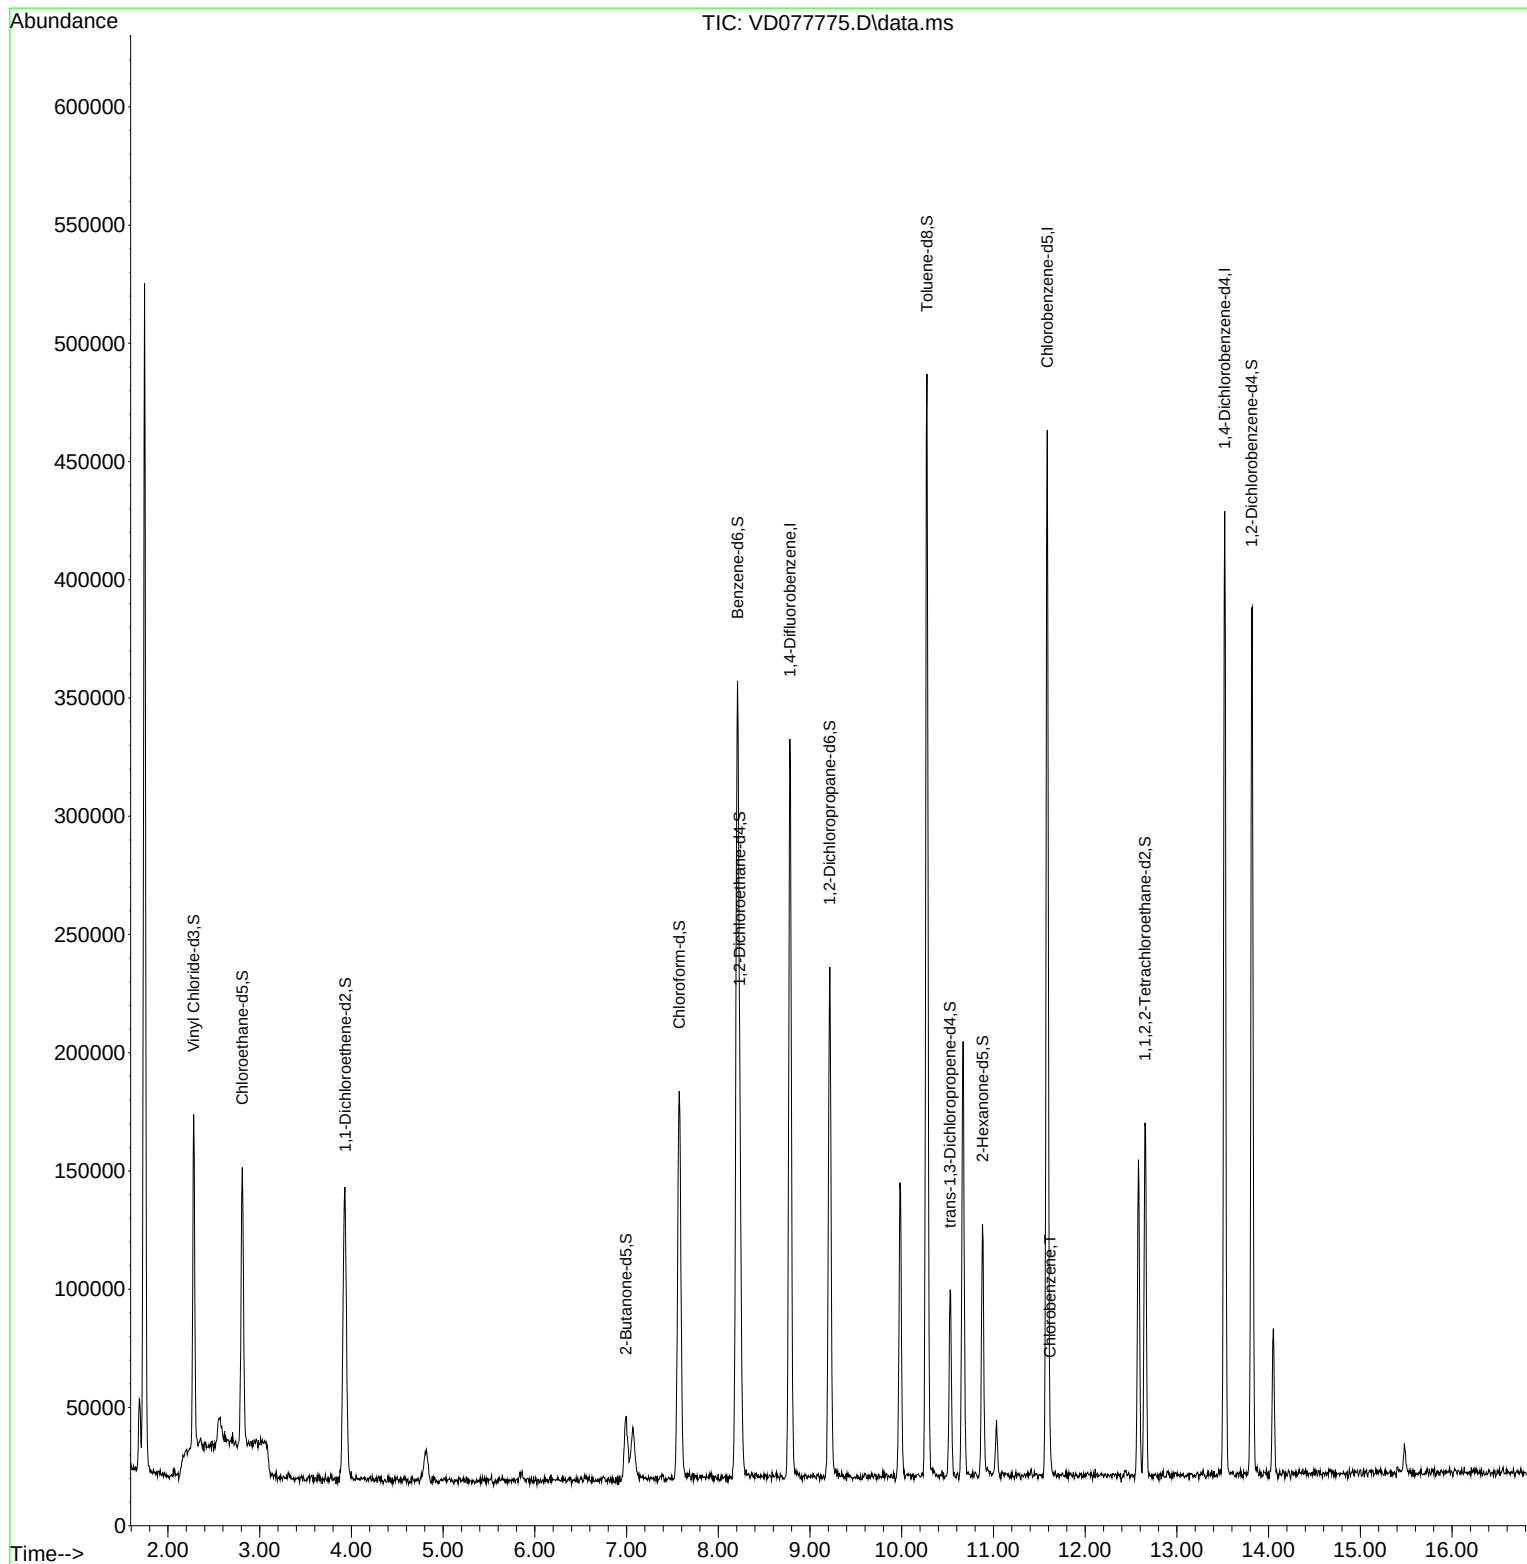

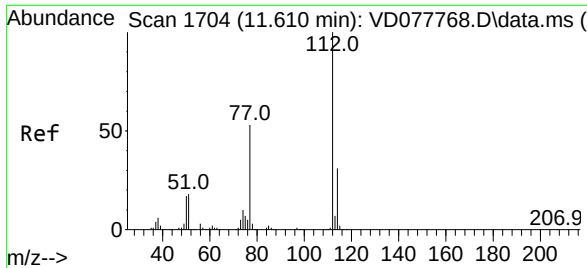

#51
Chlorobenzene
Concen: 0.428 ug/L
RT: 11.616 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD077775.D
Acq: 07 Dec 2023 12:48

Instrument :
MSVOA_D
ClientSampleId :
VIBLK131

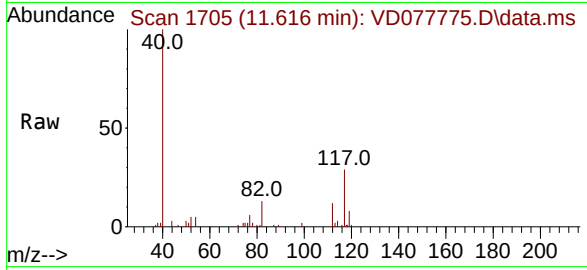

Tgt Ion:	112	Resp:	4577
Ion	Ratio	Lower	Upper
112	100		
114	25.5	22.5	41.9
77	51.8	46.4	69.6

