

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120723\
 Data File : VD077778.D
 Acq On : 07 Dec 2023 16:11
 Operator : JC/SY
 Sample : VIBLK133
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VIBLK133

Quant Time: Dec 08 00:34:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 06 00:24:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	341389	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	321759	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	147932	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.281	65	140167	15.056	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.240%		
7) Chloroethane-d5	2.811	69	129608	17.466	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.880%		
11) 1,1-Dichloroethene-d2	3.922	65	40466	16.764	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.040%		
21) 2-Butanone-d5	6.993	46	48615	41.317	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.640%		
24) Chloroform-d	7.569	84	182409	19.825	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	79.280%		
26) 1,2-Dichloroethane-d4	8.228	65	90402	19.392	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.560%		
32) Benzene-d6	8.204	84	368414	19.012	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.040%		
36) 1,2-Dichloropropane-d6	9.210	67	112113	18.961	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	75.840%		
41) Toluene-d8	10.269	98	340157	19.071	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.280%		
43) trans-1,3-Dichloroprop...	10.528	79	47777	18.273	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	73.080%		
47) 2-Hexanone-d5	10.881	63	40042	39.301	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.600%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	81428	19.058	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	76.240%		
66) 1,2-Dichlorobenzene-d4	13.816	152	106932	20.206	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.840%		
Target Compounds						Qvalue
16) Methylene chloride	4.810	84	8274	1.365	ug/L	95
33) Benzene	8.251	78	20611	0.984	ug/L	100
51) Chlorobenzene	11.610	112	234310	16.987	ug/L	98
64) 1,3-Dichlorobenzene	13.457	146	11105	1.163	ug/L	84
65) 1,4-Dichlorobenzene	13.539	146	126504	12.767	ug/L	96
67) 1,2-Dichlorobenzene	13.834	146	9987	1.162	ug/L	96
70) 1,2,4-trichlorobenzene	15.104	180	66380	12.025	ug/L	97
72) 1,2,3-Trichlorobenzene	15.528	180	29057	6.005	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120723\
Data File : VD077778.D
Acq On : 07 Dec 2023 16:11
Operator : JC/SY
Sample : VIBLK133
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VIBLK133

Quant Time: Dec 08 00:34:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 06 00:24:24 2023
Response via : Initial Calibration

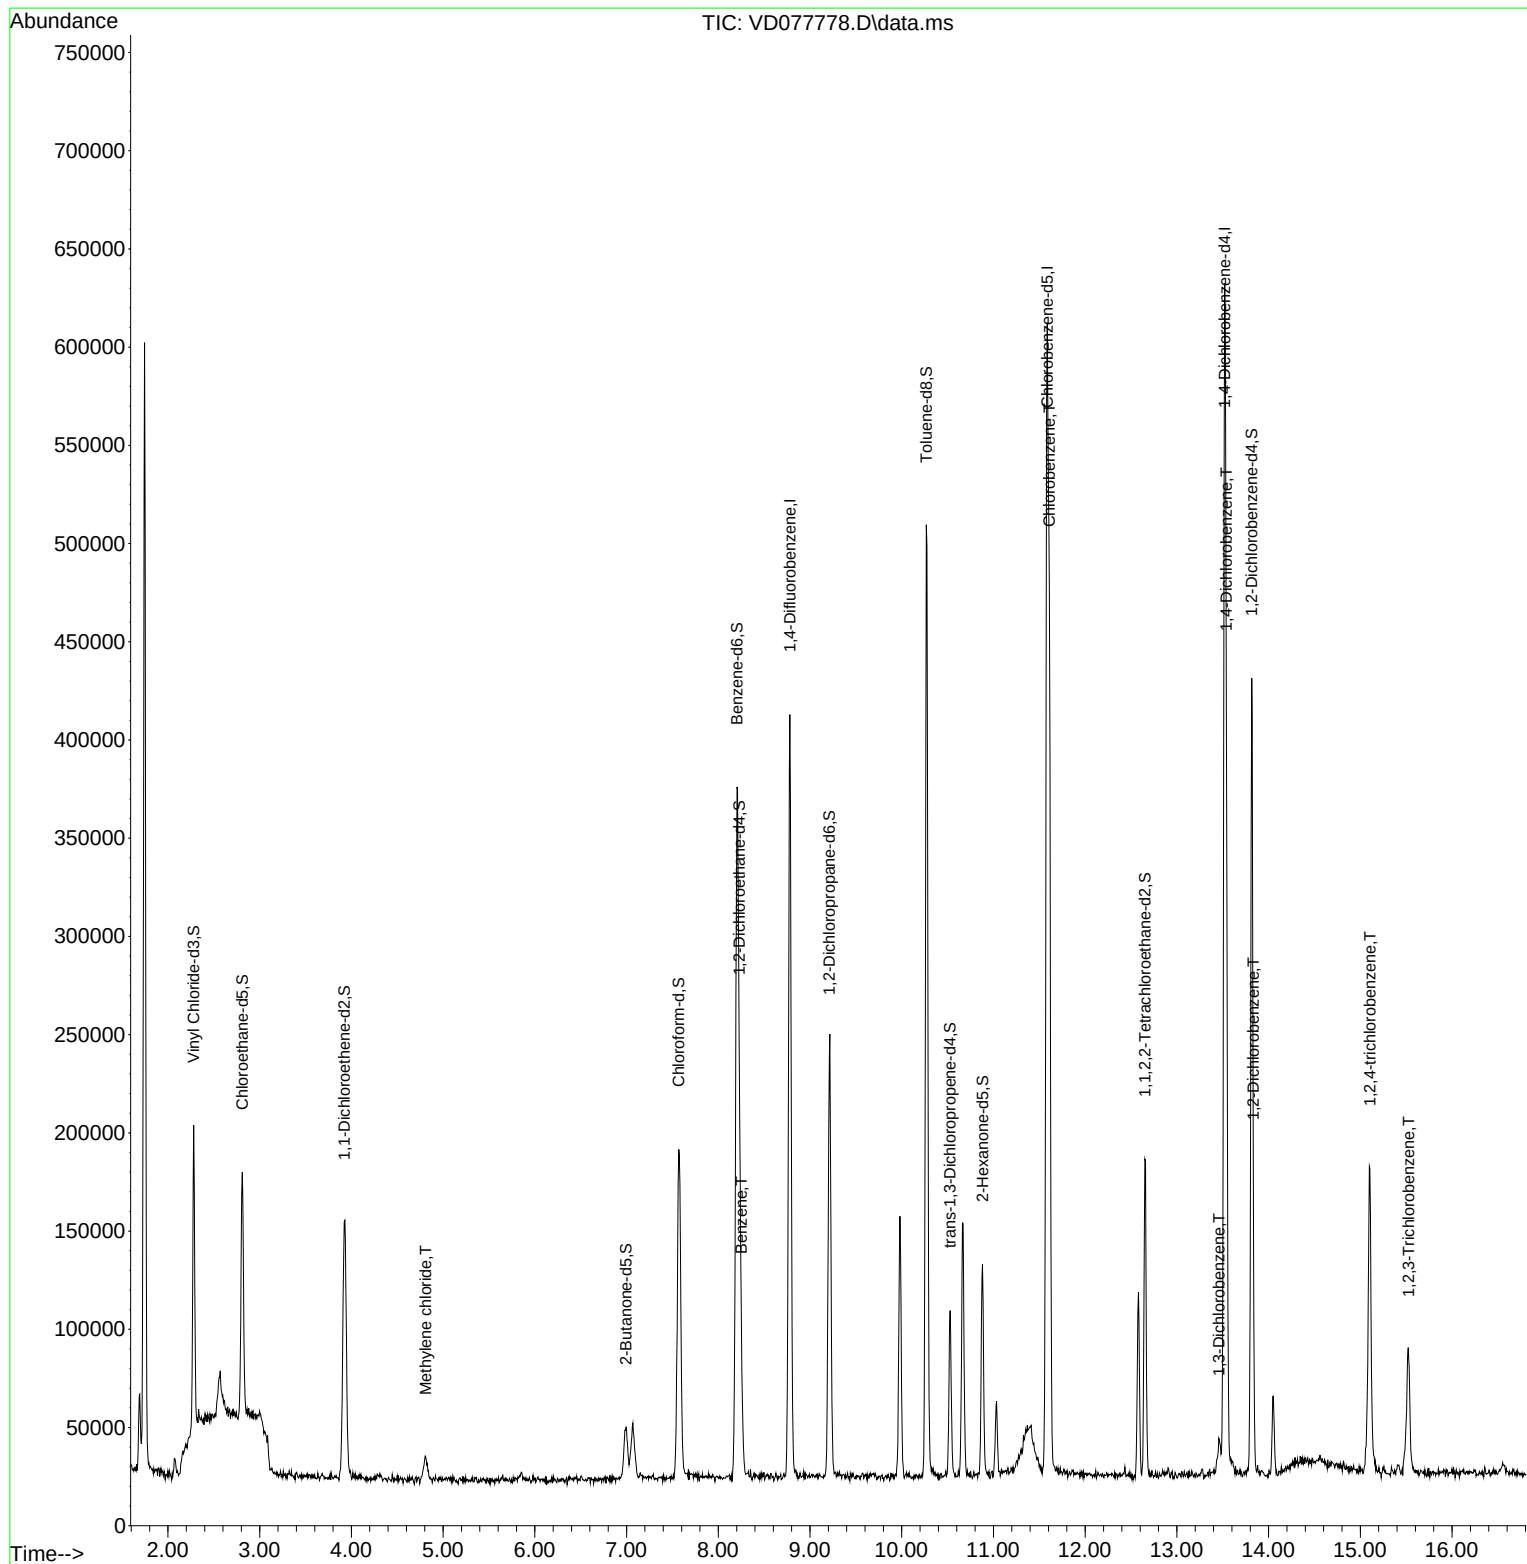




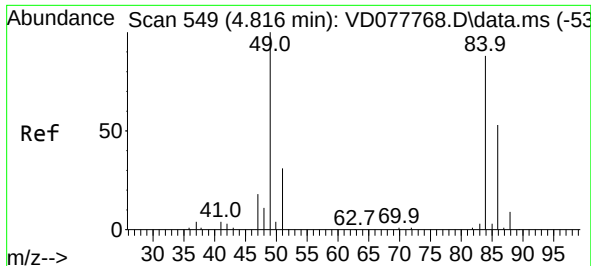


#16
Methylene chloride
Concen: 1.365 ug/L
RT: 4.810 min Scan# 549
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Instrument :
MSVOA_D
ClientSampleId :
VIBLK133




Tgt Ion: 84 Resp: 8274


Ion	Ratio	Lower	Upper
84	100		
86	50.1	40.1	74.5
49	122.3	83.2	154.6

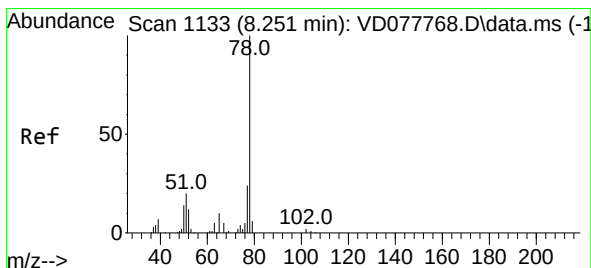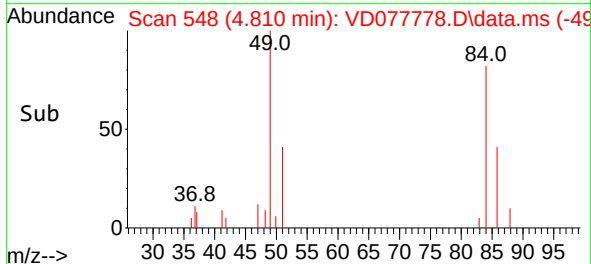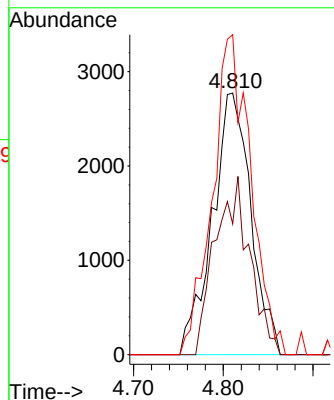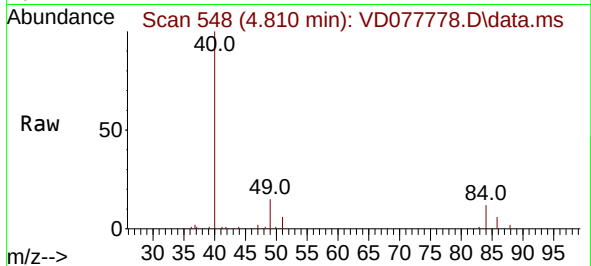

#33
Benzene
Concen: 0.984 ug/L
RT: 8.251 min Scan# 1133
Delta R.T. -0.006 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Tgt Ion: 78 Resp: 20611


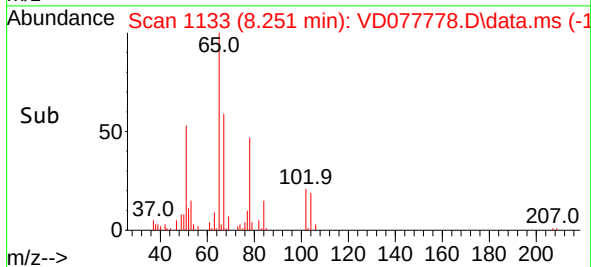
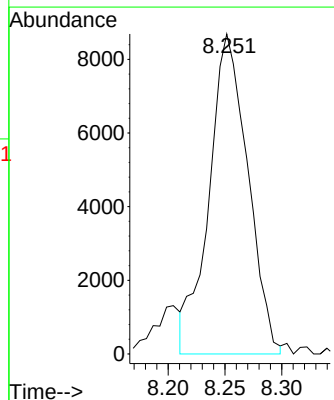
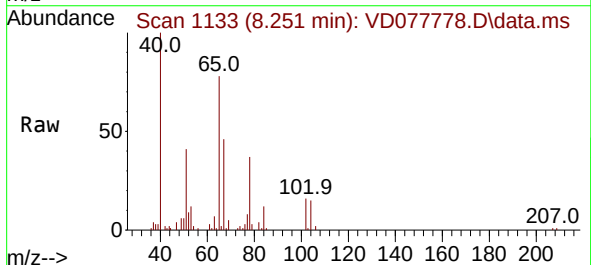


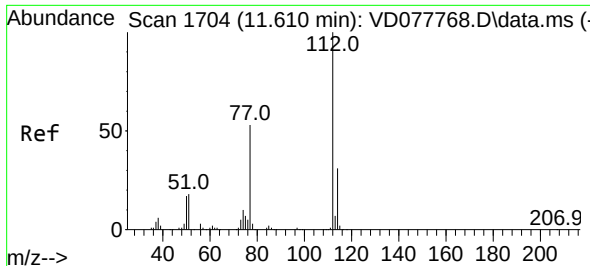

#51
Chlorobenzene
Concen: 16.987 ug/L
RT: 11.610 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11




Instrument :
MSVOA_D
ClientSampleId :
VIBLK133


Tgt Ion:112 Resp: 234310
Ion Ratio Lower Upper
112 100
114 30.4 22.5 41.9
77 57.4 46.4 69.6

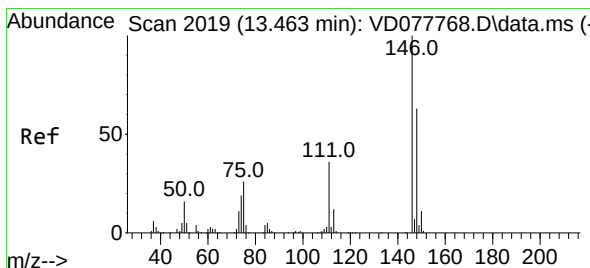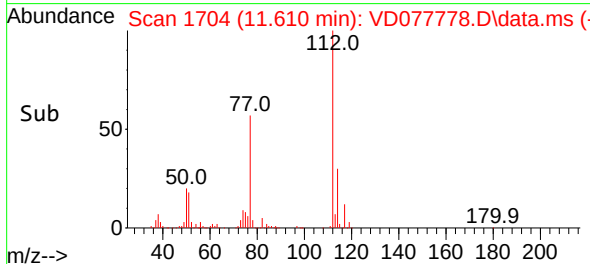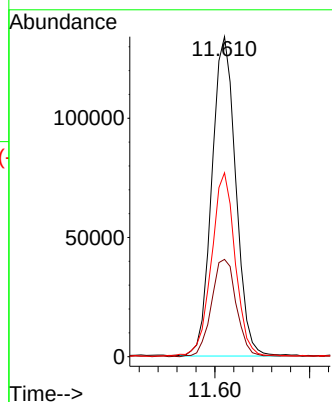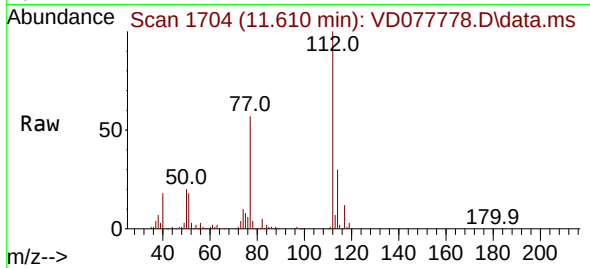

#64
1,3-Dichlorobenzene
Concen: 1.163 ug/L
RT: 13.457 min Scan# 2018
Delta R.T. -0.006 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Tgt Ion:146 Resp: 11105
Ion Ratio Lower Upper
146 100
111 29.9 26.6 49.4
148 76.6 44.0 81.6


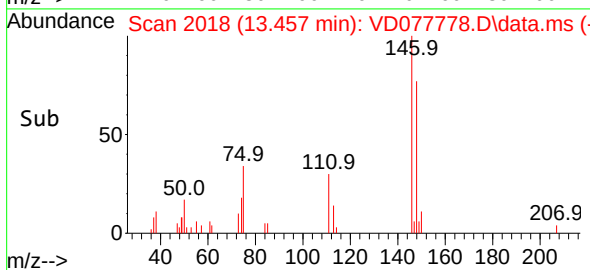
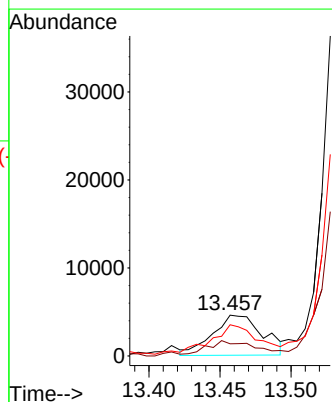
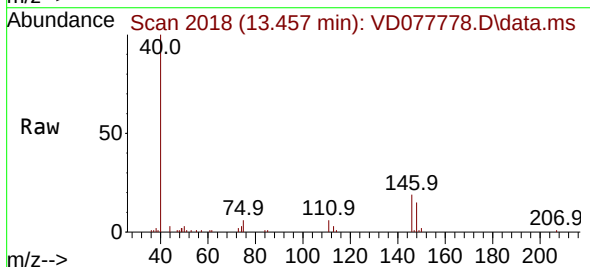


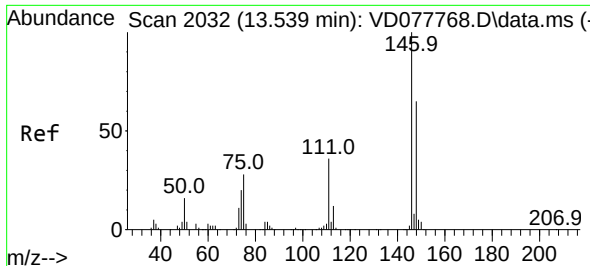

#65
1,4-Dichlorobenzene
Concen: 12.767 ug/L
RT: 13.539 min Scan# 2032
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11




Instrument :
MSVOA_D
ClientSampleId :
VIBLK133


Tgt Ion:146 Resp: 126504
Ion Ratio Lower Upper
146 100
111 33.1 26.4 49.0
148 64.5 44.0 81.8

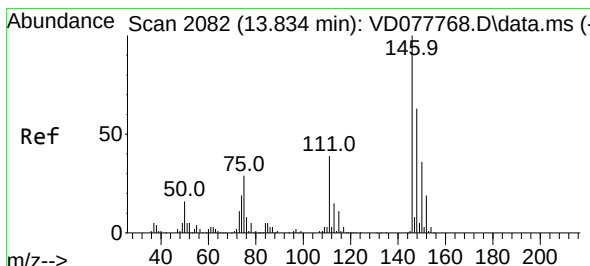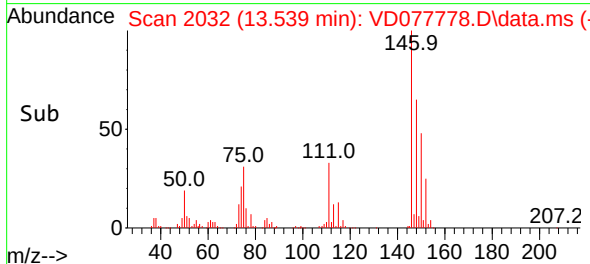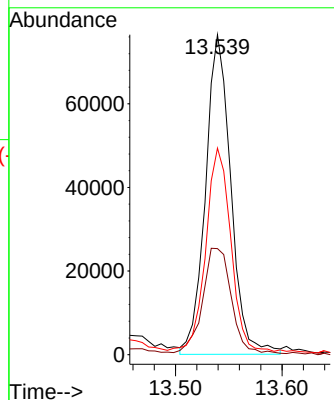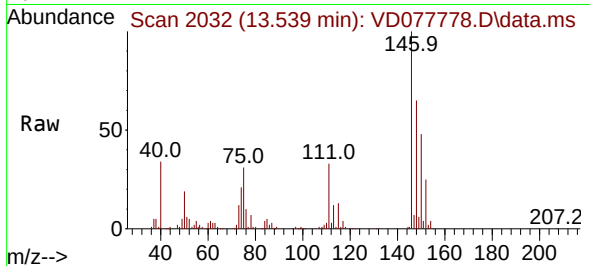

#67
1,2-Dichlorobenzene
Concen: 1.162 ug/L
RT: 13.834 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Tgt Ion:146 Resp: 9987
Ion Ratio Lower Upper
146 100
111 44.1 31.4 47.2
148 61.2 50.2 75.2


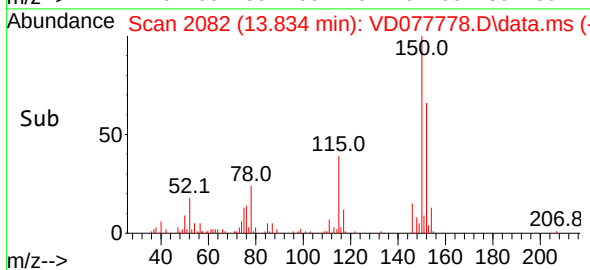
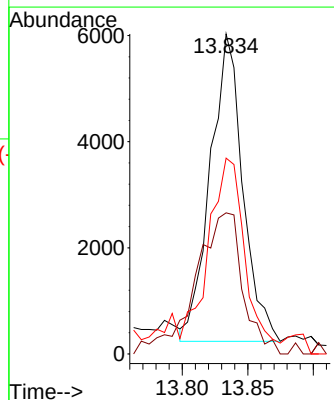
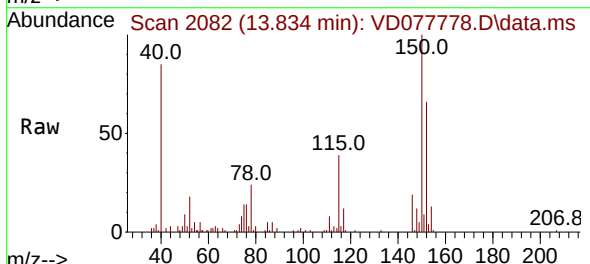


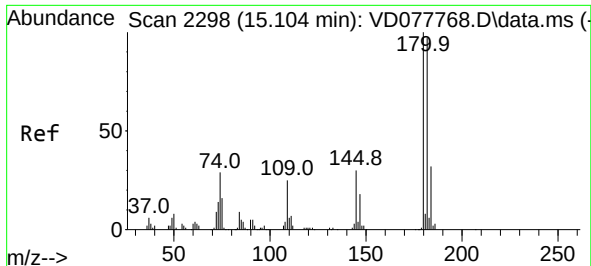

#70
1,2,4-trichlorobenzene
Concen: 12.025 ug/L
RT: 15.104 min Scan# 2298
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Instrument :
MSVOA_D
ClientSampleId :
VIBLK133

Tgt Ion:180 Resp: 66380
Ion Ratio Lower Upper
180 100
182 92.8 77.0 115.6
145 28.2 23.9 35.9

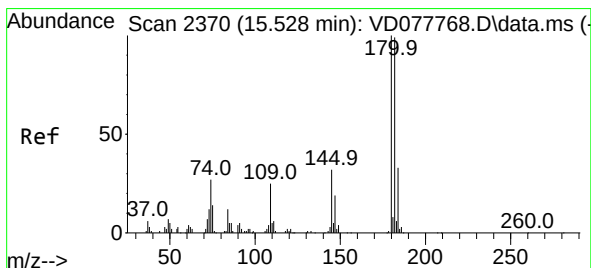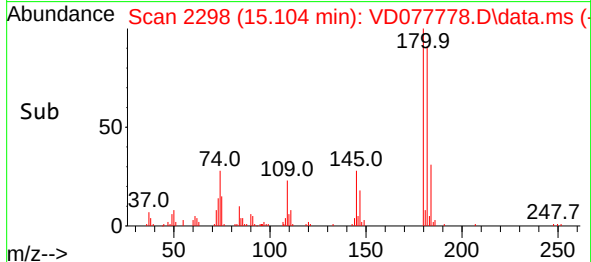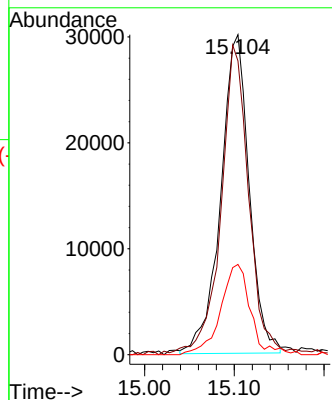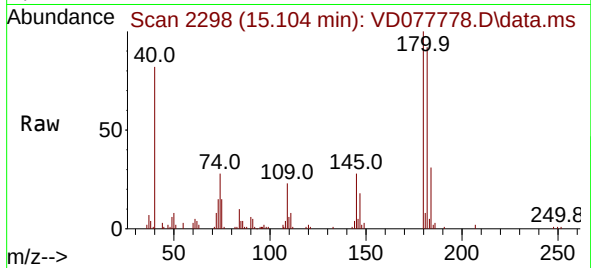

#72
1,2,3-Trichlorobenzene
Concen: 6.005 ug/L
RT: 15.528 min Scan# 2370
Delta R.T. -0.000 min
Lab File: VD077778.D
Acq: 07 Dec 2023 16:11

Tgt Ion:180 Resp: 29057
Ion Ratio Lower Upper
180 100
182 95.5 77.3 115.9
145 33.0 25.2 37.8

