
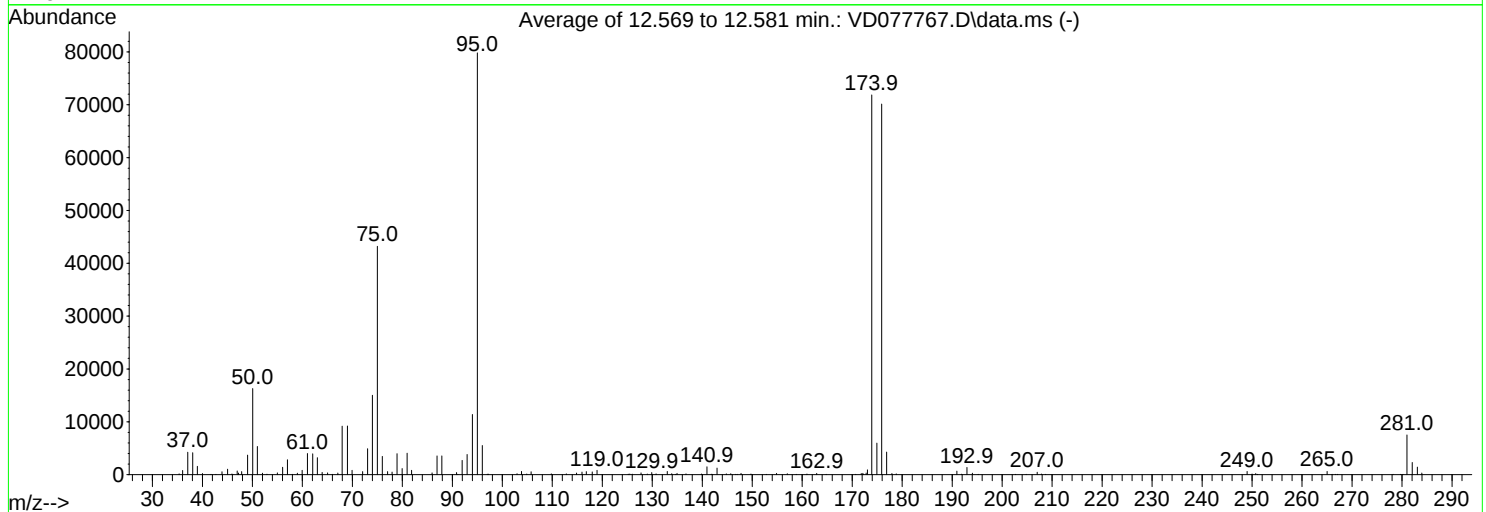


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120723\
Data File : VD077767.D
Acq On : 07 Dec 2023 08:23
Operator : JC/SY
Sample : BFB191
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB191

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Title : SFAM01.0
Last Update : Wed Dec 06 00:24:24 2023

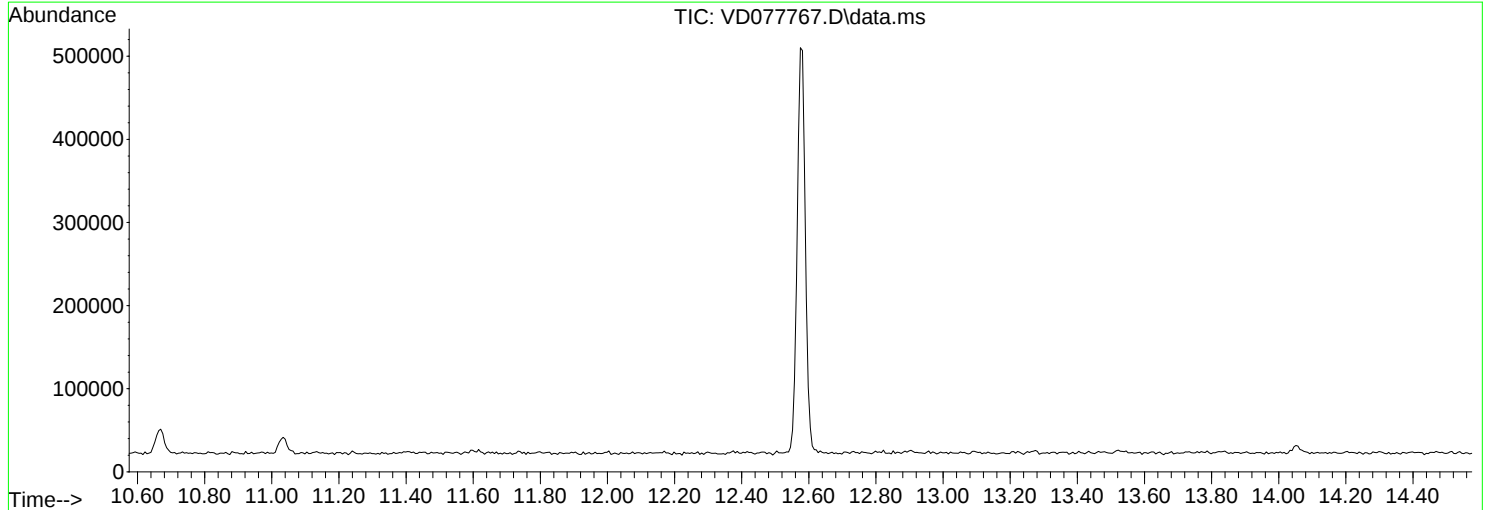

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	16293	PASS
75	95	30	80	54.1	43221	PASS
95	95	100	100	100.0	79827	PASS
96	95	5	9	6.9	5509	PASS
173	174	0.00	2	1.3	907	PASS
174	95	50	120	90.0	71859	PASS
175	174	5	9	8.3	5976	PASS
176	174	95	105	97.6	70136	PASS
177	176	5	10	6.1	4265	PASS

m/z	Abundance
35.00	184.0
39.00	244.0
40.00	21864.0
43.00	566.0
67.00	190.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

m/z	Abundance
36.10	696.0
37.10	4043.0
38.10	3512.0
39.10	1641.0
40.00	21480.0
41.70	173.0
44.00	1151.0
45.10	1029.0
47.20	930.0
47.90	411.0
49.00	3034.0
50.00	15144.0
51.00	4735.0
52.00	407.0
52.90	268.0
55.10	303.0
56.00	1122.0
57.00	2278.0
58.00	204.0
59.10	227.0
60.10	946.0
61.00	3759.0
62.00	3042.0
63.00	2793.0
63.90	280.0
65.10	232.0
67.00	230.0
68.00	8408.0
69.00	8541.0
70.00	710.0
72.00	480.0
73.00	4008.0
74.00	12380.0
75.00	37040.0
76.00	2892.0
77.10	582.0
78.00	461.0
78.90	3719.0
80.00	1079.0
80.90	3684.0
81.90	794.0
86.10	287.0
87.10	2685.0
87.90	3419.0
90.90	404.0
91.90	2357.0
93.00	3118.0
94.00	9096.0
95.00	69064.0
96.00	4442.0
103.00	244.0
103.90	411.0
104.90	220.0
105.80	475.0
114.80	242.0
116.00	565.0
116.80	257.0
118.00	268.0
119.00	681.0
126.00	240.0
127.70	388.0
129.00	377.0
130.00	298.0
133.00	478.0
134.70	172.0
135.10	151.0
136.70	202.0
139.80	163.0
141.00	1140.0
142.10	197.0
143.00	905.0
145.70	306.0
147.00	236.0
155.00	190.0
158.80	191.0
162.90	357.0
170.70	166.0
171.80	542.0
172.80	889.0
173.90	60416.0
175.00	4650.0
175.90	57344.0
176.90	3766.0
177.90	160.0
191.00	486.0
192.90	831.0
195.20	235.0
204.80	154.0
207.10	218.0
207.90	165.0
249.10	649.0
251.10	215.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

265.10	359.0
281.00	4443.0
282.10	1943.0
283.00	982.0
284.00	259.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

m/z	Abundance
35.30	202.0
36.10	870.0
37.00	4197.0
38.10	4255.0
39.10	1677.0
40.00	22576.0
43.90	1192.0
45.00	1007.0
45.90	369.0
46.90	1125.0
47.90	662.0
49.10	4147.0
50.10	17352.0
51.00	5291.0
52.00	179.0
54.90	334.0
56.10	1883.0
57.00	3229.0
58.90	222.0
59.90	716.0
61.00	4142.0
62.00	4503.0
63.00	3139.0
64.00	499.0
65.10	367.0
66.00	168.0
67.10	193.0
68.00	9322.0
69.00	10103.0
69.90	1064.0
72.10	652.0
73.00	5509.0
74.00	15803.0
75.00	45656.0
76.00	3793.0
77.10	553.0
78.00	636.0
79.00	4163.0
80.00	1395.0
80.90	4617.0
81.80	889.0
85.90	463.0
86.90	3727.0
87.90	3512.0
90.90	495.0
92.00	2919.0
93.00	4025.0
94.00	12422.0
95.00	87688.0
96.00	6149.0
97.00	245.0
103.80	686.0
104.90	158.0
105.80	445.0
109.80	210.0
112.80	247.0
114.90	306.0
116.00	516.0
116.80	708.0
117.90	724.0
118.90	882.0
125.50	391.0
127.80	308.0
130.00	288.0
130.80	255.0
132.90	657.0
133.90	367.0
134.90	247.0
136.80	234.0
140.90	1623.0
141.80	281.0
142.90	1485.0
144.80	182.0
146.70	182.0
147.70	307.0
149.80	161.0
154.80	319.0
157.00	213.0
160.90	193.0
162.90	218.0
172.00	732.0
173.10	1458.0
173.90	79320.0
174.90	6345.0
175.90	75552.0
176.90	4982.0
177.90	280.0
178.80	333.0
191.00	644.0
193.00	1421.0
194.10	451.0
206.90	598.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

207.80	206.0
249.00	628.0
250.70	266.0
264.90	614.0
266.70	202.0
278.20	156.0
281.00	8520.0
282.00	2365.0
283.10	1683.0
284.00	405.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

m/z	Abundance
35.40	228.0
36.00	839.0
37.00	4447.0
38.00	4670.0
39.00	2152.0
40.00	22176.0
42.70	203.0
44.00	1044.0
45.00	1045.0
46.10	207.0
47.00	953.0
47.80	678.0
49.00	3897.0
50.00	16384.0
51.00	5923.0
52.00	285.0
55.00	408.0
56.00	1141.0
57.00	2939.0
59.00	361.0
59.80	793.0
61.00	4099.0
62.10	4259.0
63.00	3716.0
64.00	507.0
65.00	427.0
67.10	468.0
68.00	10344.0
69.00	9005.0
70.00	662.0
72.00	641.0
73.10	5223.0
74.00	16856.0
75.00	46968.0
76.00	3724.0
76.90	578.0
77.80	321.0
78.90	4048.0
79.90	975.0
81.00	3891.0
81.90	817.0
85.80	287.0
86.90	4261.0
87.90	3707.0
90.70	291.0
91.10	200.0
92.00	2795.0
92.90	4332.0
94.00	12669.0
95.00	82728.0
96.00	5936.0
97.20	259.0
102.90	285.0
103.90	725.0
105.70	690.0
109.80	210.0
112.80	183.0
114.90	333.0
115.80	415.0
116.80	733.0
118.10	570.0
119.00	854.0
125.20	276.0
127.80	298.0
129.80	614.0
130.70	189.0
133.10	681.0
133.90	227.0
134.90	360.0
139.90	181.0
140.90	1667.0
142.90	1300.0
144.80	282.0
145.70	245.0
147.80	406.0
149.70	220.0
152.80	165.0
154.80	217.0
157.00	292.0
161.00	151.0
162.90	202.0
164.80	228.0
172.20	461.0
173.00	1263.0
173.90	75840.0
174.90	6932.0
175.90	77512.0
176.90	4048.0
178.00	234.0
178.80	155.0
190.90	879.0
191.90	249.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191

193.00	1824.0
194.00	354.0
202.70	227.0
207.10	587.0
208.70	158.0
248.90	508.0
250.00	393.0
250.80	384.0
265.10	855.0
266.00	195.0
267.10	177.0
279.70	173.0
280.20	215.0
281.00	9601.0
282.00	2627.0
283.00	1631.0
283.90	225.0

Instrument :
MSVOA_D
ClientSampleId :
BFB191