

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD120820\
 Data File : VD067905.D
 Acq On : 08 Dec 2020 10:24
 Operator : VA/SY
 Sample : VD1208SBL01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1208SBL01

Quant Time: Dec 09 04:33:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120120S.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 02 08:05:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	248751	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	353418	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	305706	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	149511	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.33	65	114561	42.90	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.80%
35) Dibromofluoromethane	7.92	113	100325	42.42	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	84.84%
50) Toluene-d8	10.34	98	387589	45.53	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	91.06%
62) 4-Bromofluorobenzene	12.64	95	127927	43.46	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.92%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD120820\
Data File : VD067905.D
Acq On : 08 Dec 2020 10:24
Operator : VA/SY
Sample : VD1208SBL01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1208SBL01

Quant Time: Dec 09 04:33:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D120120S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 02 08:05:58 2020
Response via : Initial Calibration

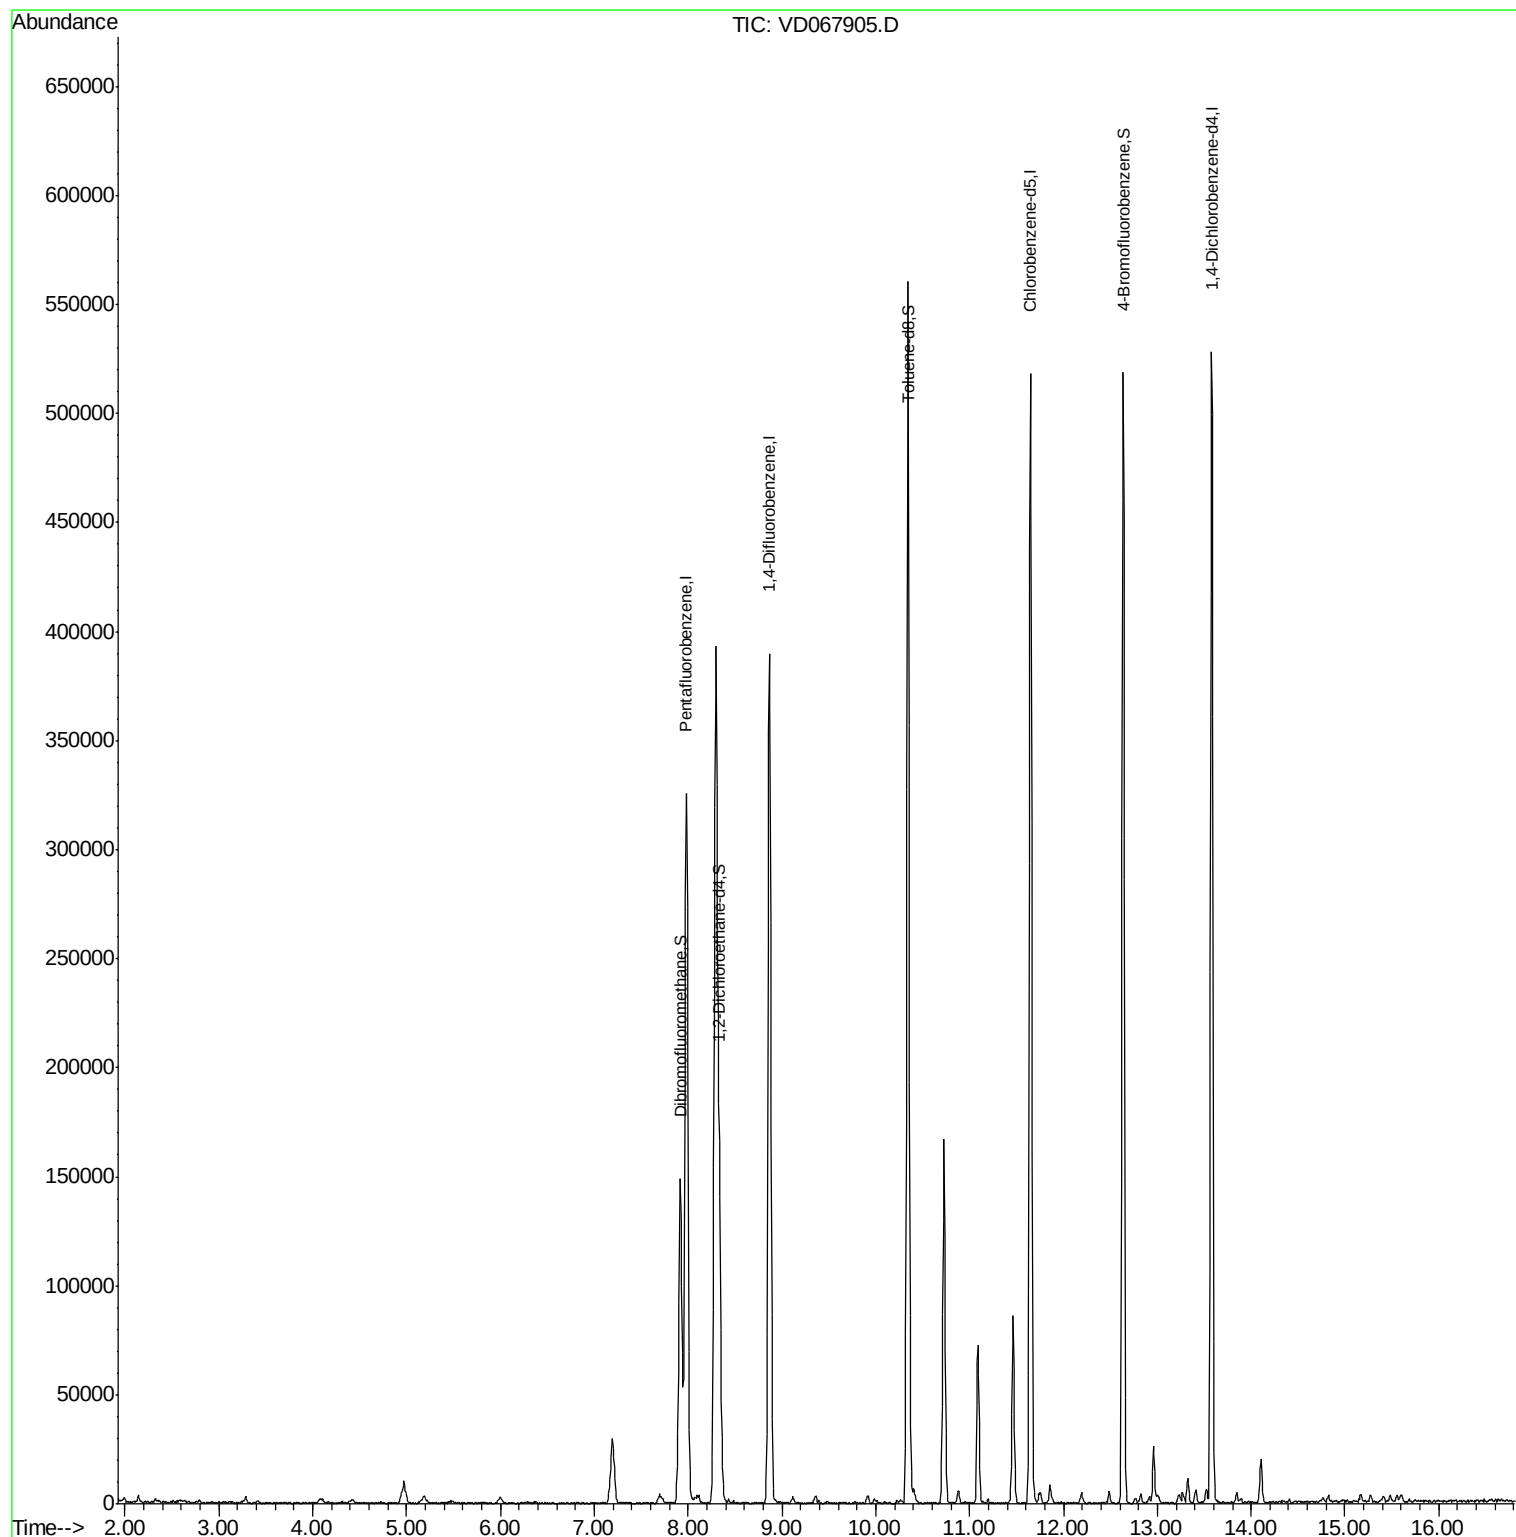

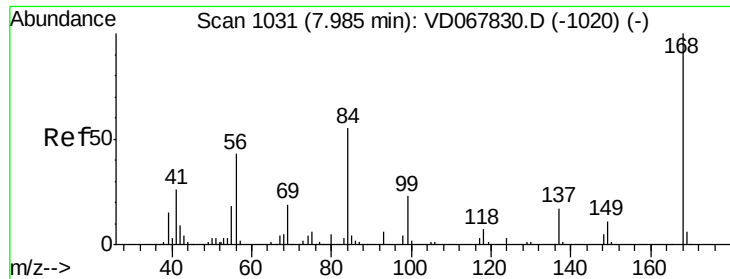

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD067905.D

Acq: 08 Dec 2020 10:24

Instrument :

MSVOA_D

ClientSampleId :


VD1208SBL01

Tot Ion:168 Resp: 248751

Ion Ratio Lower Upper

168 100

99 54.8 47.1 70.7

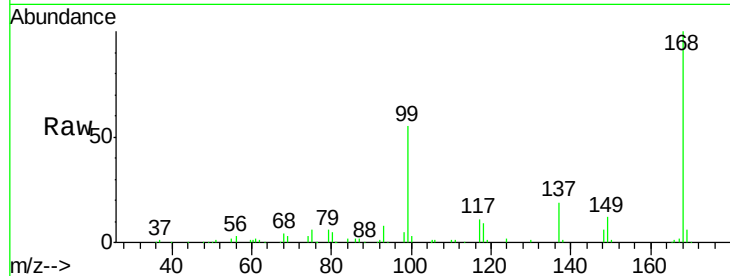

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.99

120000

100000

80000

60000

40000

20000



0

Time-->

7.90

8.00

8.10

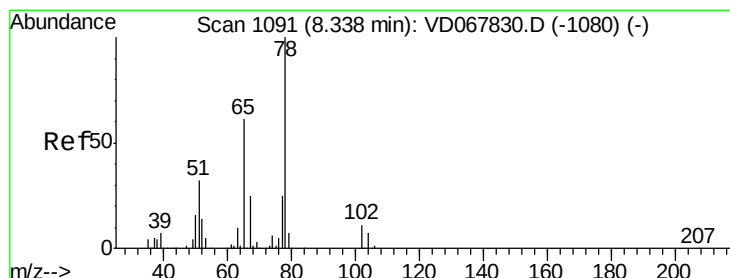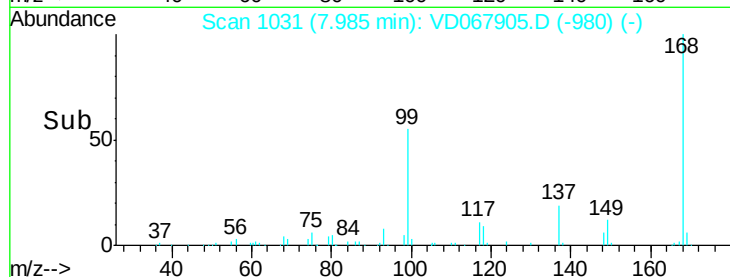

#33

1,2-Dichloroethane-d4

Concen: 42.900 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. -0.01 min

Lab File: VD067905.D


Acq: 08 Dec 2020 10:24

Tgt Ion: 65 Resp: 114561

Ion Ratio Lower Upper

65 100

67 46.7 0.0 92.0

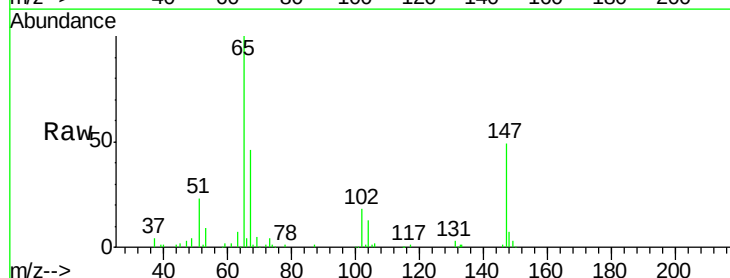

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

60000

50000

40000

30000

20000

10000


0


Time-->

8.20

8.30

8.40

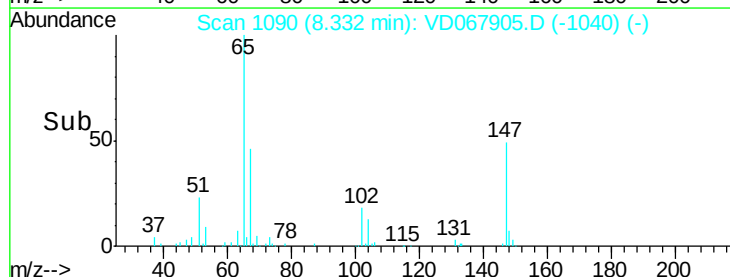


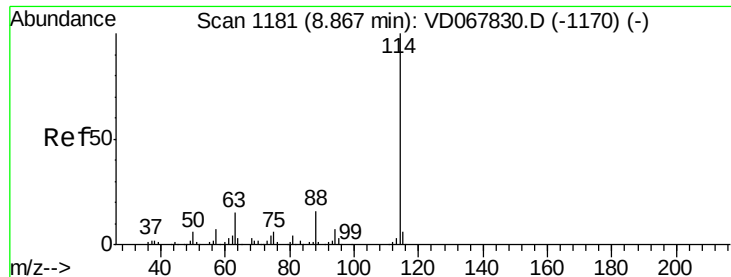




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD067905.D
 Acq: 08 Dec 2020 10:24

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1208SBL01

Tot Ion:114 Resp: 353418
 Ion Ratio Lower Upper
 114 100
 63 16.0 0.0 30.8
 88 14.0 0.0 31.8

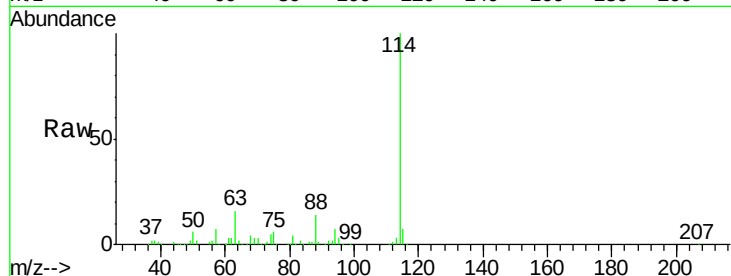


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

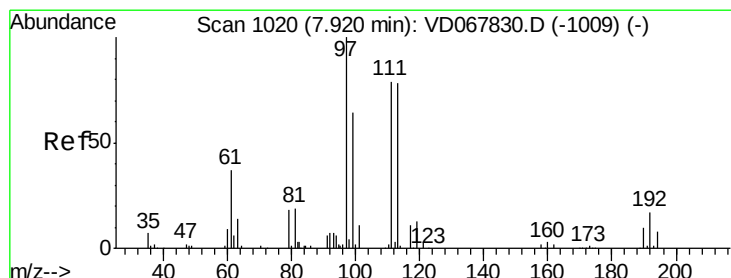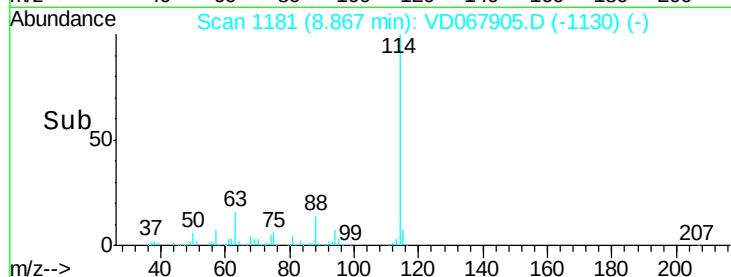
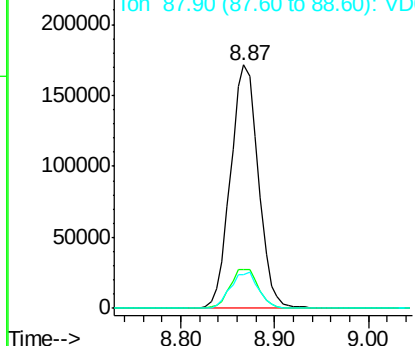



#35
 Dibromofluoromethane
 Concen: 42.423 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD067905.D
 Acq: 08 Dec 2020 10:24

Tgt Ion:113 Resp: 100325
 Ion Ratio Lower Upper
 113 100
 111 103.3 81.2 121.8
 192 21.6 16.8 25.2

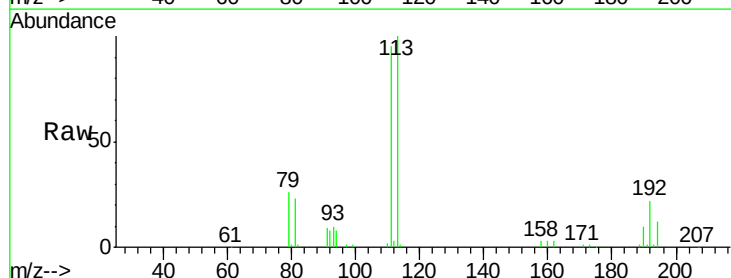

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

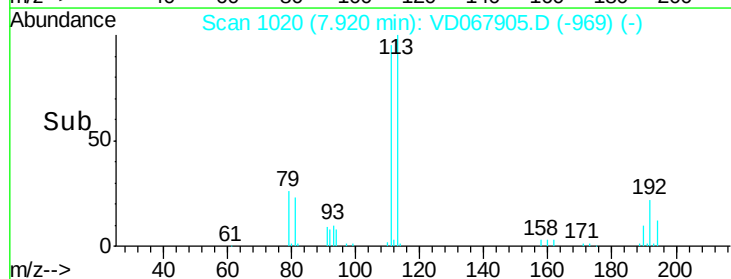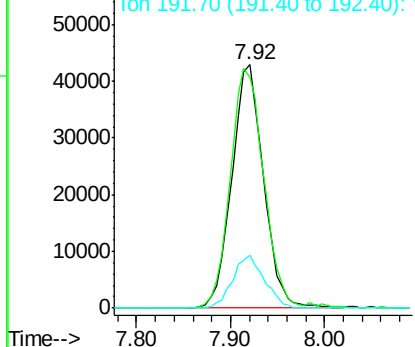

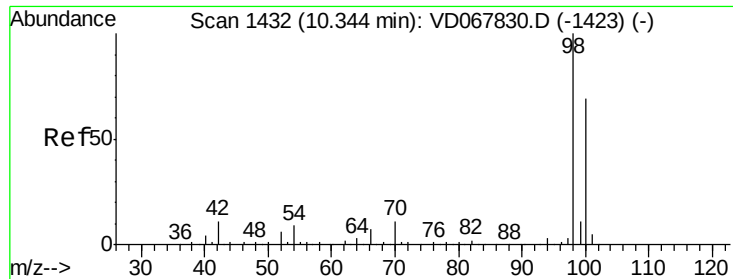

#50

Toluene-d8

Concen: 45.528 ug/l

RT: 10.34 min Scan# 1432

Delta R.T. 0.00 min

Lab File: VD067905.D

Acq: 08 Dec 2020 10:24

Instrument :

MSVOA_D

ClientSampleId :


VD1208SBL01

Tot Ion: 98 Resp: 387589

Ion Ratio Lower Upper

98 100

100 66.5 52.9 79.3

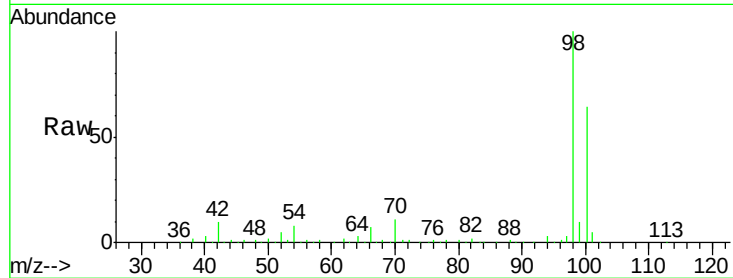

Abundance Ion 98.00 (97.70 to 98.70): VDC

Ion 100.00 (99.70 to 100.70): VDC

10.34

200000



150000

100000

50000

0

Time-->

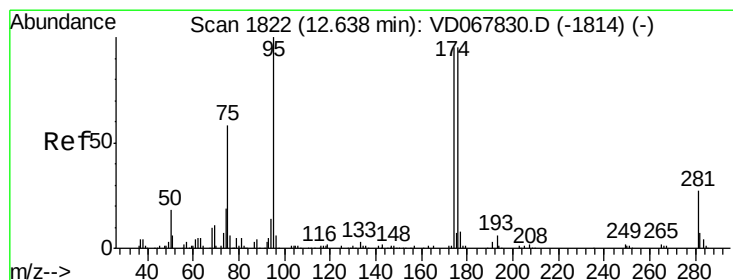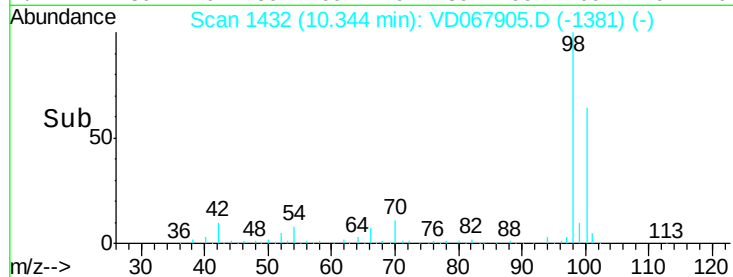

#62

4-Bromofluorobenzene

Concen: 43.465 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD067905.D

Acq: 08 Dec 2020 10:24


Tgt Ion: 95 Resp: 127927

Ion Ratio Lower Upper

95 100

174 93.1 0.0 186.0

176 92.6 0.0 184.2

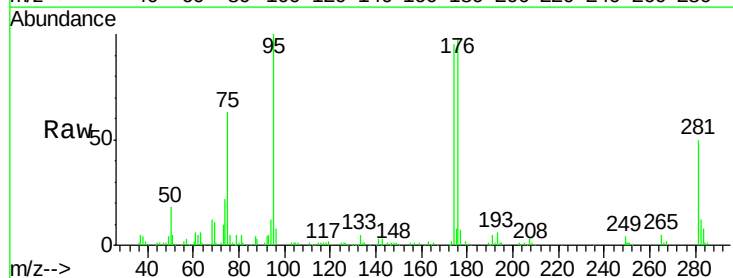

Abundance Ion 94.90 (94.60 to 95.60): VDC

Ion 173.80 (173.50 to 174.50): VDC

Ion 175.80 (175.50 to 176.50): VDC

12.64

100000

80000


60000


40000

20000

0

Time-->




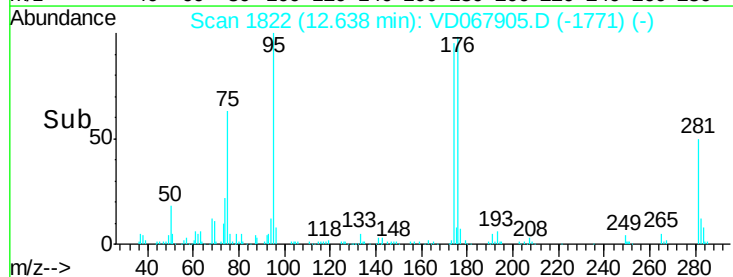


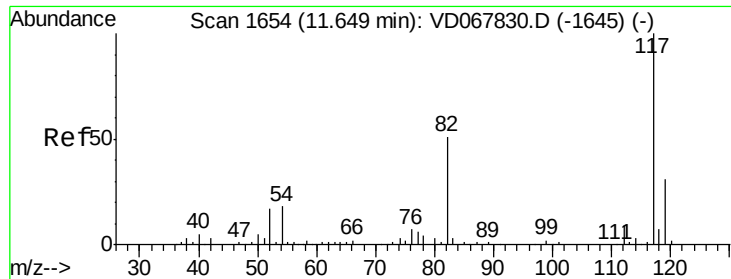

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD067905.D
Acq: 08 Dec 2020 10:24

Instrument :
MSVOA_D
ClientSampleId :
VD1208SBL01

Tot Ion:117 Resp: 305706
Ion Ratio Lower Upper
117 100
82 52.3 40.6 60.8
119 33.0 25.1 37.7

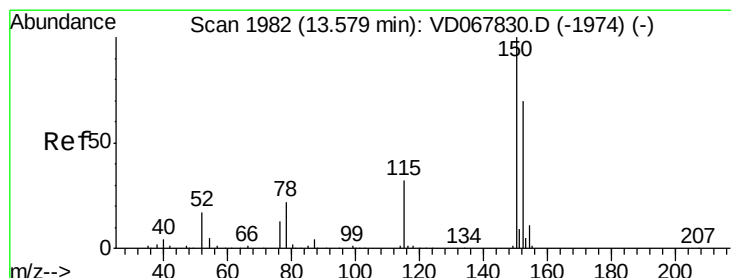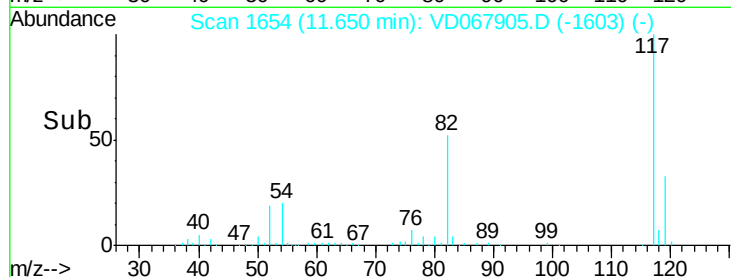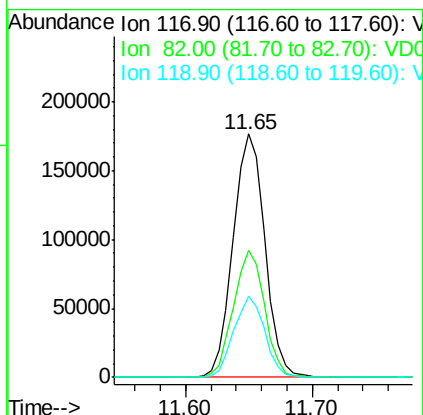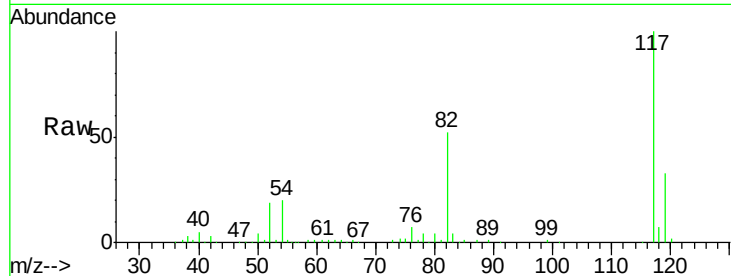

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1982
Delta R.T. 0.00 min
Lab File: VD067905.D
Acq: 08 Dec 2020 10:24

Tgt Ion:152 Resp: 149511
Ion Ratio Lower Upper
152 100
115 59.2 29.1 87.4
150 156.7 0.0 339.0

