
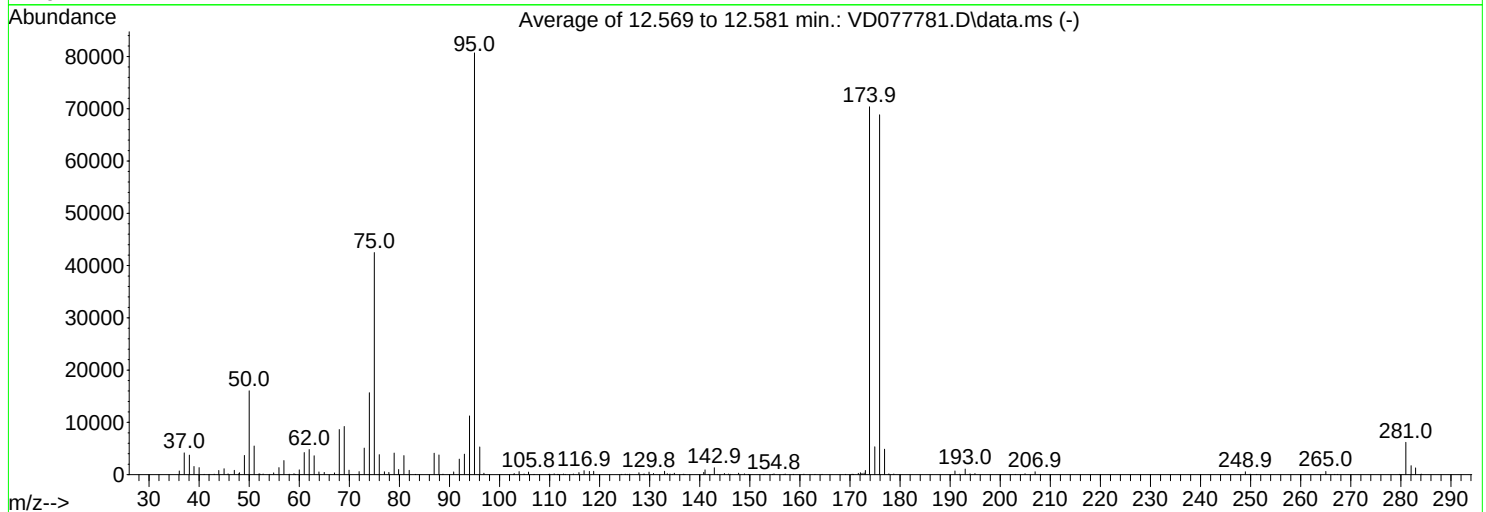


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120823\
Data File : VD077781.D
Acq On : 08 Dec 2023 08:25
Operator : JC/SY
Sample : BFB
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Fri Dec 08 13:33:18 2023

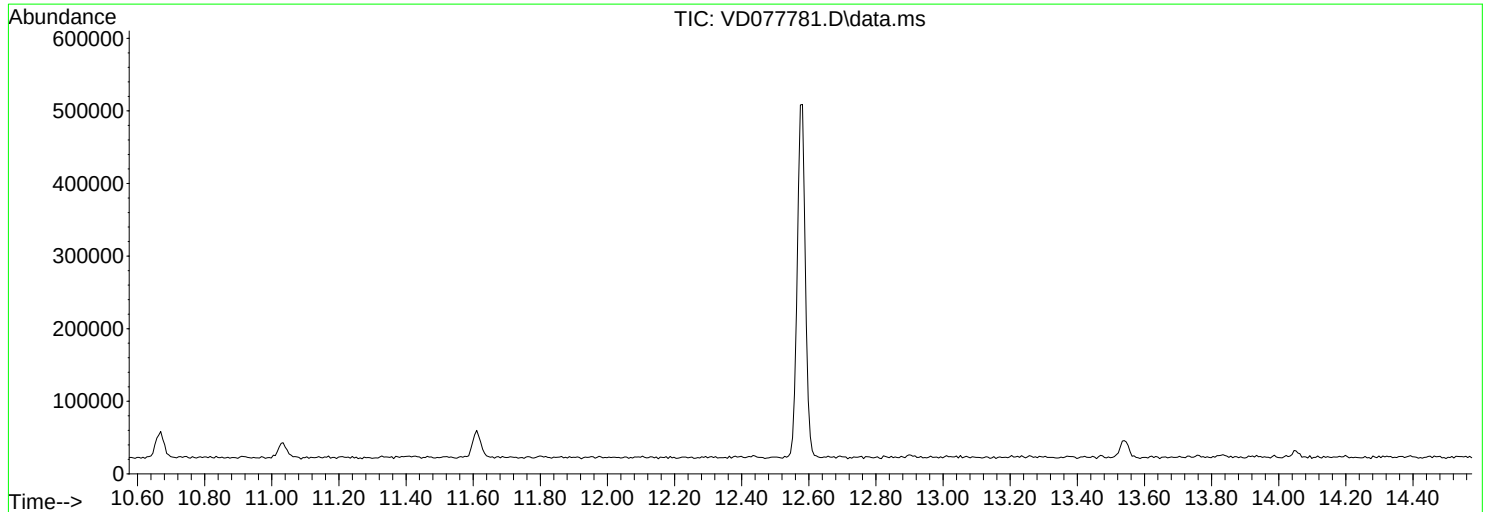

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	16028	PASS
75	95	30	60	52.7	42496	PASS
95	95	100	100	100.0	80699	PASS
96	95	5	9	6.5	5285	PASS
173	174	0.00	2	1.1	808	PASS
174	95	50	100	87.2	70379	PASS
175	174	5	9	7.6	5338	PASS
176	174	95	101	97.8	68861	PASS
177	176	5	9	7.1	4865	PASS