
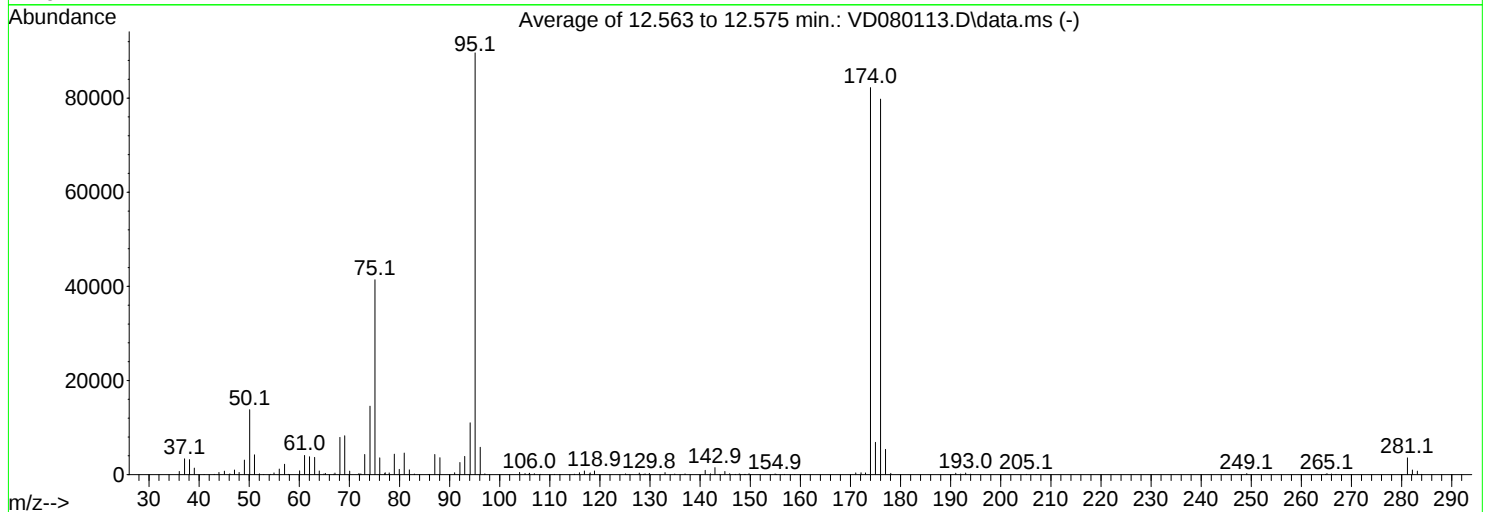


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD120924\
Data File : VD080113.D
Acq On : 09 Dec 2024 10:38
Operator : RP/MD
Sample : BFB840
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB840

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM120524SMA.M
Title : SFAM01.0
Last Update : Tue Dec 10 00:27:23 2024

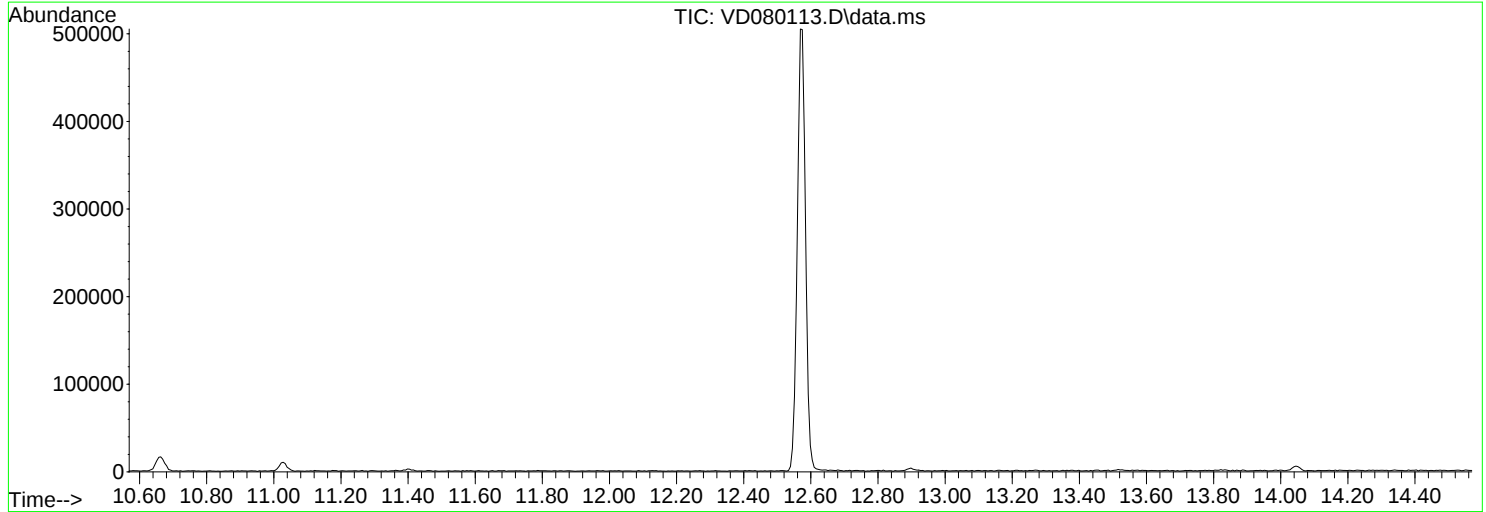

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	13811	PASS
75	95	30	80	46.2	41389	PASS
95	95	100	100	100.0	89611	PASS
96	95	5	9	6.5	5816	PASS
173	174	0.00	2	0.5	387	PASS
174	95	50	120	91.8	82227	PASS
175	174	5	9	8.3	6857	PASS
176	174	95	105	97.0	79773	PASS
177	176	5	10	6.7	5381	PASS

Scan 1859 (12.522 min): VD080113.D\data.ms
BFB840

m/z	Abundance
40.00	927.0
44.10	230.0
207.10	177.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840

m/z	Abundance
36.00	664.0
37.10	2445.0
38.10	2957.0
39.00	1191.0
40.10	845.0
44.00	724.0
45.00	672.0
47.00	597.0
48.00	552.0
49.00	2706.0
50.10	11480.0
51.10	3362.0
54.90	261.0
56.00	1107.0
57.00	1947.0
57.90	171.0
60.10	659.0
61.00	2637.0
62.00	3063.0
63.10	3326.0
64.00	764.0
65.20	493.0
66.90	274.0
68.10	6568.0
69.00	6627.0
70.10	637.0
71.90	312.0
73.10	3066.0
74.10	11963.0
75.10	33080.0
76.10	3076.0
77.00	630.0
78.00	291.0
78.90	3768.0
80.00	908.0
81.00	3726.0
81.90	950.0
83.00	219.0
87.00	3846.0
88.10	3098.0
91.10	382.0
92.10	2154.0
93.00	2531.0
94.10	9236.0
95.10	71600.0
96.10	4770.0
103.90	504.0
105.10	199.0
105.80	322.0
107.00	171.0
114.90	278.0
116.00	361.0
116.90	576.0
117.90	430.0
118.80	671.0
125.40	180.0
127.80	207.0
128.10	213.0
129.90	292.0
133.00	472.0
135.00	168.0
137.10	197.0
141.00	771.0
142.10	197.0
143.00	1288.0
144.90	620.0
145.90	211.0
148.10	255.0
149.80	155.0
158.90	166.0
171.10	336.0
173.00	1162.0
174.00	65232.0
175.00	5463.0
176.00	64024.0
177.00	4486.0
178.00	233.0
190.90	204.0
193.00	230.0
249.10	237.0
264.80	234.0
281.10	2546.0
282.20	776.0
283.10	738.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840

m/z	Abundance
36.10	671.0
37.10	3896.0
38.10	3587.0
39.00	1465.0
40.00	800.0
43.00	200.0
43.90	674.0
45.10	760.0
46.20	254.0
47.10	1415.0
48.00	392.0
49.00	3192.0
50.10	14995.0
51.00	4742.0
52.00	203.0
54.90	386.0
56.00	1157.0
57.10	2612.0
60.00	883.0
61.00	4770.0
62.10	4286.0
63.10	4011.0
64.00	889.0
64.90	430.0
67.10	535.0
68.10	8365.0
69.10	8837.0
70.10	792.0
71.90	450.0
73.00	5173.0
74.10	15513.0
75.10	45328.0
76.00	3895.0
77.20	521.0
78.00	381.0
79.00	5100.0
80.00	1371.0
80.90	4995.0
82.00	1006.0
82.90	164.0
87.10	4977.0
88.10	4055.0
90.90	551.0
92.00	2960.0
93.00	4741.0
94.10	11622.0
95.10	100976.0
96.10	7125.0
97.00	290.0
103.90	399.0
105.10	163.0
106.00	431.0
106.90	293.0
108.10	170.0
110.90	178.0
115.80	329.0
117.00	958.0
118.10	477.0
118.90	1035.0
125.10	279.0
125.80	206.0
127.80	406.0
128.70	249.0
129.10	261.0
129.80	224.0
133.00	375.0
134.90	244.0
136.90	309.0
140.90	1104.0
142.00	294.0
143.00	1423.0
145.00	716.0
146.00	199.0
147.00	201.0
147.80	264.0
148.80	188.0
149.70	249.0
155.00	360.0
160.90	154.0
171.00	418.0
172.20	487.0
174.00	90736.0
175.00	7416.0
176.00	85032.0
177.00	5285.0
178.00	237.0
191.00	316.0
192.00	193.0
193.00	415.0
205.10	220.0
207.20	231.0
249.00	267.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840

265.10	344.0
266.00	202.0
266.90	197.0
281.20	3473.0
282.10	872.0
283.20	636.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840

m/z	Abundance
36.10	741.0
37.10	3779.0
38.10	3028.0
39.10	1538.0
40.00	710.0
41.00	158.0
44.00	753.0
45.00	810.0
46.10	256.0
47.00	990.0
48.00	519.0
49.10	3415.0
50.10	14958.0
51.10	4555.0
52.10	293.0
52.90	166.0
54.20	220.0
55.00	475.0
56.00	1331.0
57.00	2074.0
60.00	881.0
61.10	4854.0
62.00	4056.0
63.00	3650.0
64.00	675.0
65.20	299.0
67.10	506.0
68.10	8793.0
69.10	9349.0
69.90	834.0
72.30	538.0
73.00	4633.0
74.10	16159.0
75.10	45760.0
76.00	3789.0
77.10	699.0
77.90	459.0
79.00	4229.0
79.90	1050.0
80.90	5050.0
81.90	1072.0
85.90	254.0
87.00	4016.0
88.00	3703.0
90.90	297.0
92.10	2603.0
93.00	4314.0
94.10	12160.0
95.10	96256.0
96.10	5552.0
97.10	209.0
104.00	570.0
105.00	331.0
105.90	450.0
106.80	153.0
112.00	151.0
115.90	546.0
116.80	804.0
118.00	690.0
119.00	686.0
125.10	215.0
127.90	409.0
128.90	227.0
129.90	330.0
133.00	457.0
141.10	844.0
142.90	1792.0
143.90	191.0
145.00	719.0
145.80	205.0
147.80	292.0
149.00	185.0
149.80	228.0
154.80	186.0
155.20	191.0
156.80	211.0
171.10	358.0
172.00	785.0
174.00	90712.0
175.00	7692.0
176.00	90264.0
177.00	6372.0
178.10	342.0
191.10	388.0
192.00	210.0
193.00	363.0
194.00	327.0
207.00	405.0
249.20	220.0
265.10	422.0
266.00	261.0
281.20	4741.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840

282.10	1352.0
283.10	875.0
284.00	213.0

Instrument :
MSVOA_D
ClientSampleId :
BFB840