
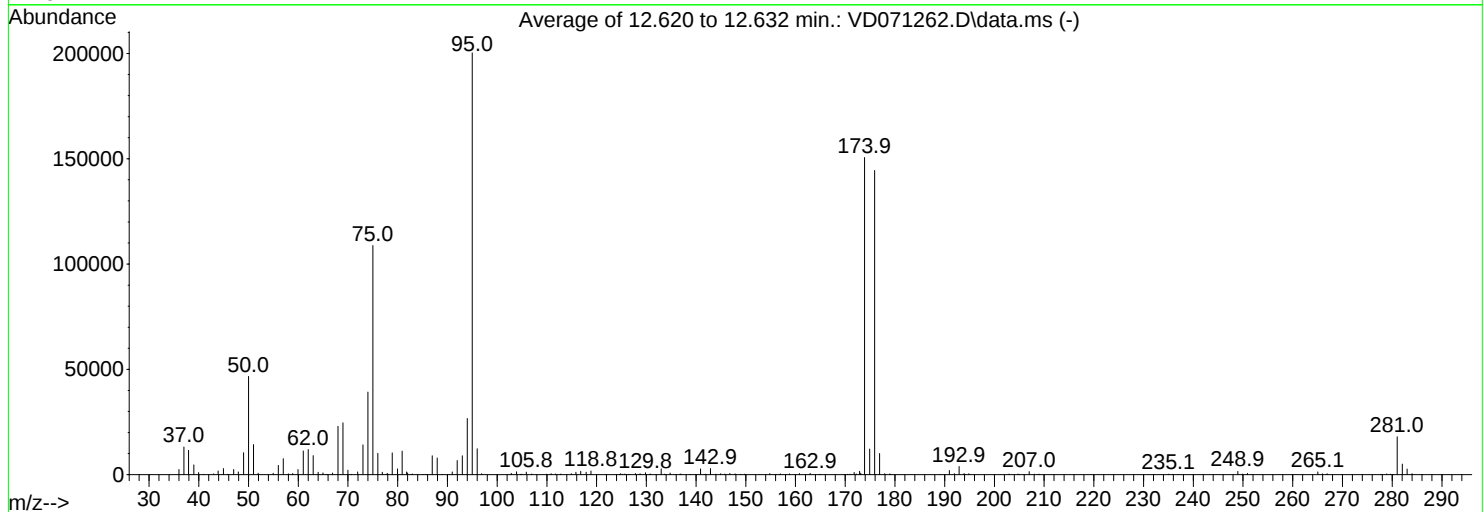


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121121\
Data File : VD071262.D
Acq On : 11 Dec 2021 10:08
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Title : SW846 8260
Last Update : Mon Nov 29 17:54:09 2021

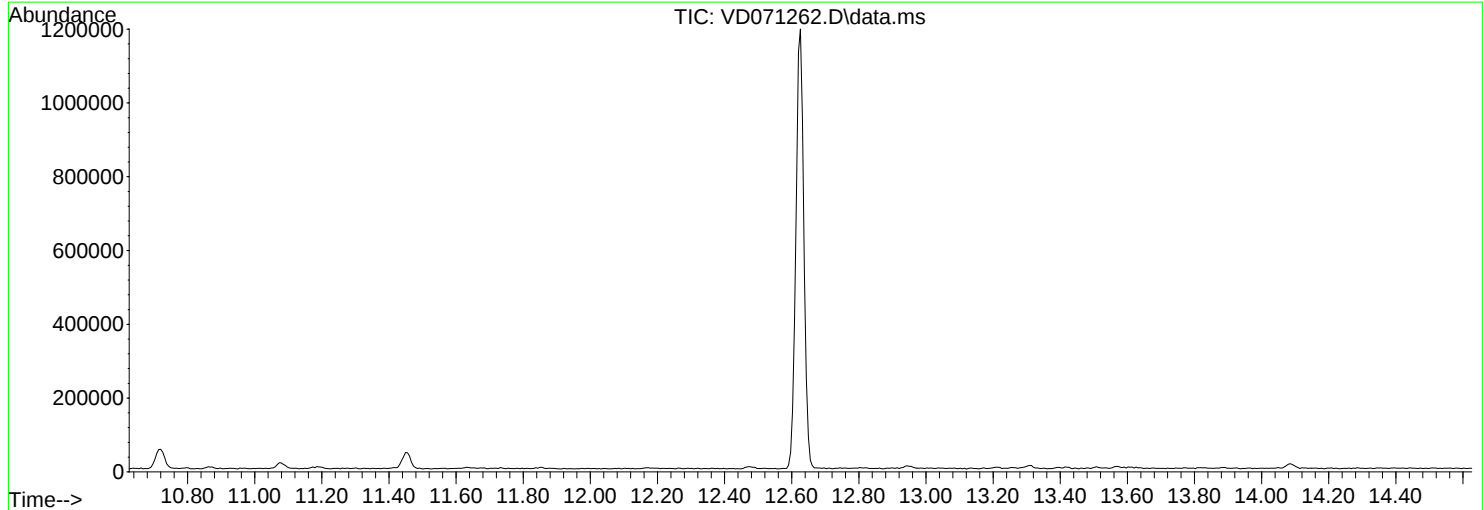

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	46629	PASS
75	95	30	60	54.3	108816	PASS
95	95	100	100	100.0	200299	PASS
96	95	5	9	6.2	12347	PASS
173	174	0.00	2	1.0	1573	PASS
174	95	50	100	75.2	150571	PASS
175	174	5	9	8.1	12147	PASS
176	174	95	101	95.9	144469	PASS
177	176	5	9	6.9	10016	PASS