


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD121218\
Data File : VD060538.D
Acq On : 12 Dec 2018 10:34
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Title : SW846 8260
Last Update : Thu Dec 06 01:49:20 2018

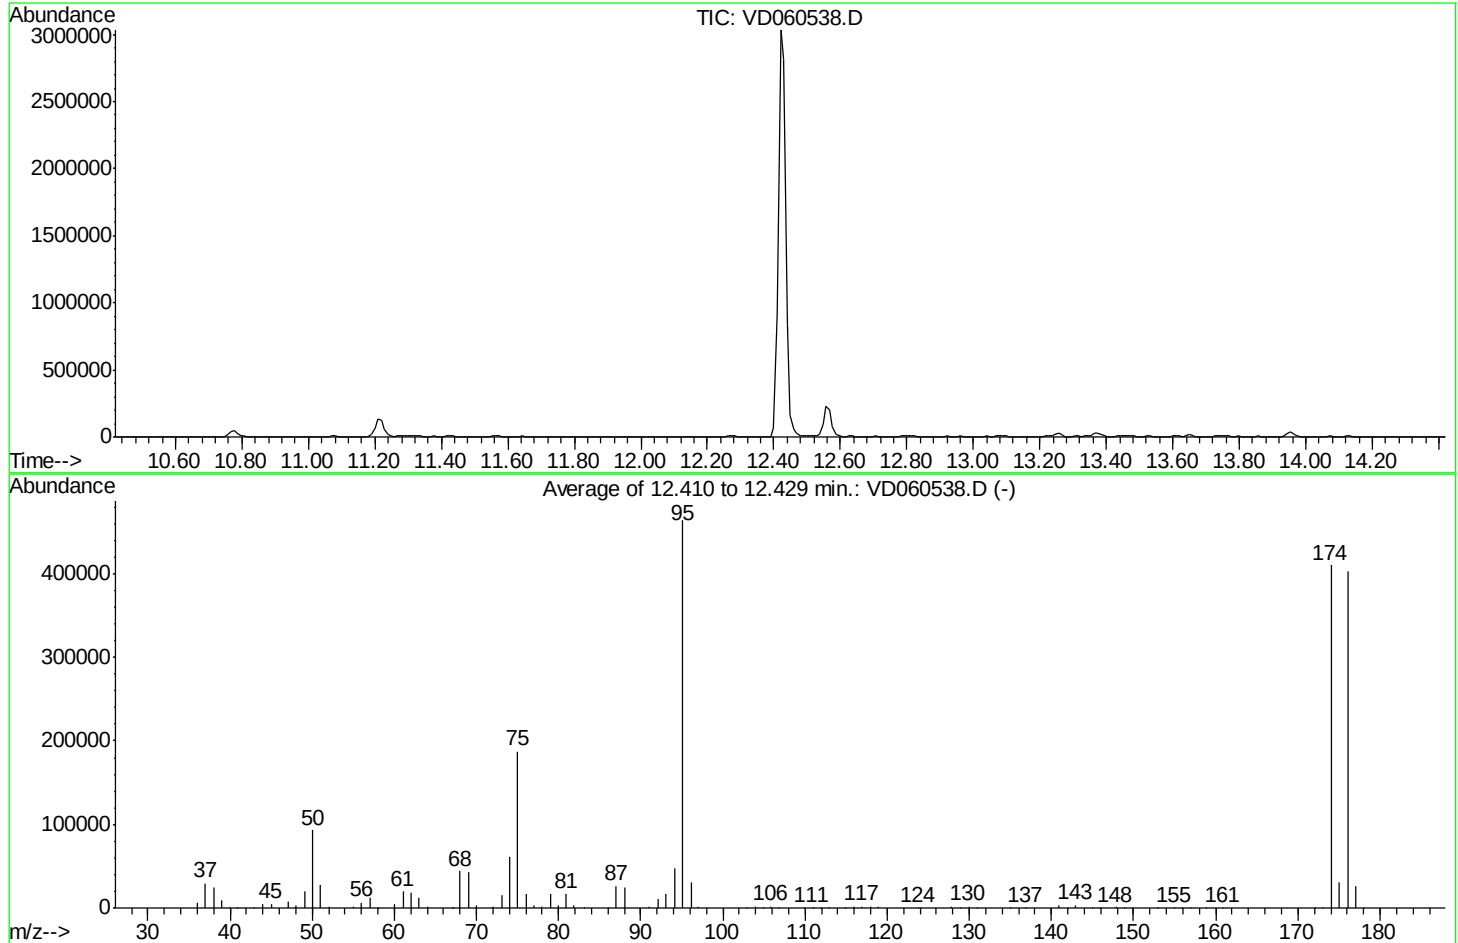

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1102

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	92858	PASS
75	95	30	60	40.4	187333	PASS
95	95	100	100	100.0	463914	PASS
96	95	5	9	6.7	31246	PASS
173	174	0.00	2	0.1	259	PASS
174	95	50	100	88.4	410200	PASS
175	174	5	9	7.3	29992	PASS
176	174	95	101	98.4	403594	PASS
177	176	5	9	6.5	26247	PASS