

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121223\
 Data File : VD077824.D
 Acq On : 11 Dec 2023 21:04
 Operator : JC/SY
 Sample : 05628-01
 Misc : 5.05G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-01-7.5-8.0

Quant Time: Dec 12 00:52:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 08 13:33:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	141802	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	328541	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	326854	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	146003	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	92181	55.167	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.340%
35) Dibromofluoromethane	7.805	113	107348	46.646	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.300%
50) Toluene-d8	10.269	98	442782	48.039	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.080%
62) 4-Bromofluorobenzene	12.575	95	123176	44.699	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	89.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121223\
Data File : VD077824.D
Acq On : 11 Dec 2023 21:04
Operator : JC/SY
Sample : 05628-01
Misc : 5.05G/5.0ml/MSVOA_D/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-01-7.5-8.0

Quant Time: Dec 12 00:52:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Fri Dec 08 13:33:18 2023
Response via : Initial Calibration



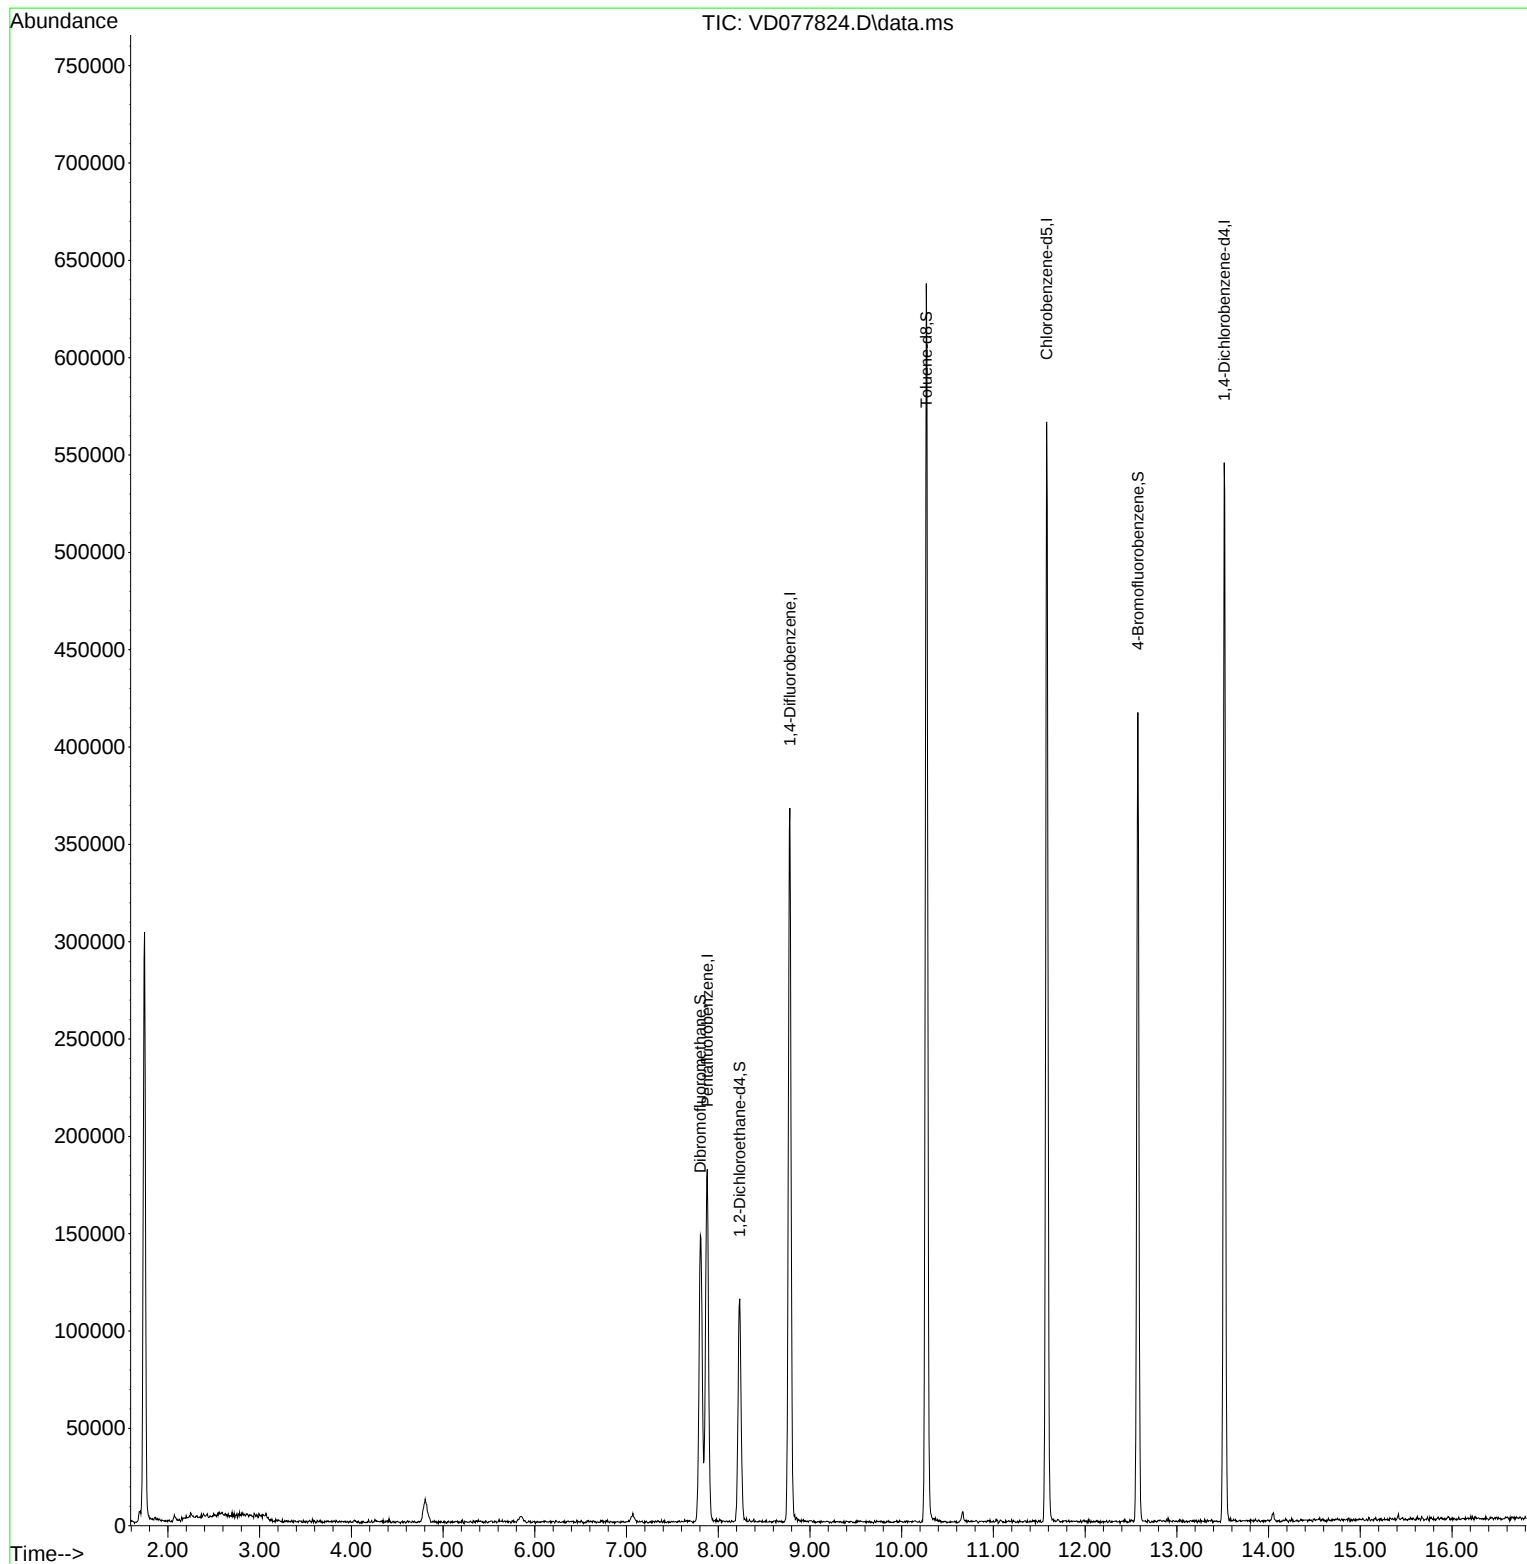


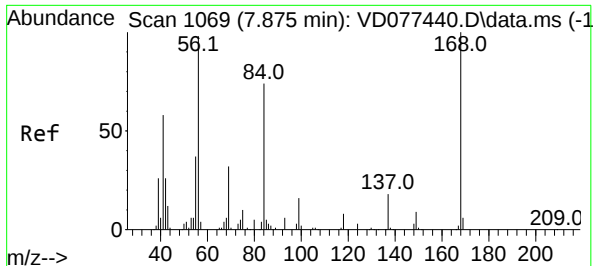

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 110
Delta R.T. 0.006 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04




Instrument :
MSVOA_D
ClientSampleId :
SB-01-7.5-8.0


Tgt Ion:168 Resp: 141802
Ion Ratio Lower Upper
168 100
99 52.3 36.7 55.1

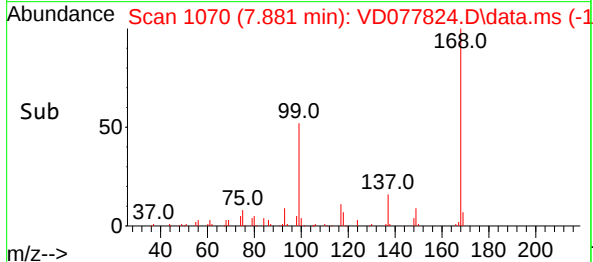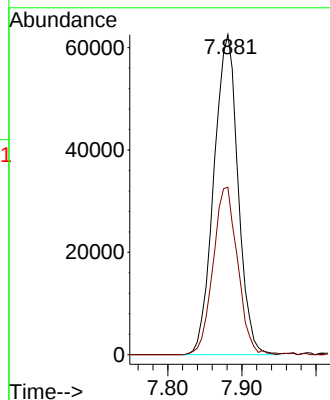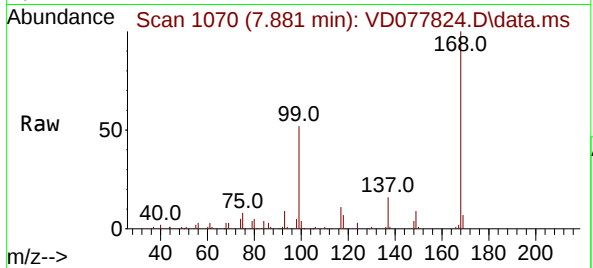

#33
1,2-Dichloroethane-d4
Concen: 55.167 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04

Tgt Ion: 65 Resp: 92181
Ion Ratio Lower Upper
65 100
67 52.8 0.0 115.0

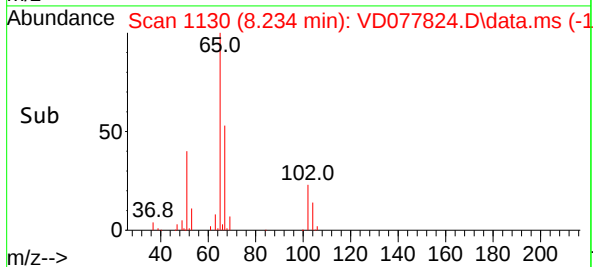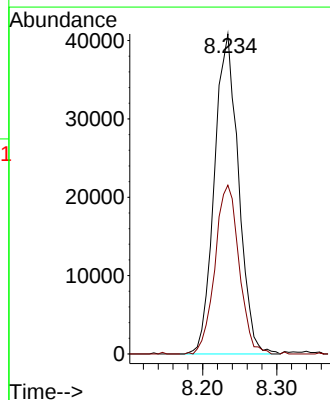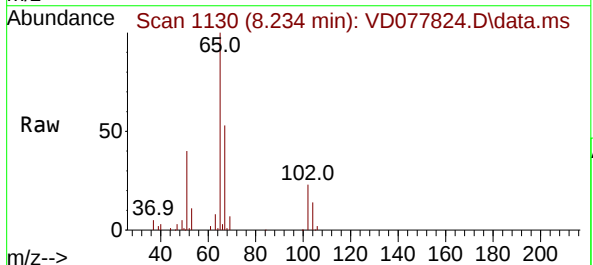

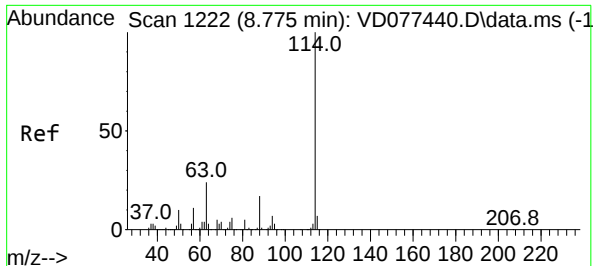

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD077824.D

Acq: 11 Dec 2023 21:04

Instrument :

MSVOA_D

ClientSampleId :

SB-01-7.5-8.0




Tgt Ion:114 Resp: 328541

Ion Ratio Lower Upper

114 100

63 19.3 0.0 33.4

88 15.2 0.0 26.2

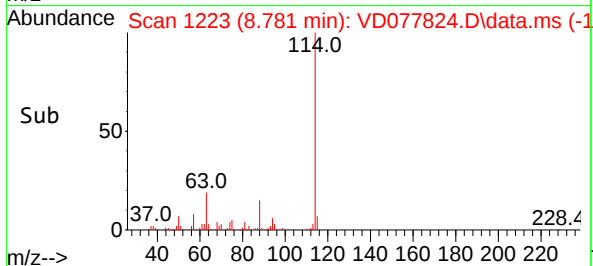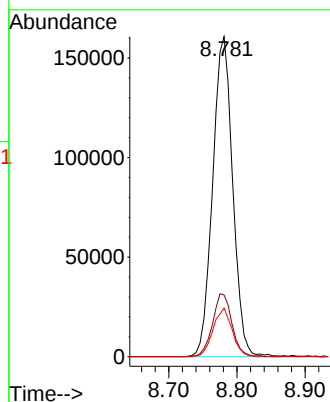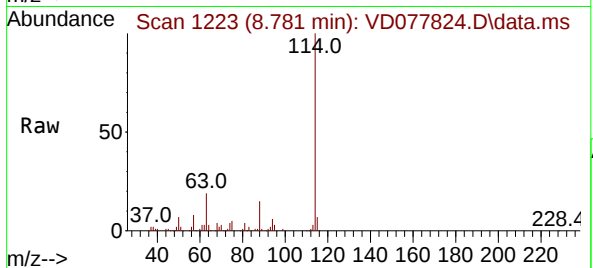

#35

Dibromofluoromethane

Concen: 46.646 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. 0.001 min

Lab File: VD077824.D

Acq: 11 Dec 2023 21:04




Tgt Ion:113 Resp: 107348

Ion Ratio Lower Upper

113 100

111 105.0 84.7 127.1

192 19.2 16.8 25.2

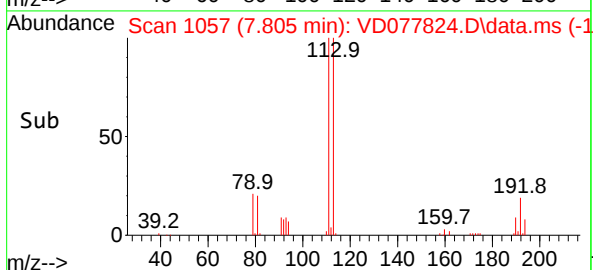
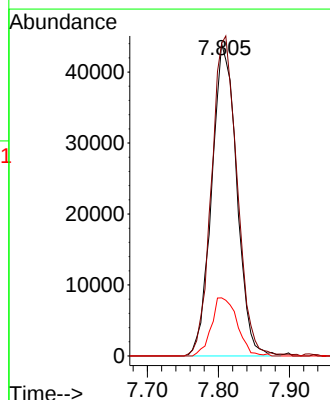
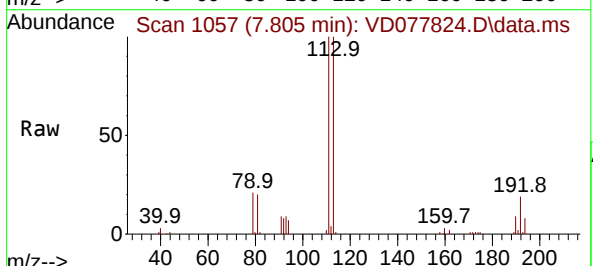




#50
Toluene-d8
Concen: 48.039 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04




Instrument :
MSVOA_D
ClientSampleId :
SB-01-7.5-8.0


Tgt Ion: 98 Resp: 442782
Ion Ratio Lower Upper
98 100
100 63.4 50.3 75.5

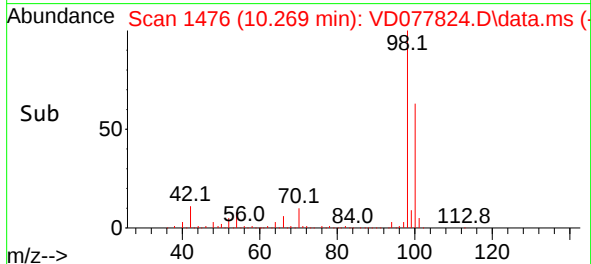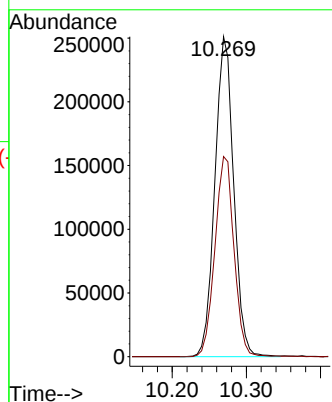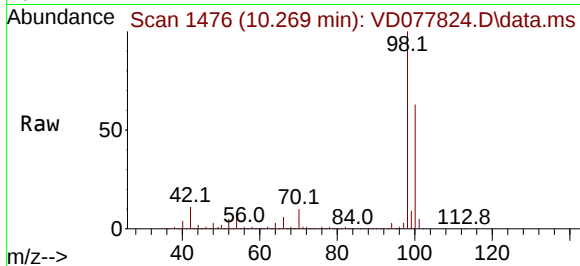

#62
4-Bromofluorobenzene
Concen: 44.699 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04

Tgt Ion: 95 Resp: 123176
Ion Ratio Lower Upper
95 100
174 90.5 0.0 201.8
176 88.5 0.0 191.8


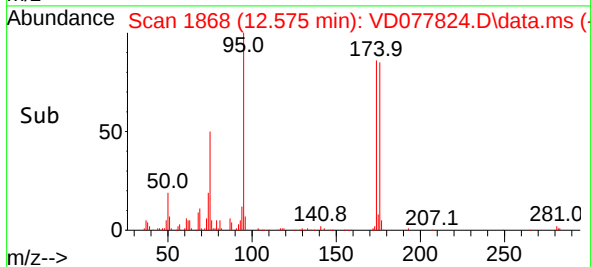
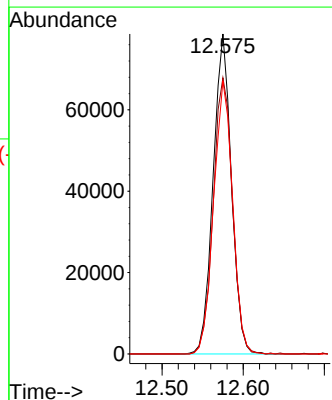
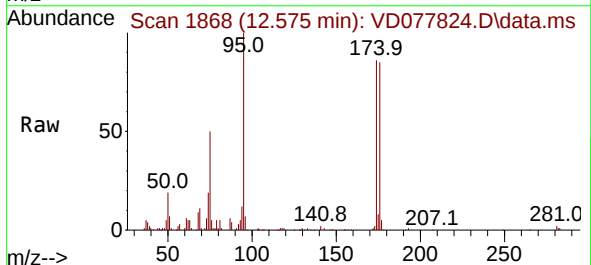


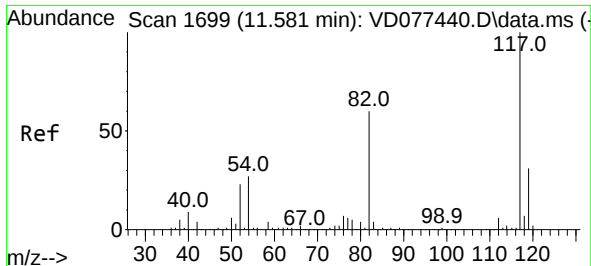

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04

Instrument :
MSVOA_D
ClientSampleId :
SB-01-7.5-8.0

Tgt Ion:117 Resp: 326854
Ion Ratio Lower Upper
117 100
82 53.0 38.3 57.5
119 32.4 25.0 37.4

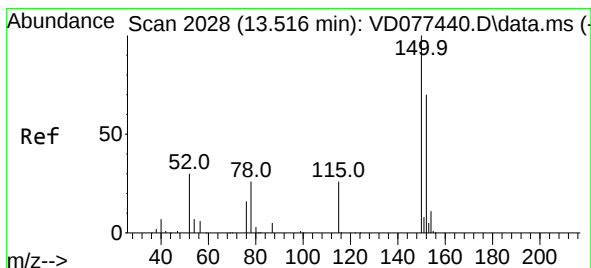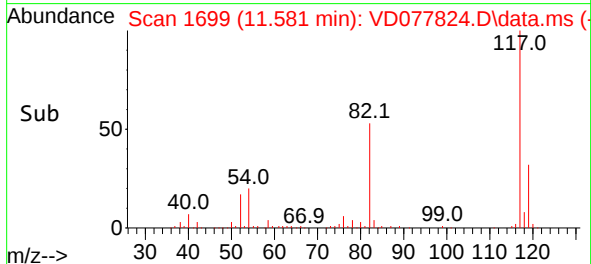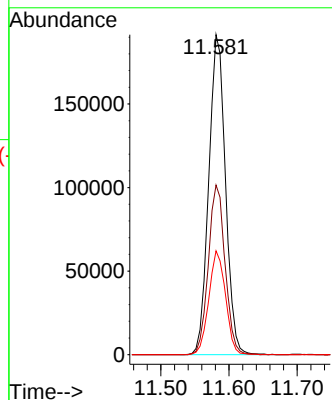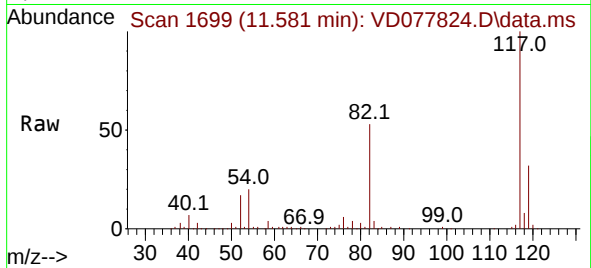

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD077824.D
Acq: 11 Dec 2023 21:04

Tgt Ion:152 Resp: 146003
Ion Ratio Lower Upper
152 100
115 56.4 27.1 81.3
150 157.5 0.0 353.6

