
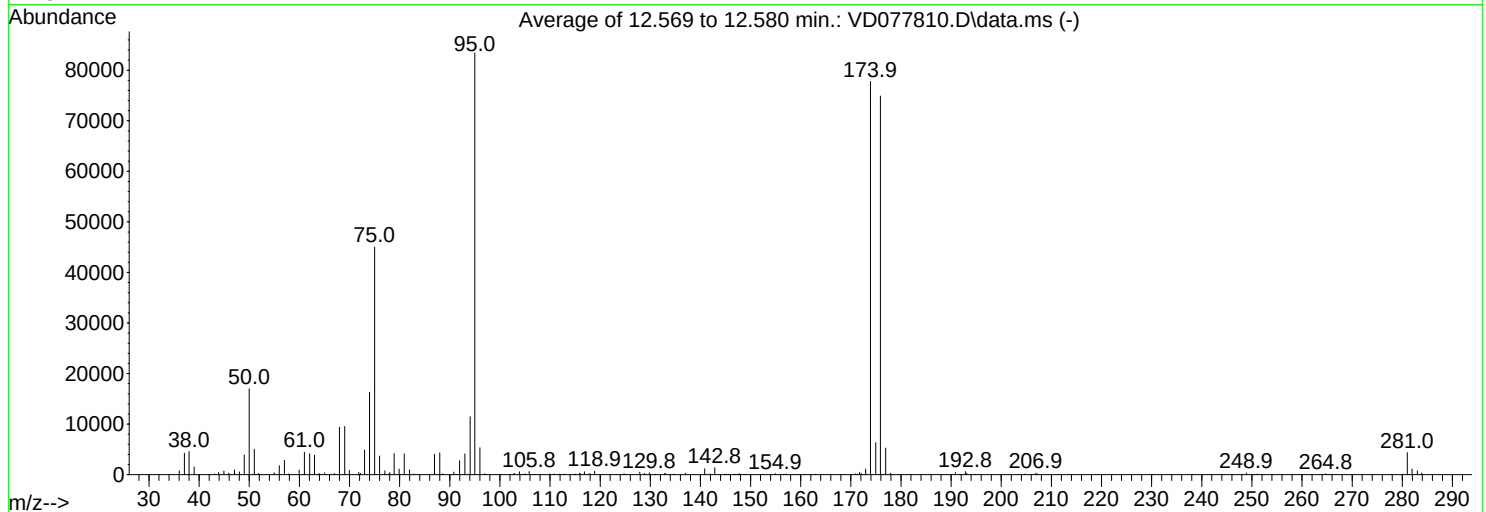


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121223\
Data File : VD077810.D
Acq On : 11 Dec 2023 13:22
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Fri Dec 08 13:33:18 2023

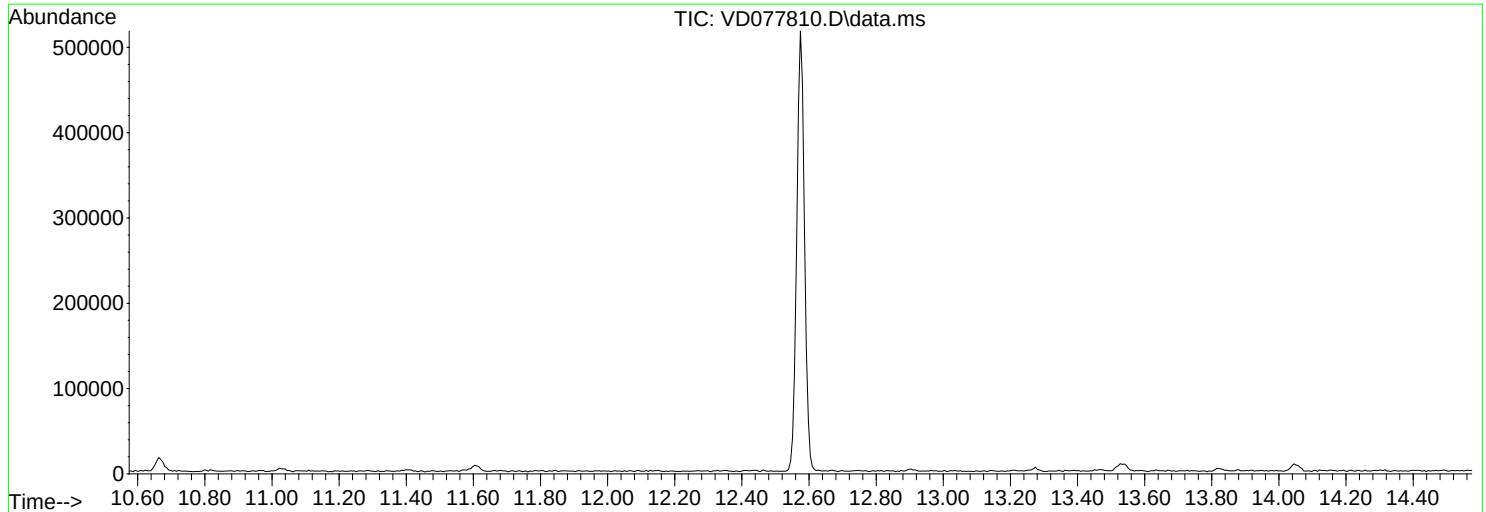

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	16996	PASS
75	95	30	60	53.9	45003	PASS
95	95	100	100	100.0	83443	PASS
96	95	5	9	6.4	5326	PASS
173	174	0.00	2	1.4	1122	PASS
174	95	50	100	93.2	77763	PASS
175	174	5	9	8.1	6321	PASS
176	174	95	101	96.3	74896	PASS
177	176	5	9	7.0	5257	PASS