


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD121318\
 Data File : VD060551.D
 Acq On : 13 Dec 2018 10:06
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
 Title : SW846 8260
 Last Update : Thu Dec 06 01:49:20 2018

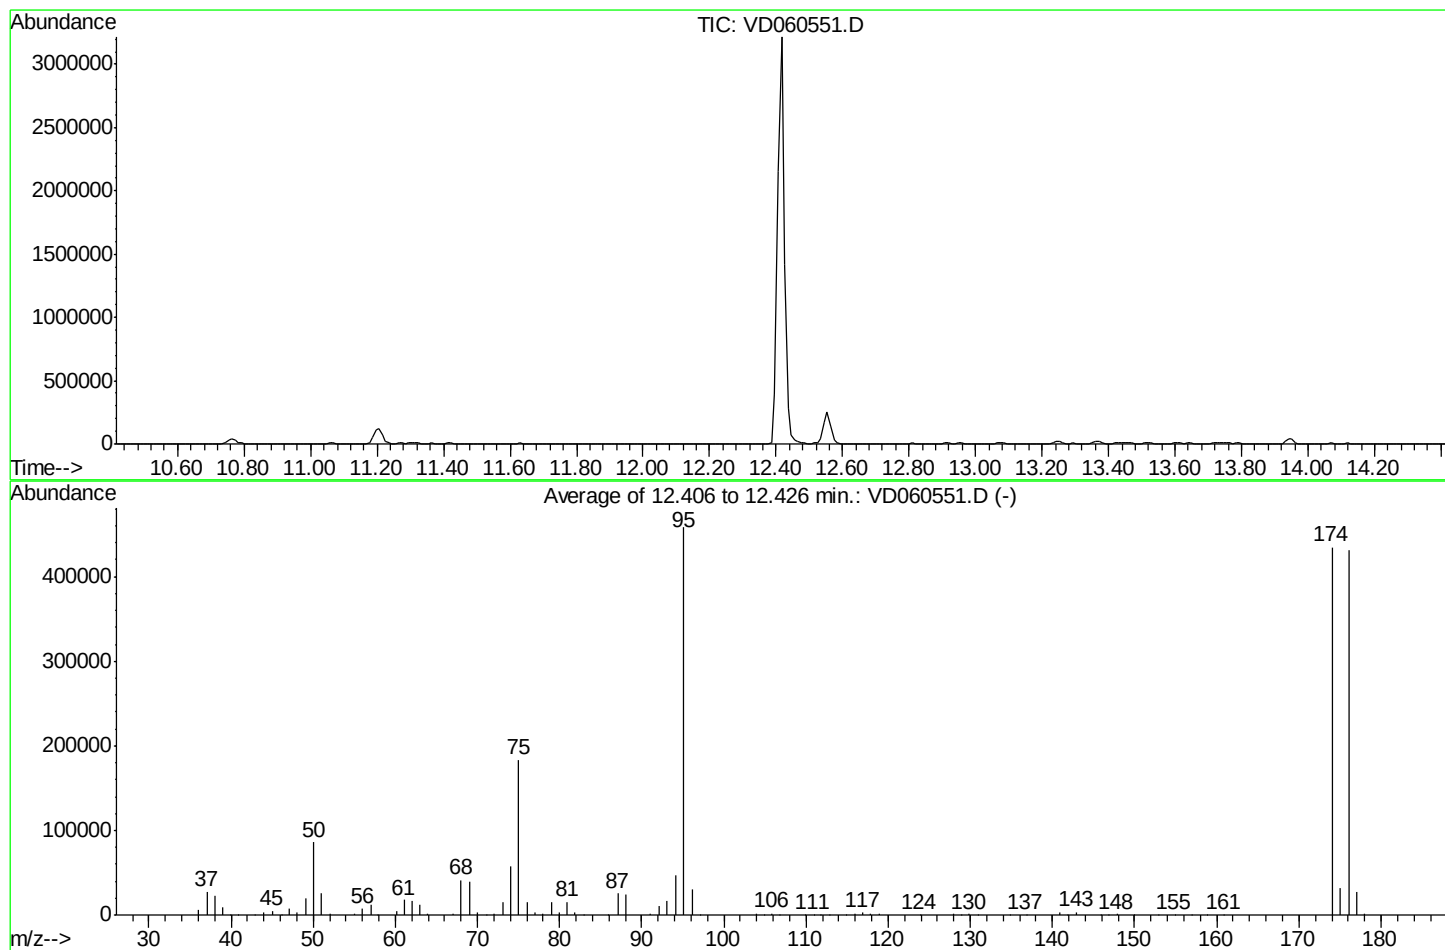

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1101

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	86032	PASS
75	95	30	60	40.0	183154	PASS
95	95	100	100	100.0	458304	PASS
96	95	5	9	6.7	30507	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.9	435072	PASS
175	174	5	9	7.4	32117	PASS
176	174	95	101	99.3	431914	PASS
177	176	5	9	6.4	27538	PASS