

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD121319\
 Data File : VD064512.D
 Acq On : 13 Dec 2019 17:48
 Operator : VA/SY
 Sample : K6267-02
 Misc : 2.20G/5.00ml/MSVOA D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 WO-4

Quant Time: Dec 14 00:38:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 29 07:18:03 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	411233	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	622472	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	574510	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	271394	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	149077	40.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	80.10%	
35) Dibromofluoromethane	7.92	113	180897	46.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.24%	
50) Toluene-d8	10.34	98	734695	49.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.46%	
62) 4-Bromofluorobenzene	12.64	95	240106	50.57	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.14%	
Target Compounds						
30) Chloroform	7.71	83	17712	2.490	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD121319\
Data File : VD064512.D
Acq On : 13 Dec 2019 17:48
Operator : VA/SY
Sample : K6267-02
Misc : 2.20G/5.00ml/MSVOA D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
WO-4

Quant Time: Dec 14 00:38:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Quant Title : SW846 8260
QLast Update : Fri Nov 29 07:18:03 2019
Response via : Initial Calibration

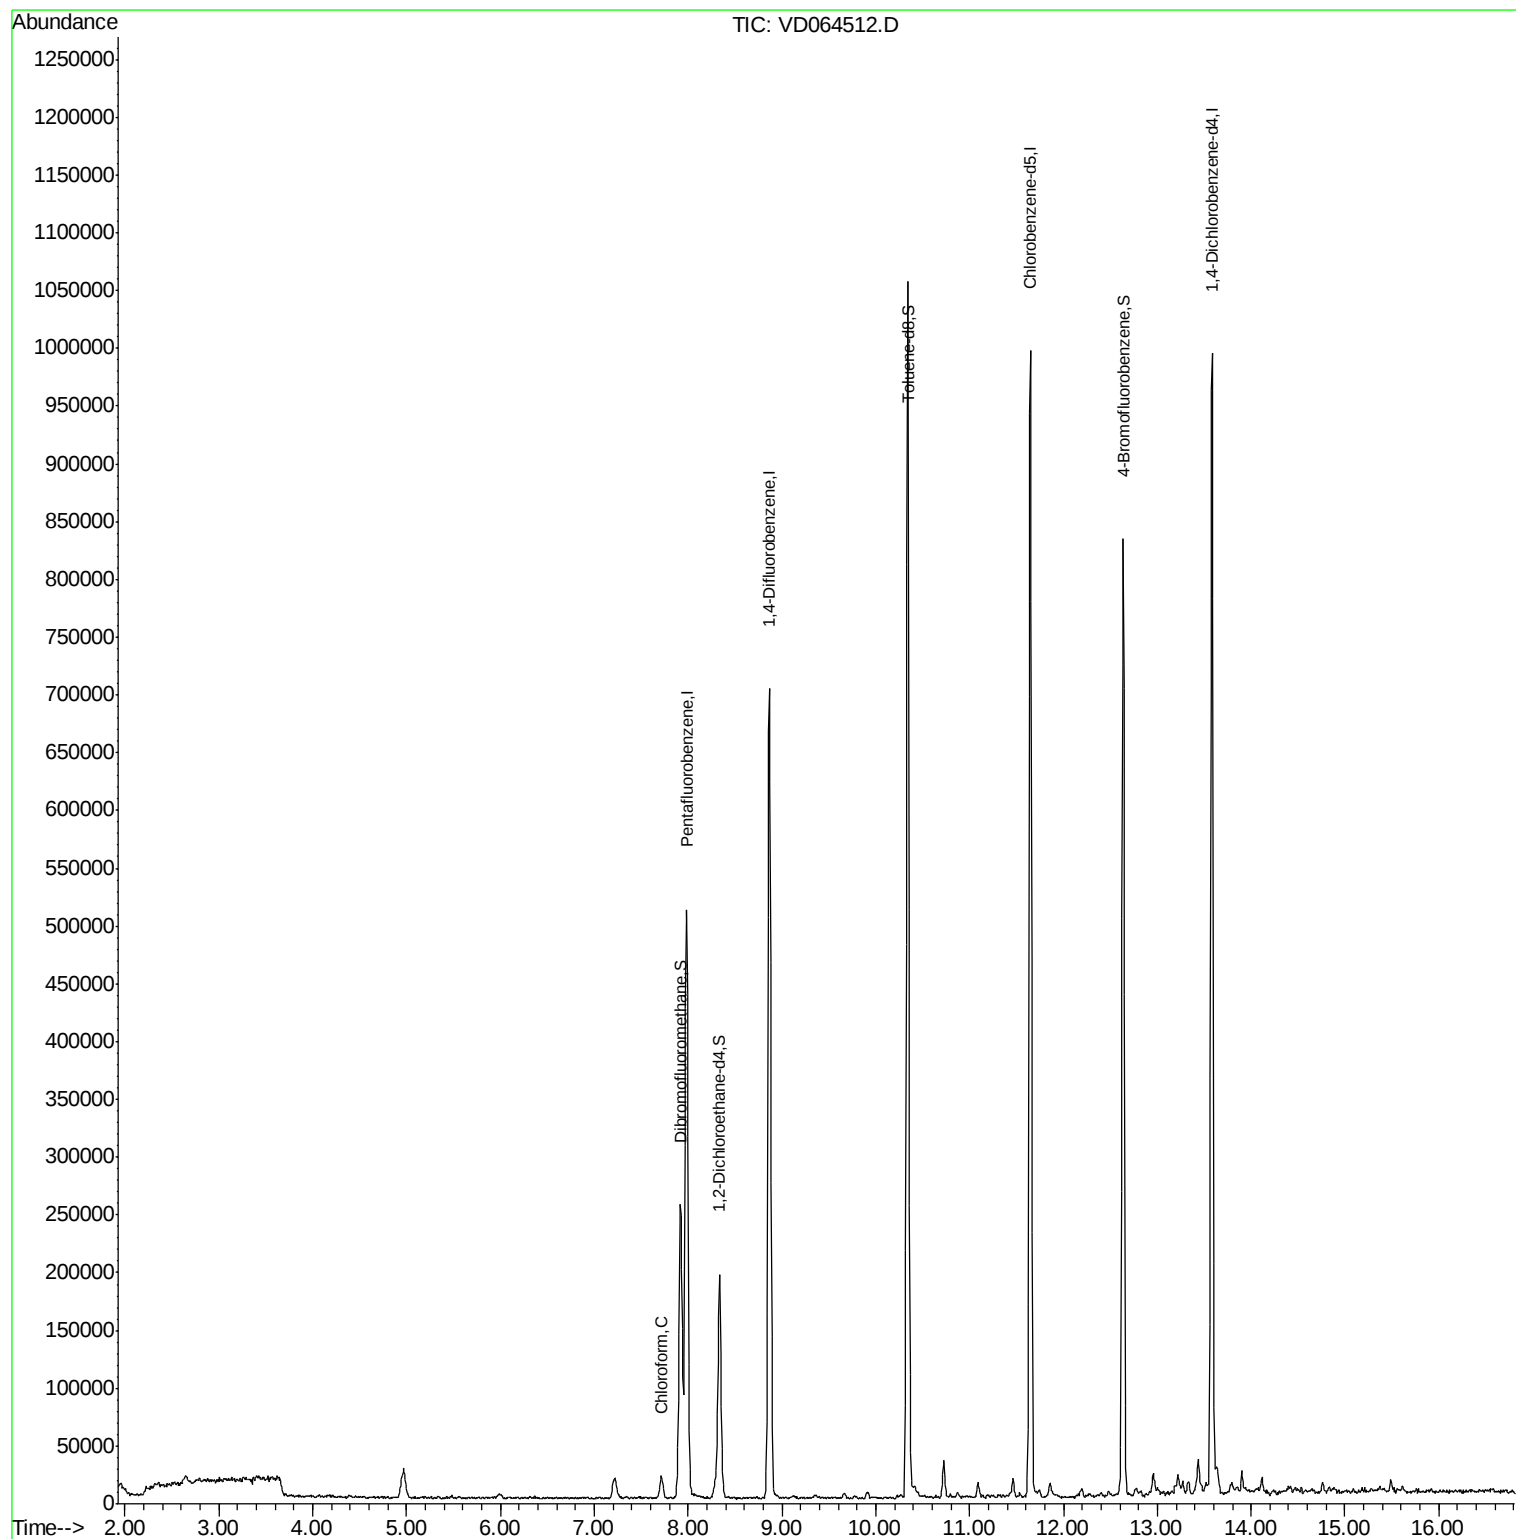

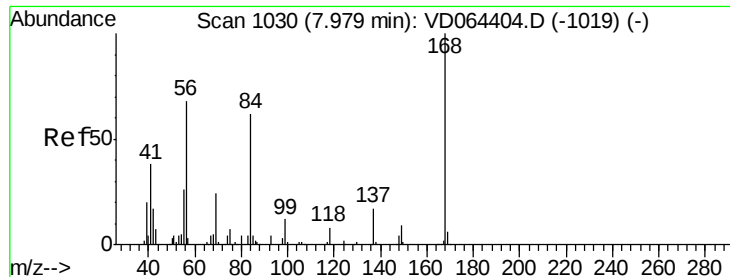

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.01 min

Lab File: VD064512.D

Acq: 13 Dec 2019 17:48

Instrument :

MSVOA_D

ClientSampleId :


WO-4

Tot Ion:168 Resp: 411233

Ion Ratio Lower Upper

168 100

99 50.7 40.7 61.1

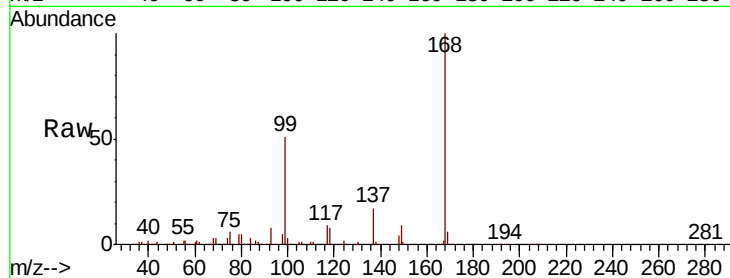

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

200000



150000

100000

50000

0

Time-->

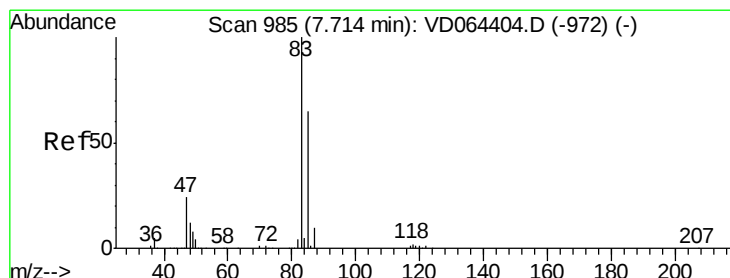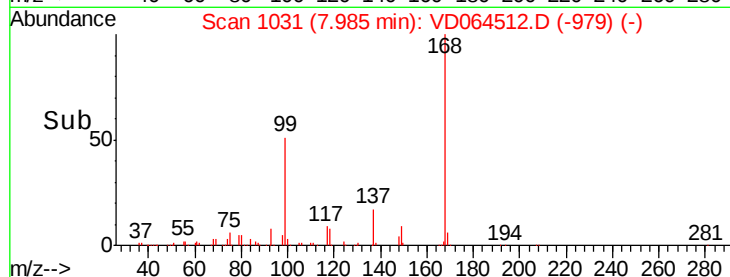

#30

Chloroform

Concen: 2.490 ug/l

RT: 7.71 min Scan# 985

Delta R.T. 0.00 min

Lab File: VD064512.D


Acq: 13 Dec 2019 17:48

Tgt Ion: 83 Resp: 17712

Ion Ratio Lower Upper

83 100

85 58.6 51.8 77.6

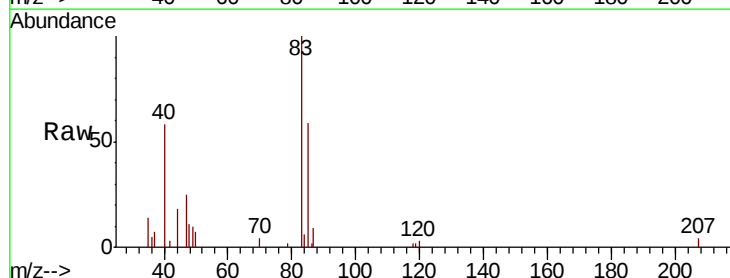

Abundance Ion 82.90 (82.60 to 83.60): VDC

Ion 84.90 (84.60 to 85.60): VDC

7.71

8000


6000


4000

2000

0

Time-->




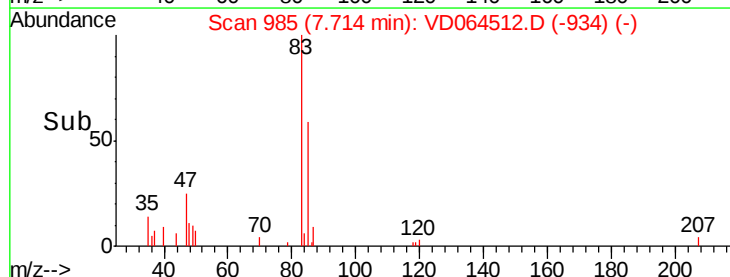


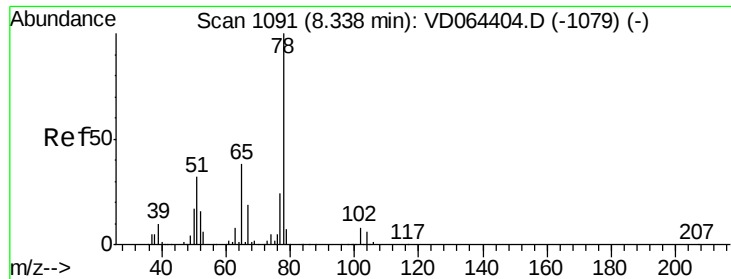

#33
 1,2-Dichloroethane-d4
 Concen: 40.050 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. -0.01 min
 Lab File: VD064512.D
 Acq: 13 Dec 2019 17:48




Instrument :
 MSVOA_D
 ClientSampleId :
 WO-4


Tot Ion: 65 Resp: 149077
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 102.0

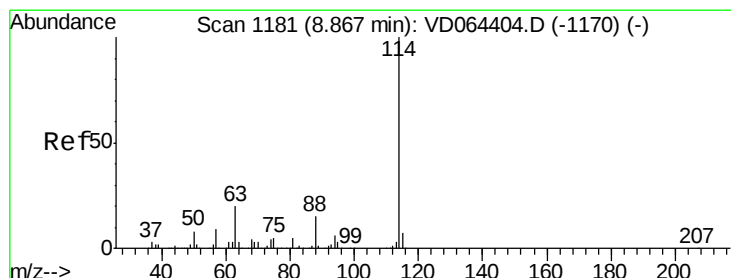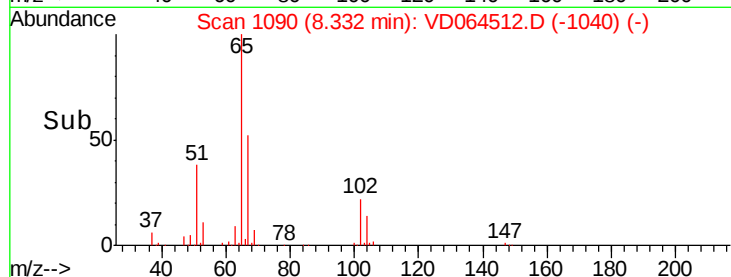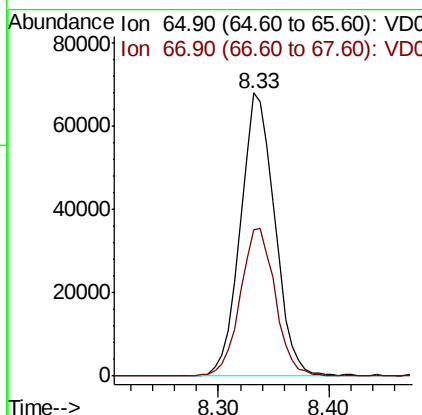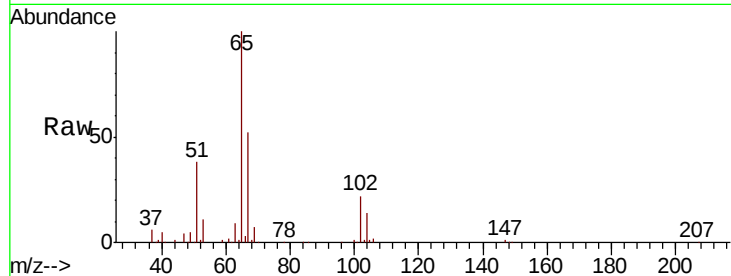

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD064512.D
 Acq: 13 Dec 2019 17:48

Tgt Ion: 114 Resp: 622472
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.0
 88 13.6 0.0 29.2


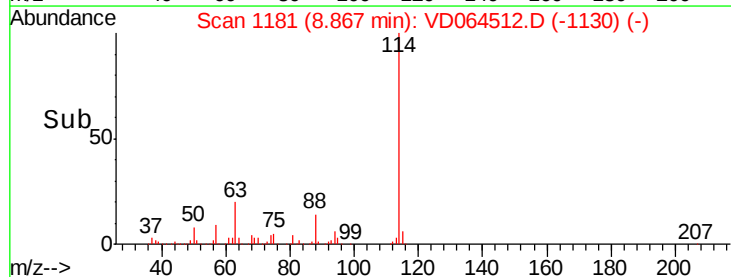
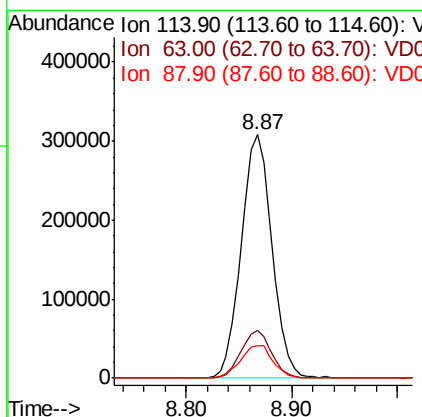
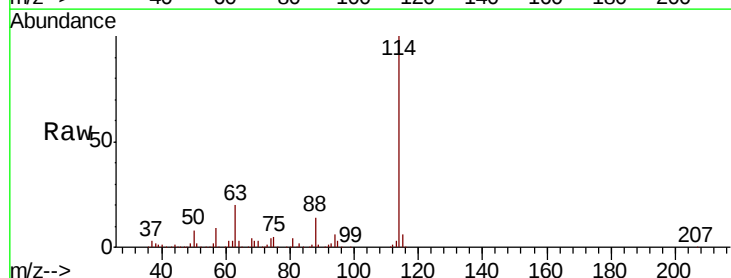


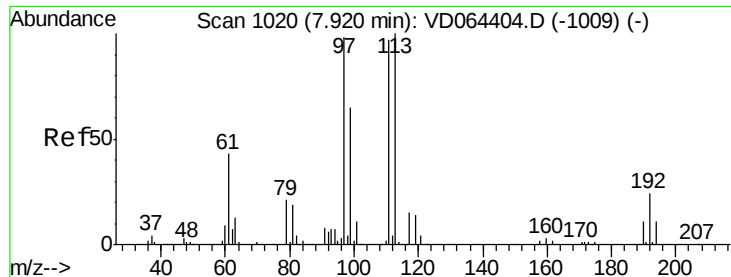

#35
 Dibromofluoromethane
 Concen: 46.125 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD064512.D
 Acq: 13 Dec 2019 17:48




Instrument :
 MSVOA_D
 ClientSampleID :
 WO-4


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.6	79.4	119.2
192	23.1	18.6	28.0

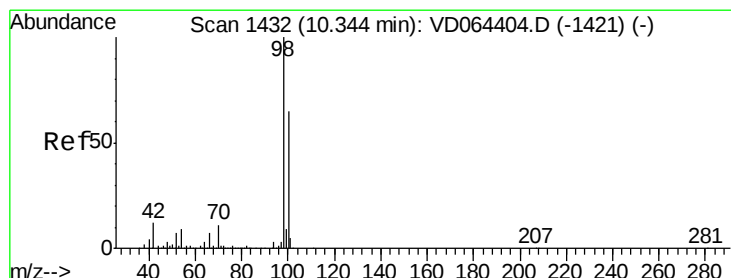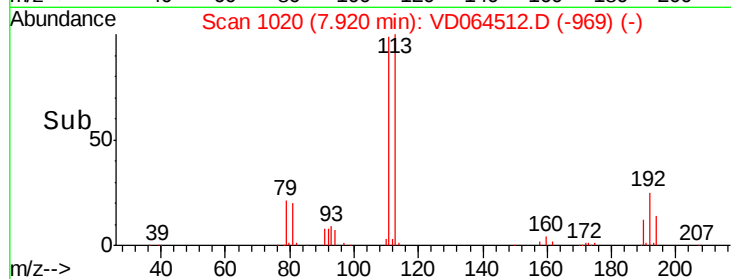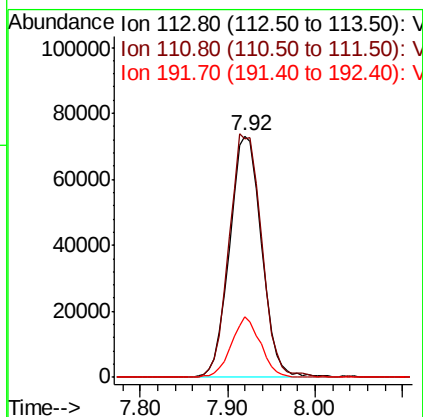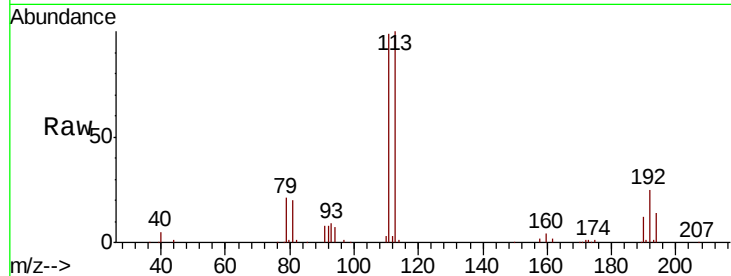

#50
 Toluene-d8
 Concen: 49.731 ug/l
 RT: 10.34 min Scan# 1432
 Delta R.T. 0.00 min
 Lab File: VD064512.D
 Acq: 13 Dec 2019 17:48

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.3	52.6	79.0


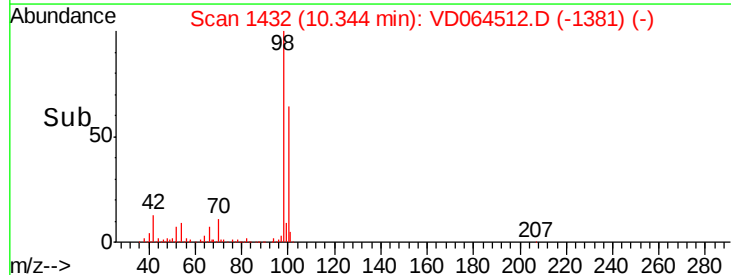
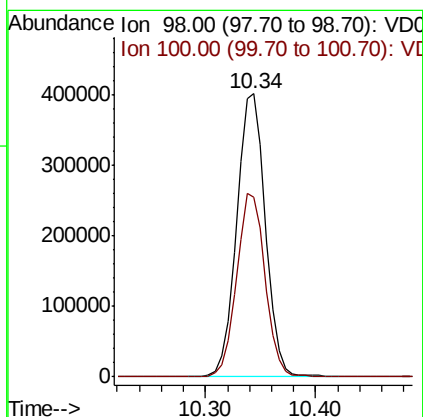
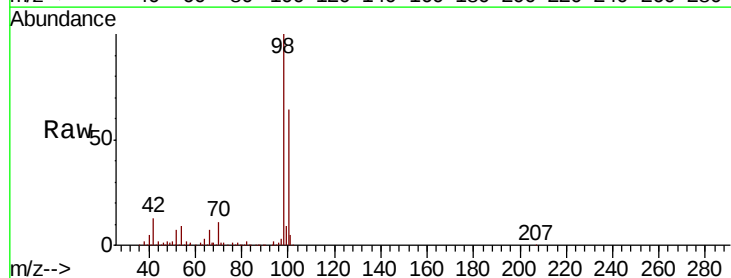


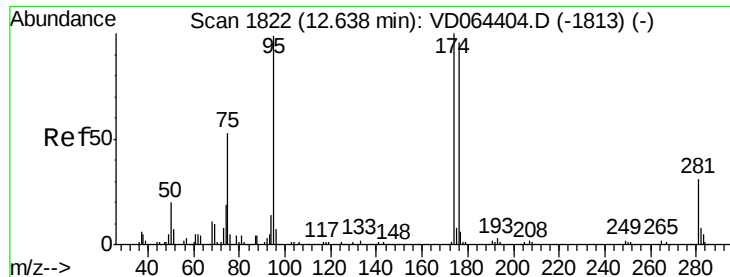

#62
4-Bromofluorobenzene
Concen: 50.573 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD064512.D
Acq: 13 Dec 2019 17:48




Instrument :
MSVOA_D
ClientSampled :
WO-4


Tot Ion: 95 Resp: 240106
Ion Ratio Lower Upper
95 100
174 96.2 0.0 197.2
176 93.5 0.0 189.6

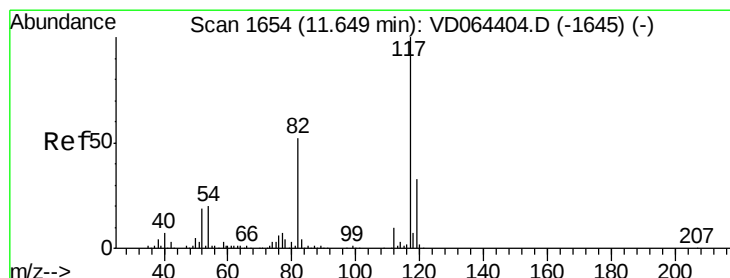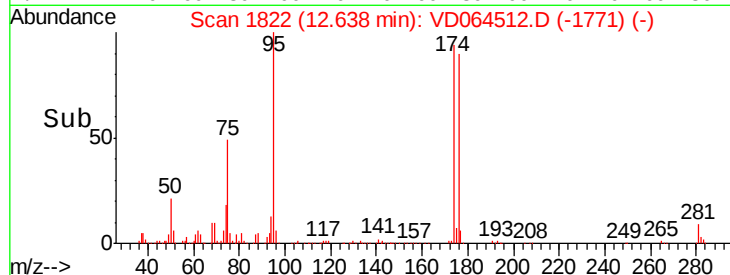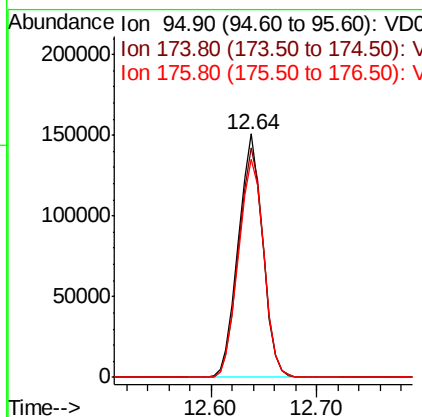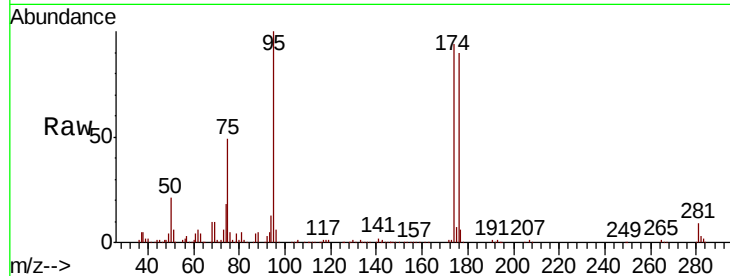

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD064512.D
Acq: 13 Dec 2019 17:48

Tgt Ion: 117 Resp: 574510
Ion Ratio Lower Upper
117 100
82 51.9 41.4 62.2
119 31.9 26.2 39.2

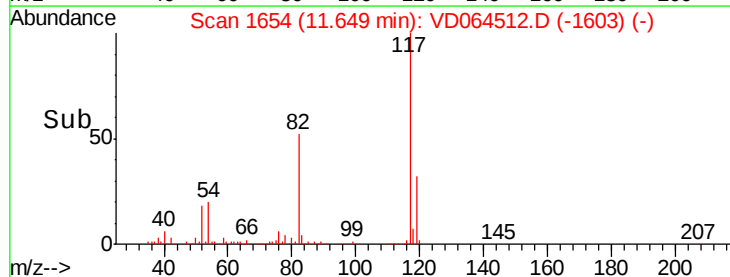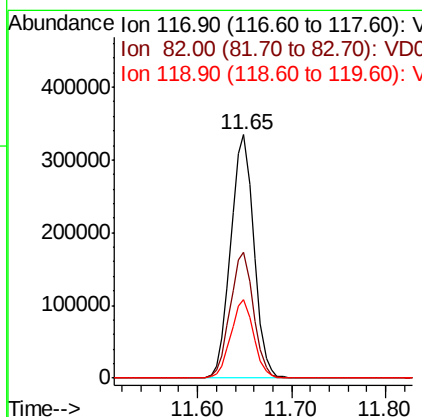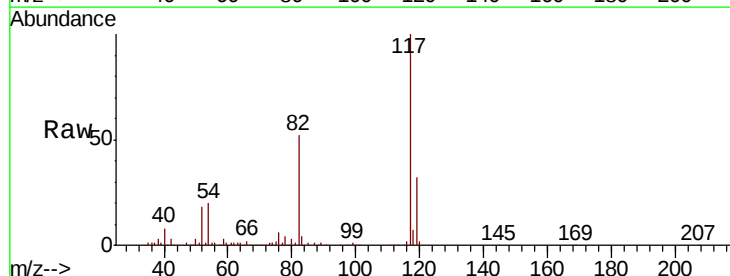

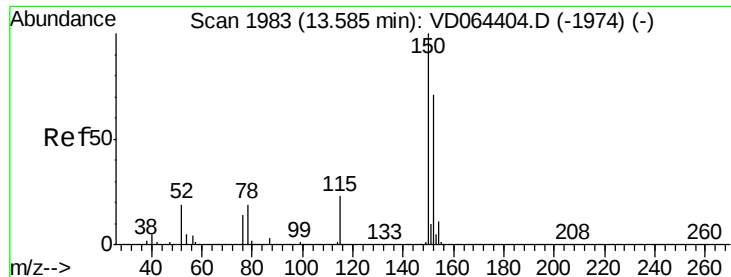

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.00 min

Lab File: VD064512.D

Acq: 13 Dec 2019 17:48

Instrument :

MSVOA_D

ClientSampleId :

WO-4


Tot Ion:152 Resp: 271394

Ion Ratio Lower Upper

152 100

115 56.2 26.7 80.1

150 158.5 0.0 347.2

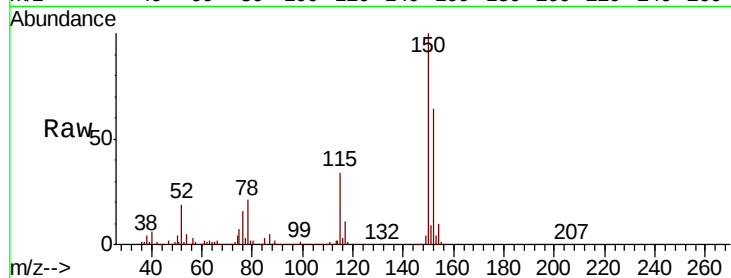

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

