

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121323\
 Data File : VD077853.D
 Acq On : 13 Dec 2023 11:10
 Operator : RP/MD
 Sample : VD1213SBL01
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1213SBL01

Quant Time: Dec 14 01:49:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 08 13:33:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	209503	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.781	114	366070	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.587	117	347178	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	157760	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	95545	38.703	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	77.400%
35) Dibromofluoromethane	7.810	113	108617	42.359	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	84.720%
50) Toluene-d8	10.269	98	467993	45.569	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	91.140%
62) 4-Bromofluorobenzene	12.575	95	132913	43.288	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	86.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121323\
Data File : VD077853.D
Acq On : 13 Dec 2023 11:10
Operator : RP/MD
Sample : VD1213SBL01
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1213SBL01

Quant Time: Dec 14 01:49:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Fri Dec 08 13:33:18 2023
Response via : Initial Calibration




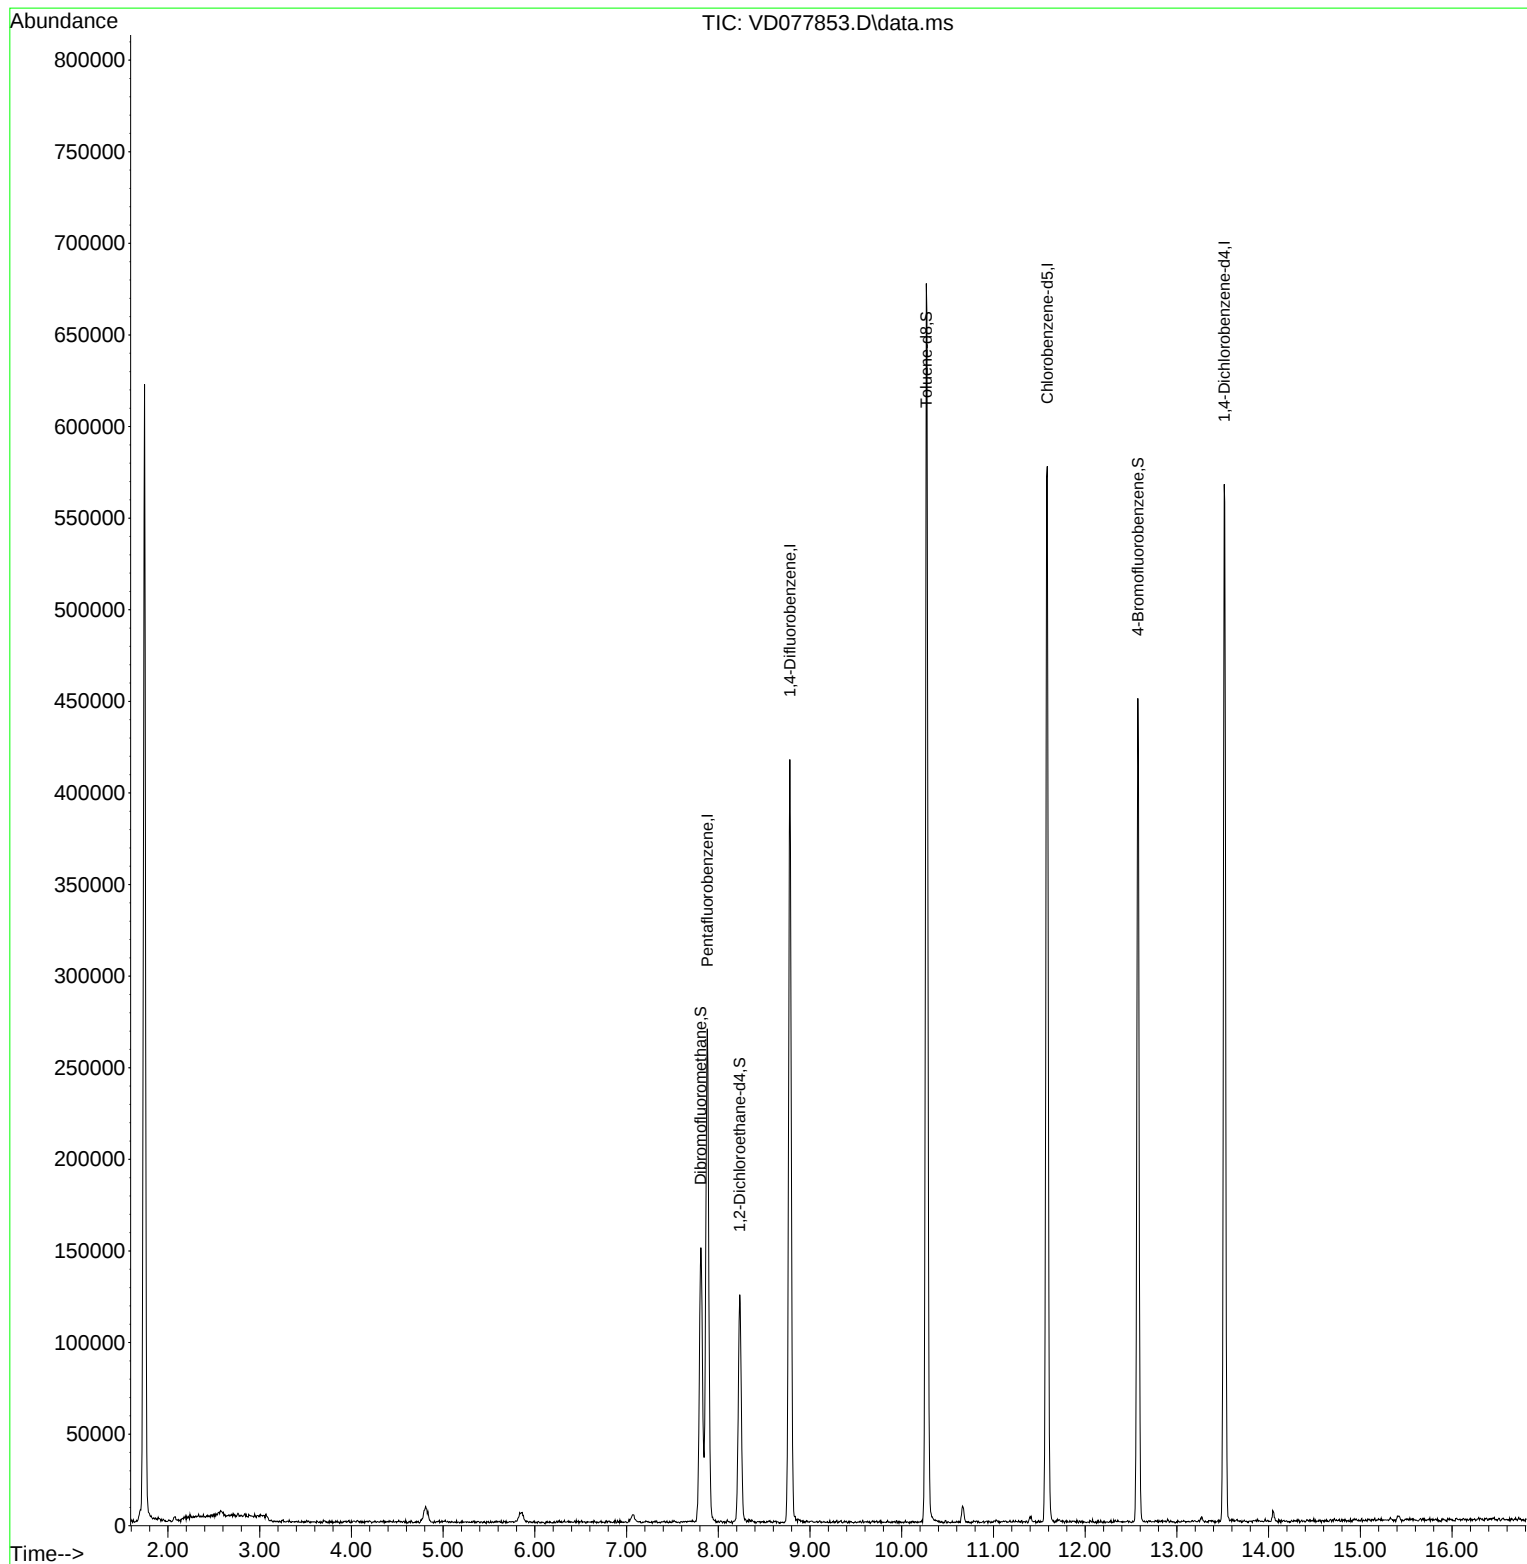


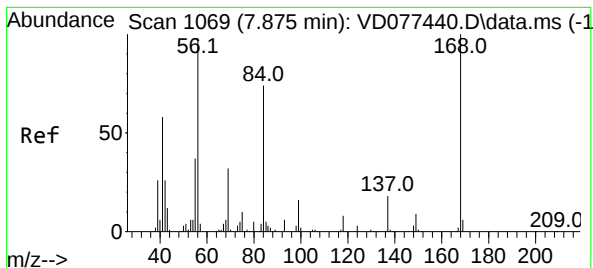

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10




Instrument :
MSVOA_D
ClientSampleId :
VD1213SBL01


Tgt Ion:168 Resp: 209503
Ion Ratio Lower Upper
168 100
99 55.8 36.7 55.1#

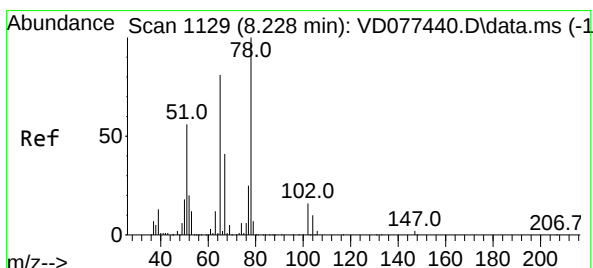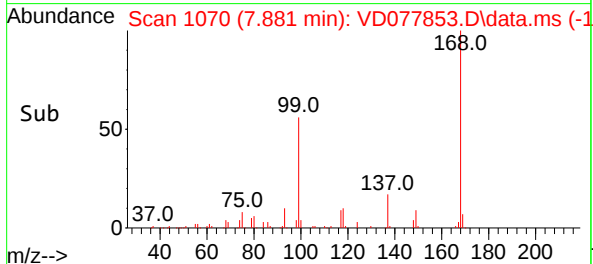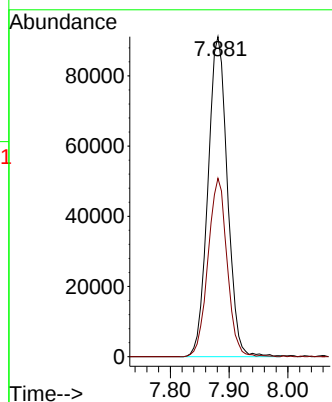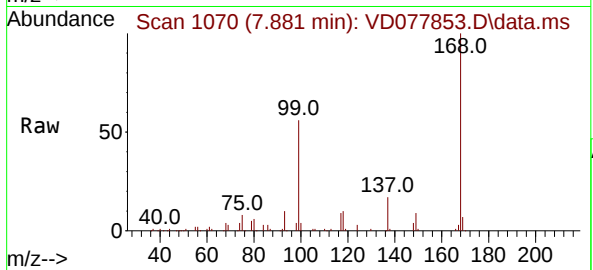

#33
1,2-Dichloroethane-d4
Concen: 38.703 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10

Tgt Ion: 65 Resp: 95545
Ion Ratio Lower Upper
65 100
67 54.5 0.0 115.0

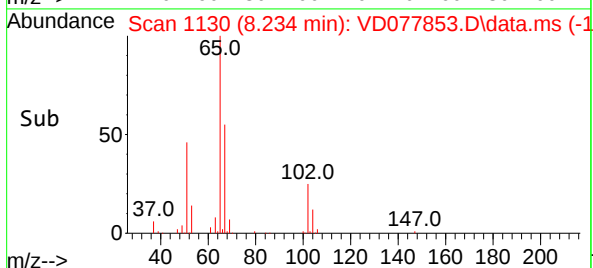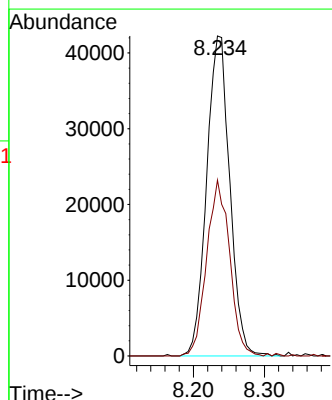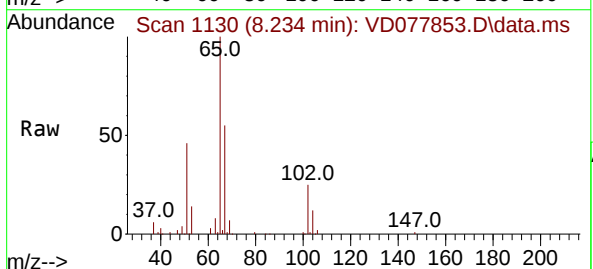

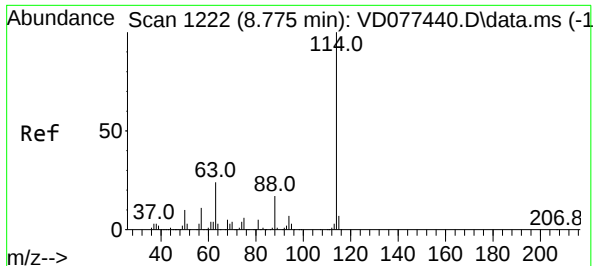

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD077853.D

Acq: 13 Dec 2023 11:10

Instrument :

MSVOA_D

ClientSampleId :

VD1213SBL01




Tgt Ion:114 Resp: 366070

Ion Ratio Lower Upper

114 100

63 19.0 0.0 33.4

88 13.9 0.0 26.2

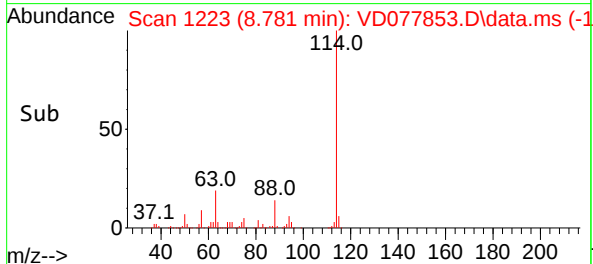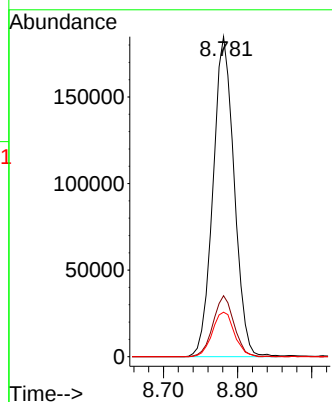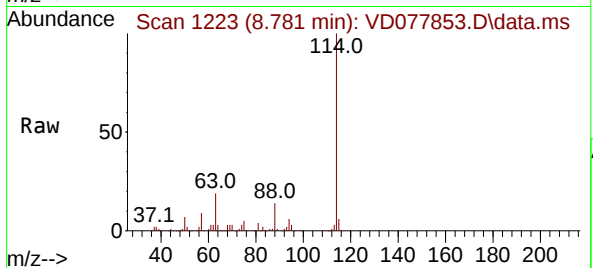

#35

Dibromofluoromethane

Concen: 42.359 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD077853.D

Acq: 13 Dec 2023 11:10




Tgt Ion:113 Resp: 108617

Ion Ratio Lower Upper

113 100

111 103.1 84.7 127.1

192 19.5 16.8 25.2


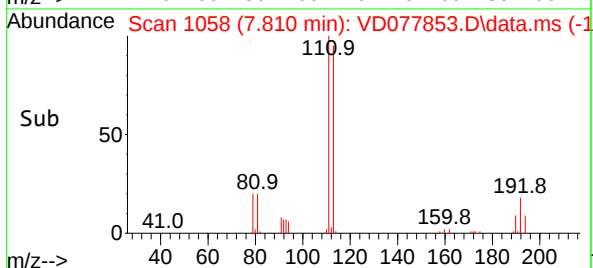
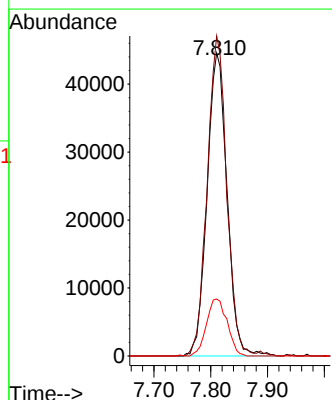
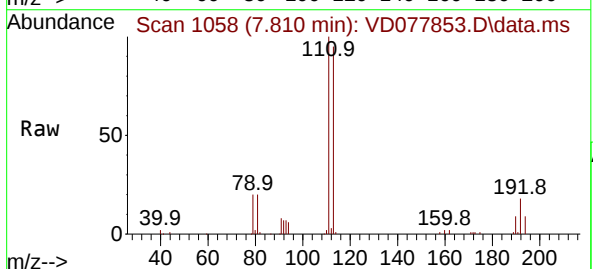




#50
Toluene-d8
Concen: 45.569 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10




Instrument :
MSVOA_D
ClientSampleId :
VD1213SBL01


Tgt Ion: 98 Resp: 467993
Ion Ratio Lower Upper
98 100
100 64.0 50.3 75.5

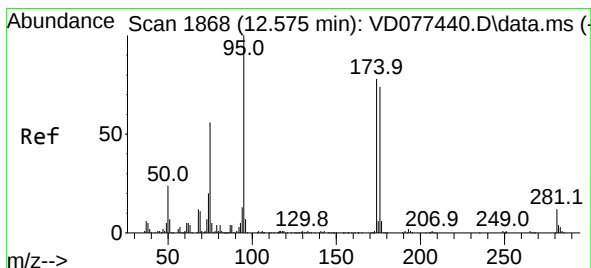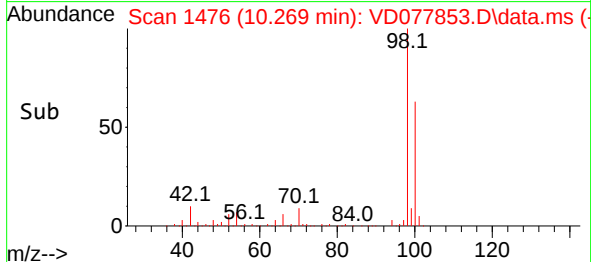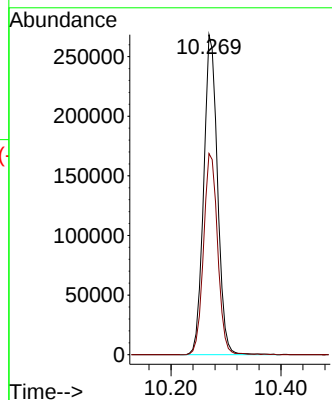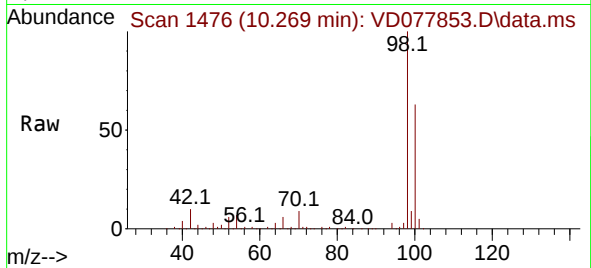

#62
4-Bromofluorobenzene
Concen: 43.288 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10

Tgt Ion: 95 Resp: 132913
Ion Ratio Lower Upper
95 100
174 91.2 0.0 201.8
176 87.7 0.0 191.8


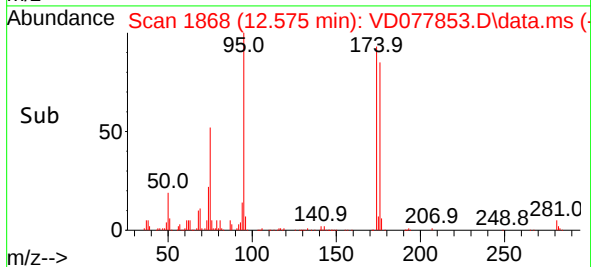
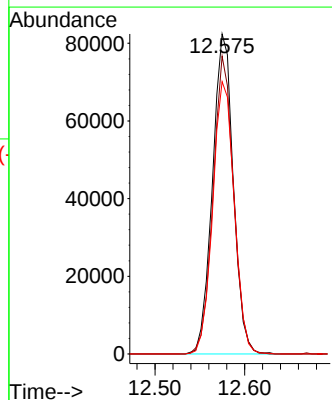
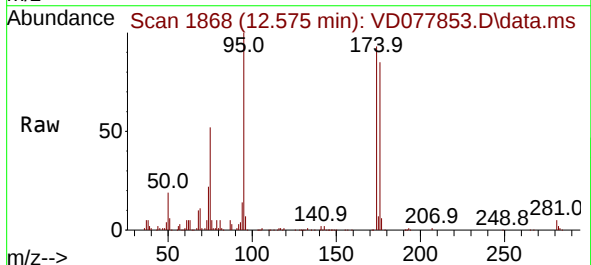


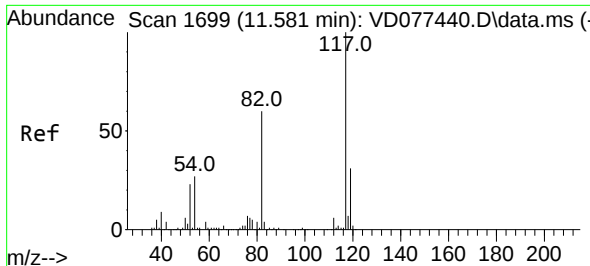

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.587 min Scan# 11
Delta R.T. 0.006 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10

Instrument :
MSVOA_D
ClientSampleId :
VD1213SBL01

Tgt Ion:117 Resp: 347178
Ion Ratio Lower Upper
117 100
82 53.2 38.3 57.5
119 31.2 25.0 37.4

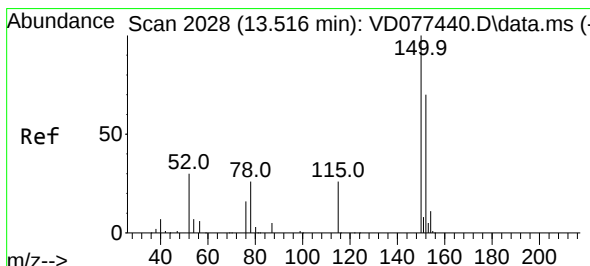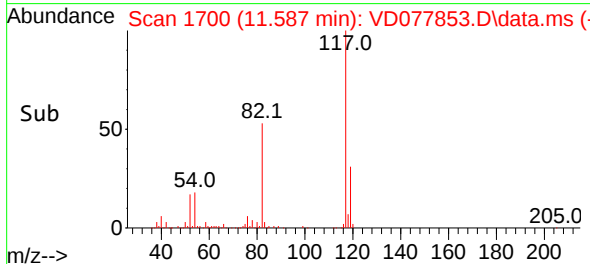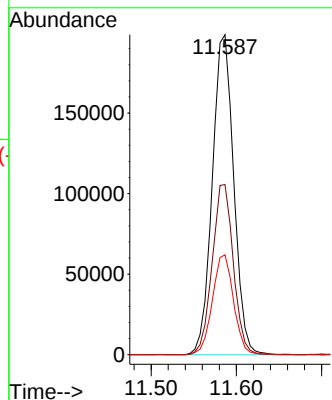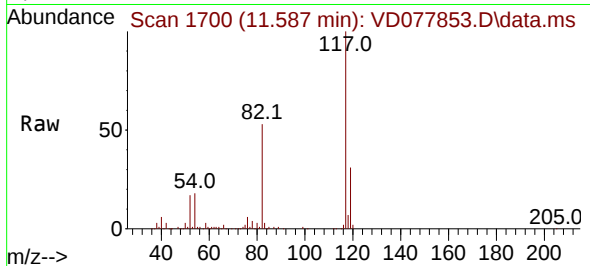

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD077853.D
Acq: 13 Dec 2023 11:10

Tgt Ion:152 Resp: 157760
Ion Ratio Lower Upper
152 100
115 56.3 27.1 81.3
150 155.2 0.0 353.6

