
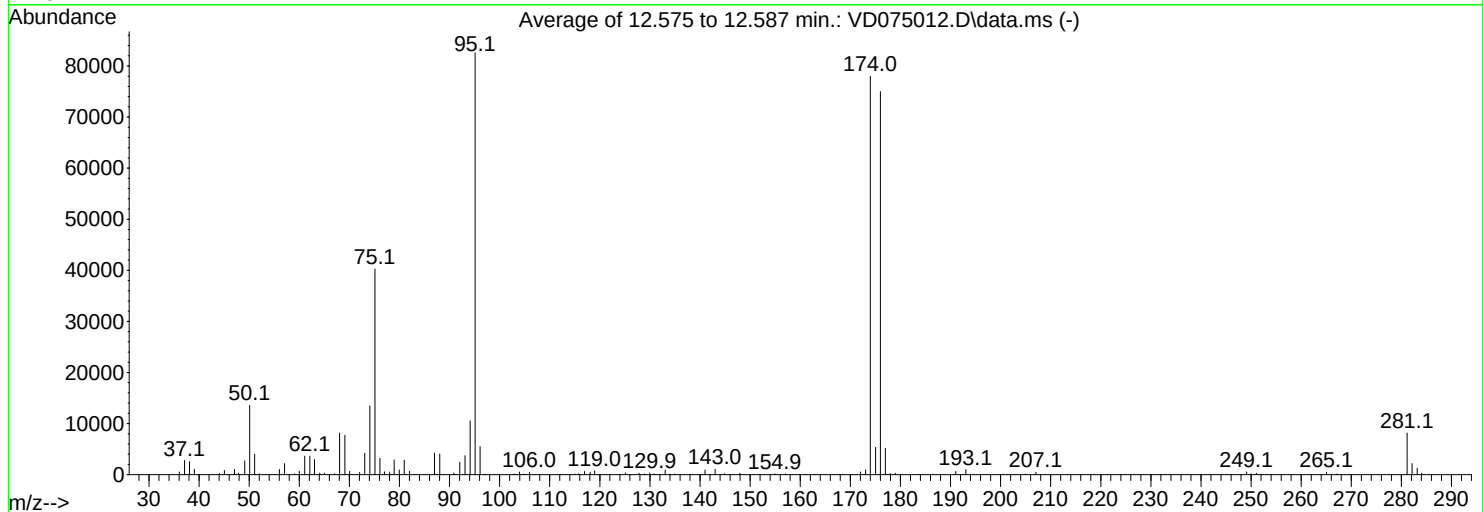


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121422\
 Data File : VD075012.D
 Acq On : 14 Dec 2022 09:31
 Operator : KP/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D121422S.M
 Title : SW846 8260
 Last Update : Thu Dec 15 03:27:53 2022

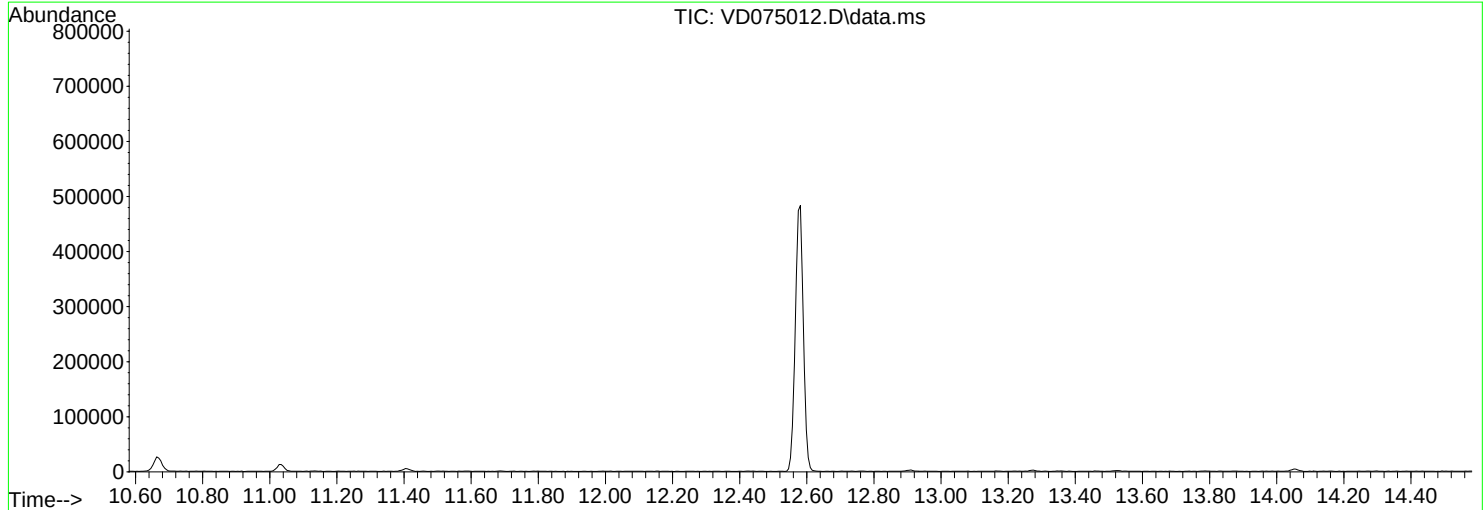

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	13570	PASS
75	95	30	60	48.8	40264	PASS
95	95	100	100	100.0	82573	PASS
96	95	5	9	6.7	5500	PASS
173	174	0.00	2	1.2	907	PASS
174	95	50	100	94.5	78011	PASS
175	174	5	9	6.9	5374	PASS
176	174	95	101	96.1	74976	PASS
177	176	5	9	6.9	5146	PASS