




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121423\
 Data File : VD077875.D
 Acq On : 14 Dec 2023 11:37
 Operator : RP/MD
 Sample : 05788-06
 Misc : 2.62G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCLS0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/15/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 15 07:12:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 06 00:24:24 2023
 Response via : Initial Calibration

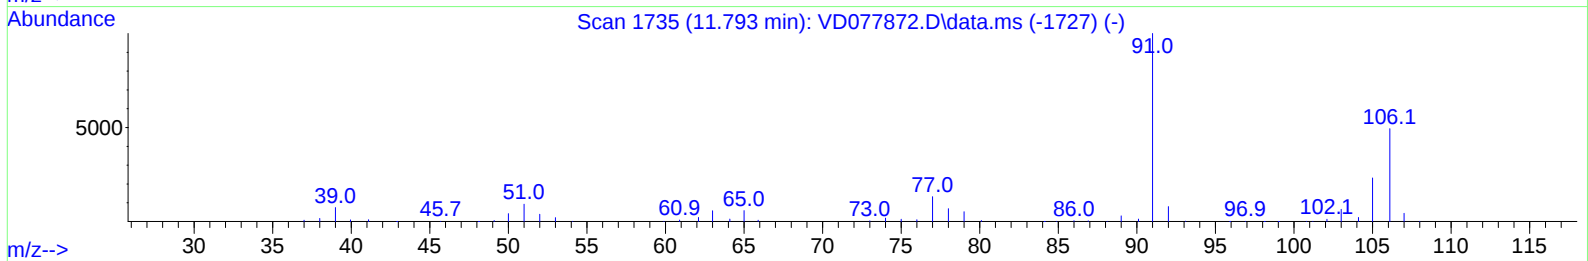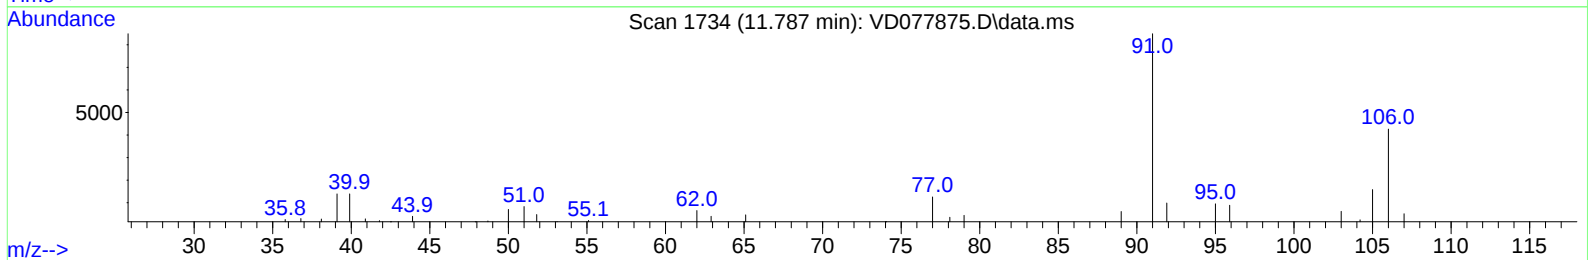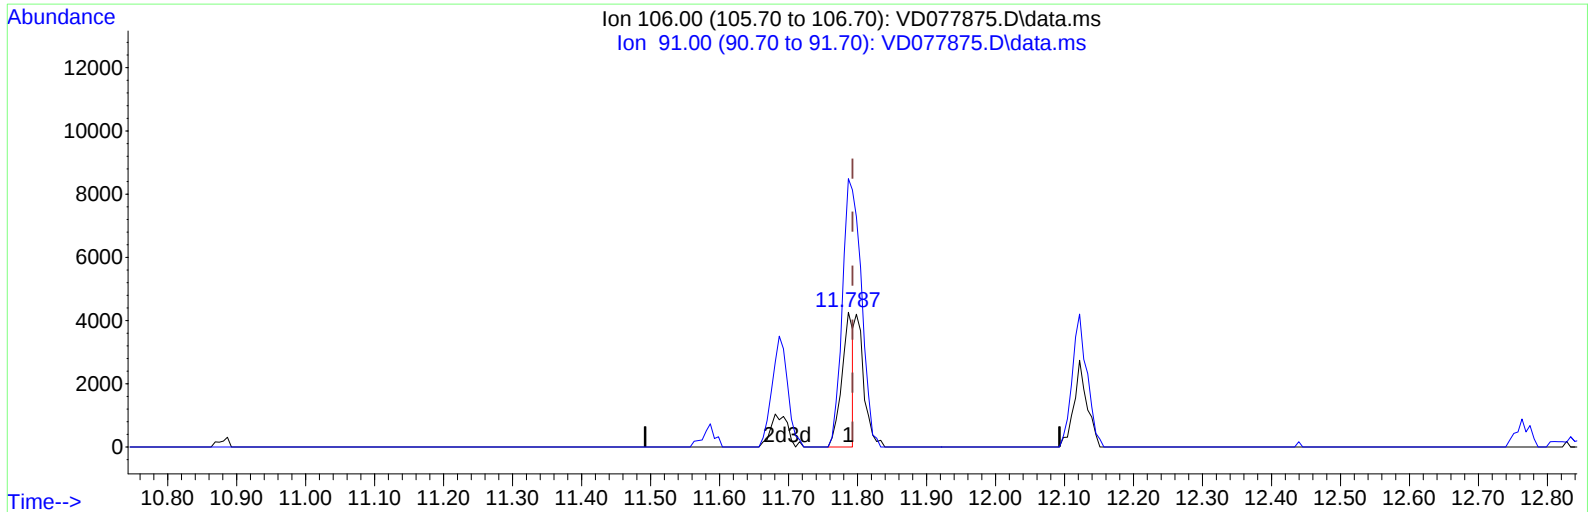

TIC: VD077875.D\data.ms

(53) m,p-Xylene (T)

11.787min (-0.006) 0.46 ug/L

response 4868

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	201.20	199.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121423\
 Data File : VD077875.D
 Acq On : 14 Dec 2023 11:37
 Operator : RP/MD
 Sample : 05788-06
 Misc : 2.62G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCLS0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/15/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 15 07:12:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 06 00:24:24 2023
 Response via : Initial Calibration

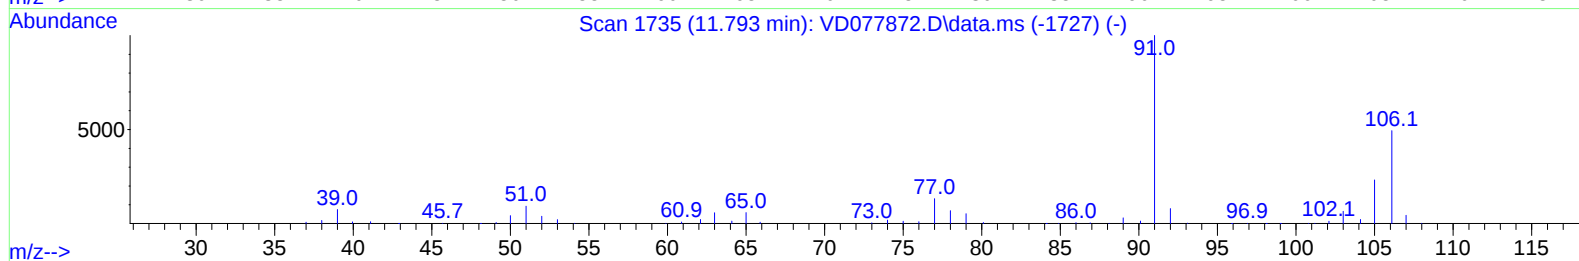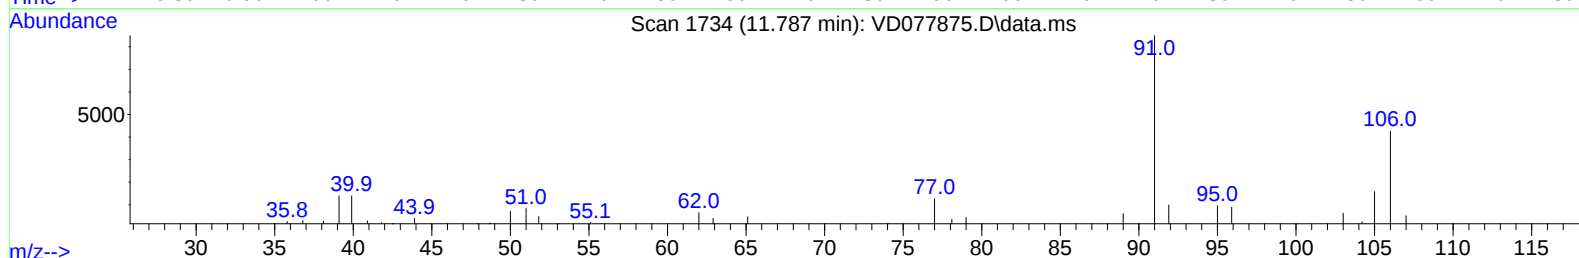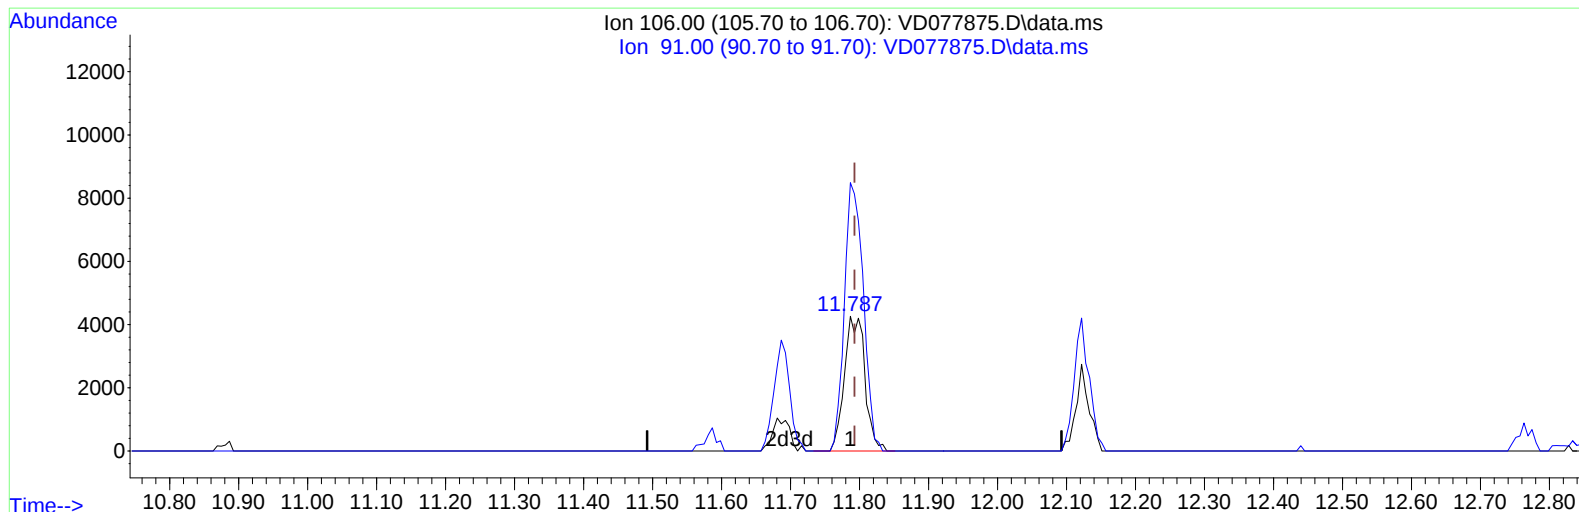

TIC: VD077875.D\data.ms

(53) m,p-Xylene (T)

11.787min (-0.006) 0.83 ug/L m

response 8791

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	201.20	199.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121423\
 Data File : VD077875.D
 Acq On : 14 Dec 2023 11:37
 Operator : RP/MD
 Sample : 05788-06
 Misc : 2.62G/10ml/MSVOA_D/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCLS0

Manual IntegrationsAPPROVED

Quant Time: Dec 15 07:12:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 06 00:24:24 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/15/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	414513	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117	365548	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	150441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.287	65	148264	13.116	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.480%
7) Chloroethane-d5	2.811	69	134474	14.925	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.680%
11) 1,1-Dichloroethene-d2	3.934	65	38278	13.060	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.240%
21) 2-Butanone-d5	6.993	46	30009	21.005	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	42.020%
24) Chloroform-d	7.575	84	170154	15.231	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	60.920%
26) 1,2-Dichloroethane-d4	8.234	65	75096	13.267	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	53.080%#
32) Benzene-d6	8.204	84	351680	15.974	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	63.880%
36) 1,2-Dichloropropane-d6	9.210	67	103378	15.390	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	61.560%#
41) Toluene-d8	10.269	98	318654	15.725	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	62.880%
43) trans-1,3-Dichloroprop...	10.528	79	39001	13.130	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.520%
47) 2-Hexanone-d5	10.881	63	26007	22.468	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	44.940%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	58691	12.091	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	48.360%
66) 1,2-Dichlorobenzene-d4	13.816	152	80238	14.909	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	59.640%#
Target Compounds						
					Qvalue	
13) Acetone	4.022	43	109967	60.076	ug/L	98
16) Methylene chloride	4.805	84	9077	1.233	ug/L	93
22) 2-Butanone	7.087	43	13979	6.785	ug/L #	76
42) Toluene	10.334	91	32209	1.275	ug/L	85
53) m,p-Xylene	11.787	106	8791m	0.830	ug/L	
54) o-Xylene	12.122	106	3617	0.357	ug/L	60
65) 1,4-Dichlorobenzene	13.539	146	4932	0.489	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121423\
Data File : VD077875.D
Acq On : 14 Dec 2023 11:37
Operator : RP/MD
Sample : 05788-06
Misc : 2.62G/10ml/MSVOA_D/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCLS0

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/15/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 15 07:12:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 06 00:24:24 2023
Response via : Initial Calibration

