

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121521\
 Data File : VD071344.D
 Acq On : 15 Dec 2021 15:56
 Operator : VA/SY
 Sample : M5083-01
 Misc : 6.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BB1

Quant Time: Dec 16 04:29:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 29 17:54:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	320708	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	543134	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	616884	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	292912	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	155174	41.235	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	82.480%
35) Dibromofluoromethane	7.914	113	165292	47.791	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	95.580%
50) Toluene-d8	10.338	98	699694	53.161	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	106.320%
62) 4-Bromofluorobenzene	12.620	95	312120	68.412	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	136.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121521\
Data File : VD071344.D
Acq On : 15 Dec 2021 15:56
Operator : VA/SY
Sample : M5083-01
Misc : 6.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BB1

Quant Time: Dec 16 04:29:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 29 17:54:09 2021
Response via : Initial Calibration




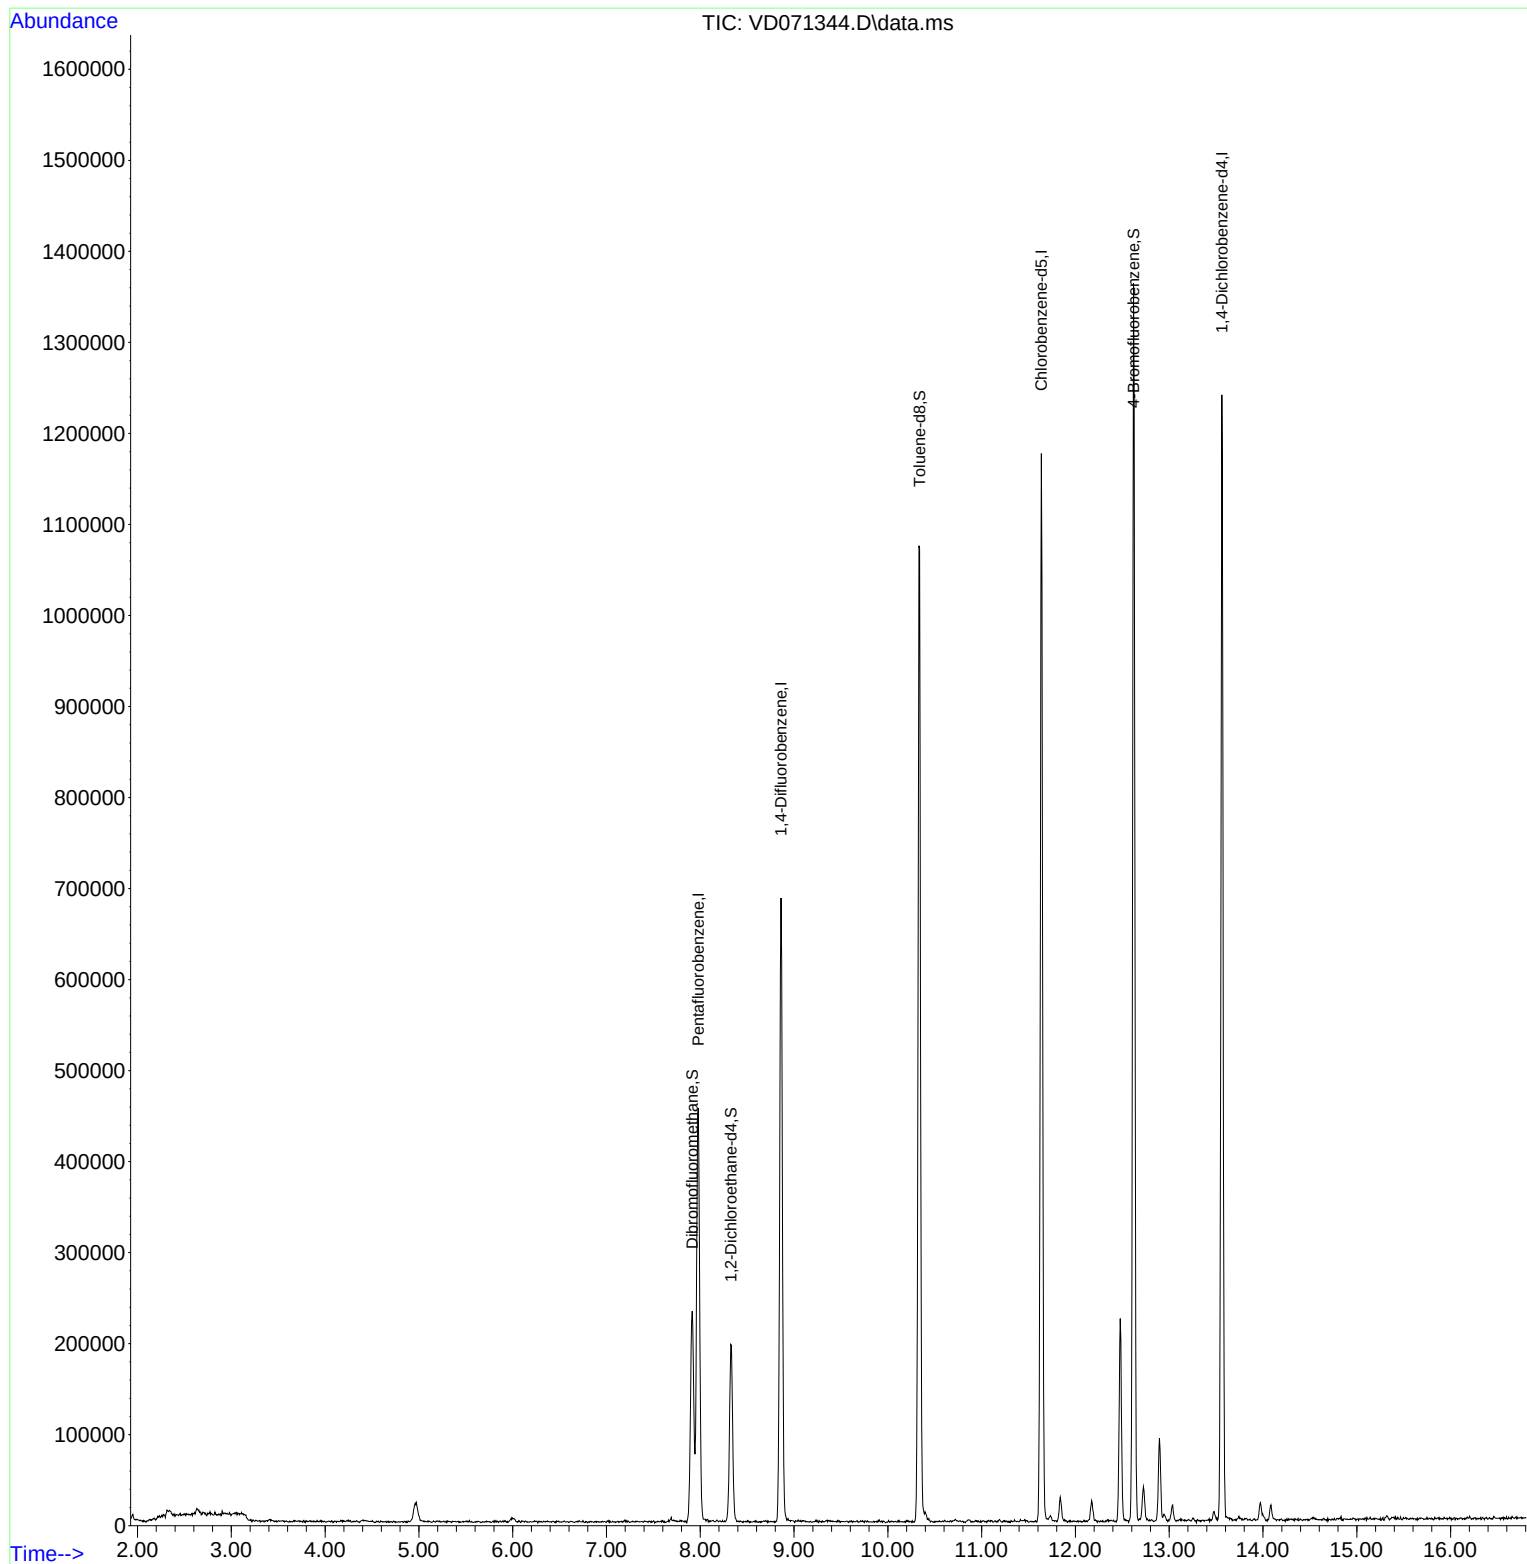


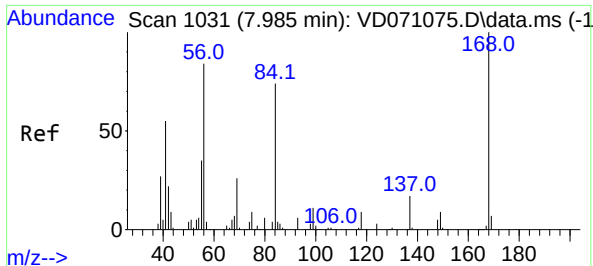

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1031
Delta R.T. -0.006 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56




Instrument :
MSVOA_D
ClientSampleId :
BB1


Tgt Ion:168 Resp: 320708
Ion Ratio Lower Upper
168 100
99 61.2 46.6 69.8

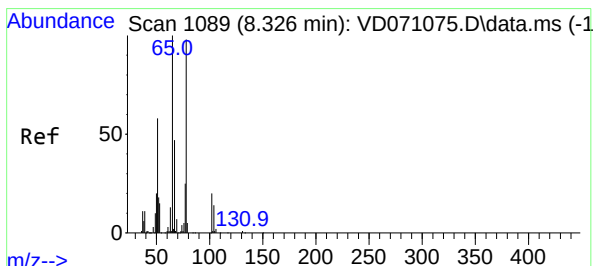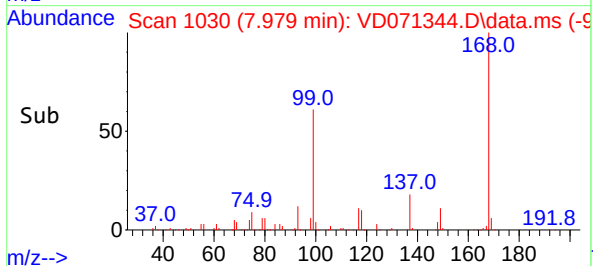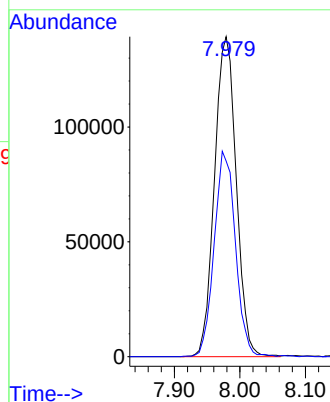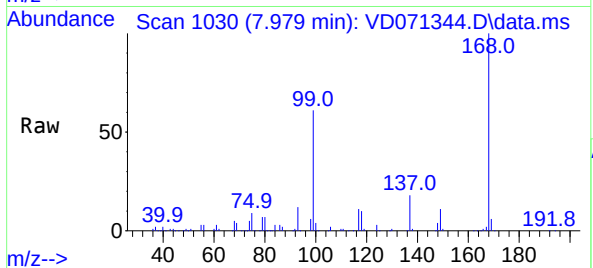

#33
1,2-Dichloroethane-d4
Concen: 41.235 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56

Tgt Ion: 65 Resp: 155174
Ion Ratio Lower Upper
65 100
67 50.7 0.0 112.2


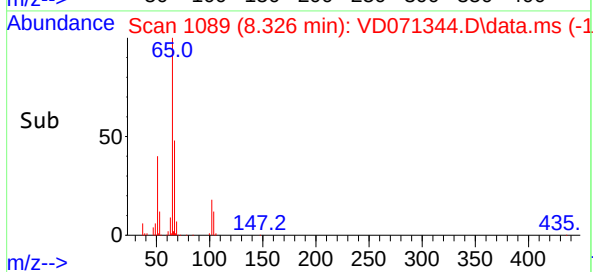
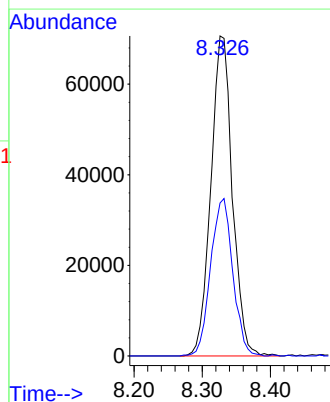
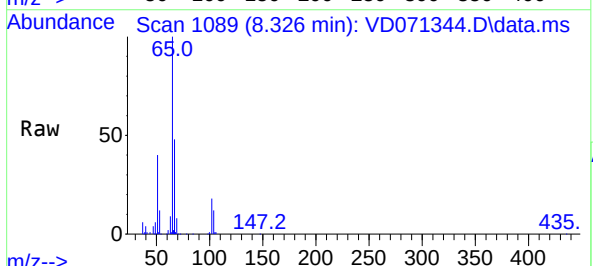


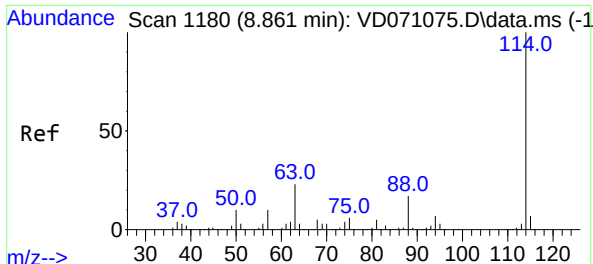

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56




Instrument :
MSVOA_D
ClientSampleId :
BB1


Tgt Ion:114 Resp: 543134
Ion Ratio Lower Upper
114 100
63 23.7 0.0 41.8
88 15.7 0.0 32.8

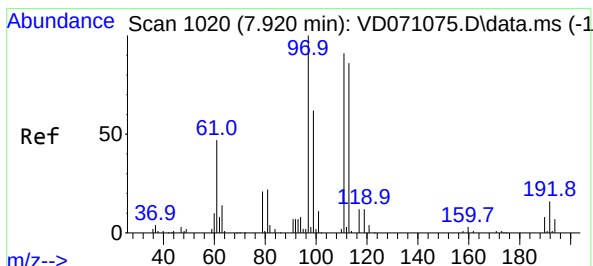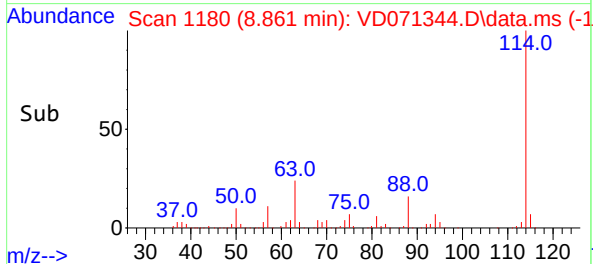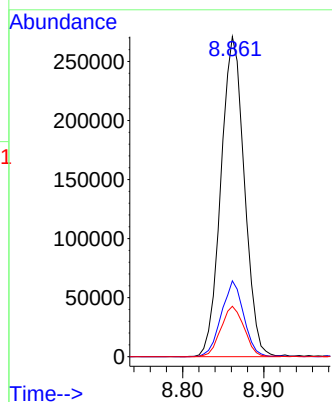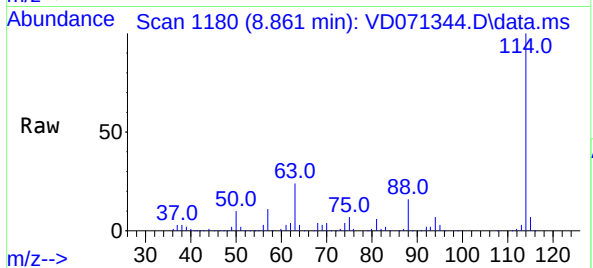

#35
Dibromofluoromethane
Concen: 47.791 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56

Tgt Ion:113 Resp: 165292
Ion Ratio Lower Upper
113 100
111 103.7 82.0 123.0
192 17.9 15.2 22.8


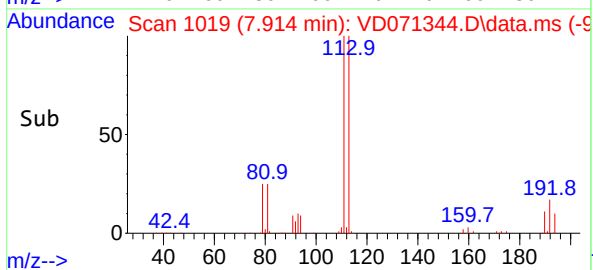
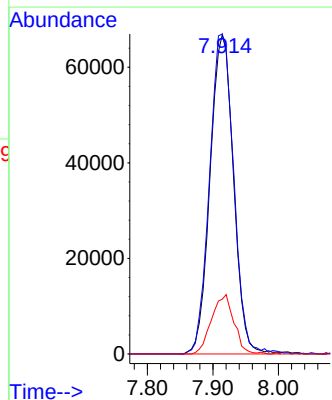
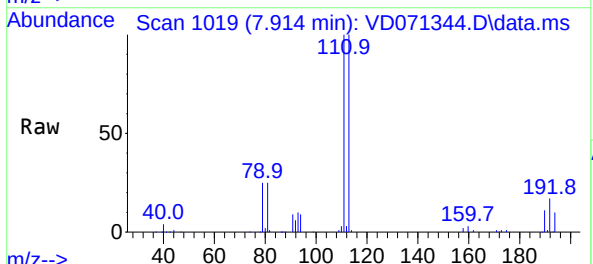


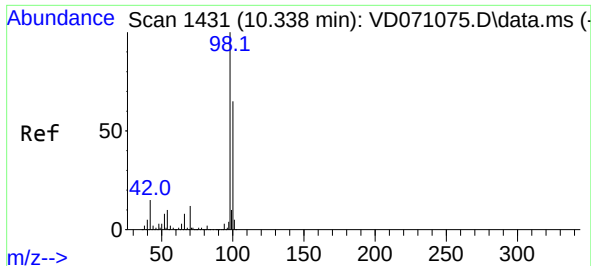

#50
Toluene-d8
Concen: 53.161 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56




Instrument :
MSVOA_D
ClientSampleId :
BB1


Tgt Ion: 98 Resp: 699694
Ion Ratio Lower Upper
98 100
100 65.6 51.8 77.6

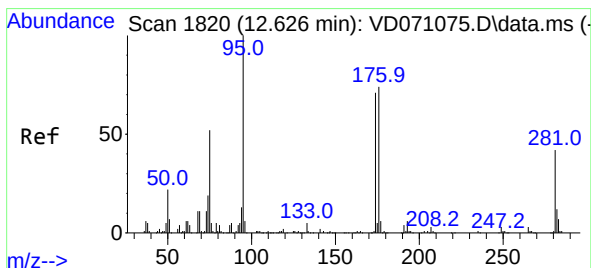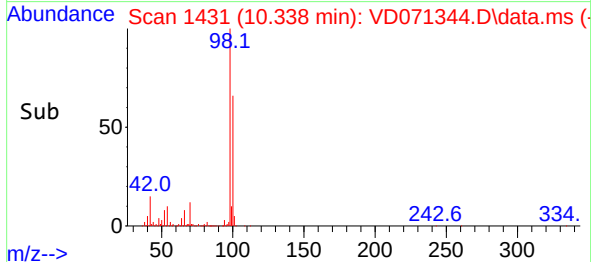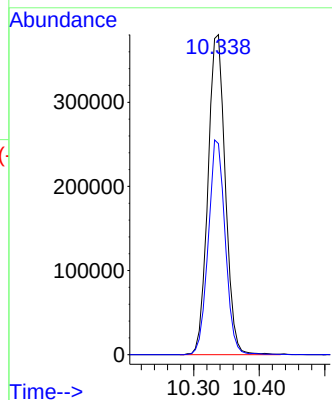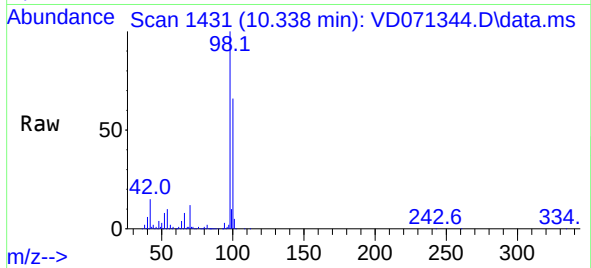

#62
4-Bromofluorobenzene
Concen: 68.412 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.006 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56

Tgt Ion: 95 Resp: 312120
Ion Ratio Lower Upper
95 100
174 74.6 0.0 159.4
176 72.2 0.0 154.0


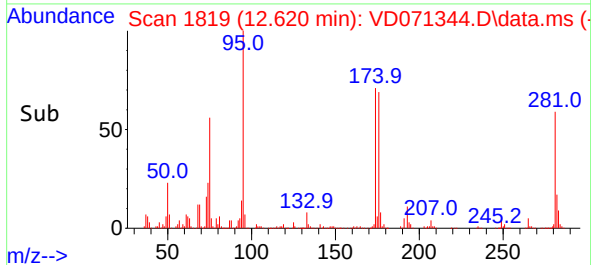
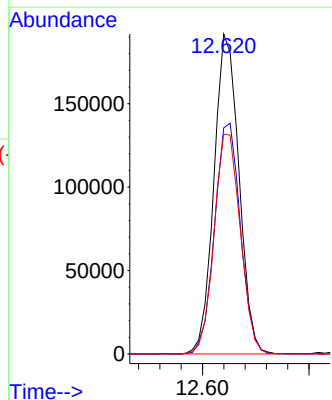
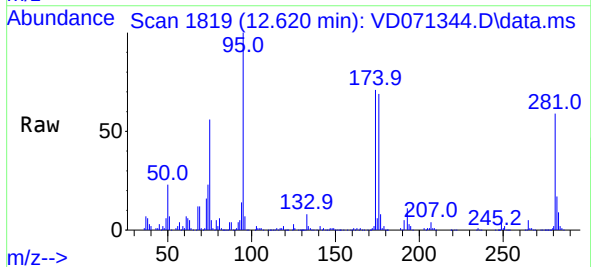


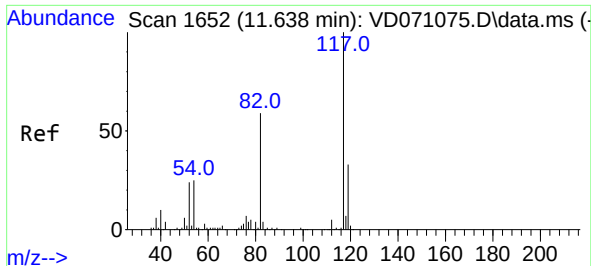

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56

Instrument :
MSVOA_D
ClientSampleId :
BB1

Tgt Ion:117 Resp: 616884
Ion Ratio Lower Upper
117 100
82 57.0 44.7 67.1
119 30.2 26.2 39.4

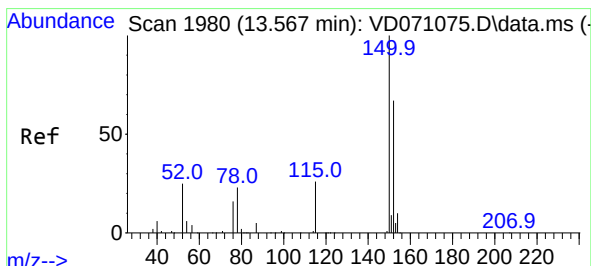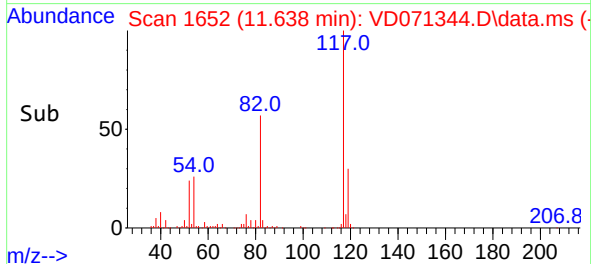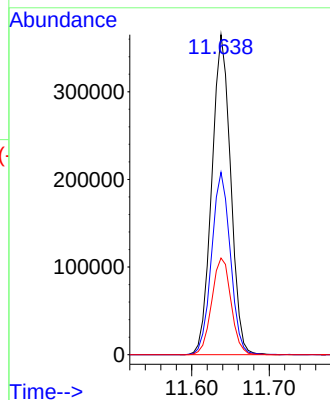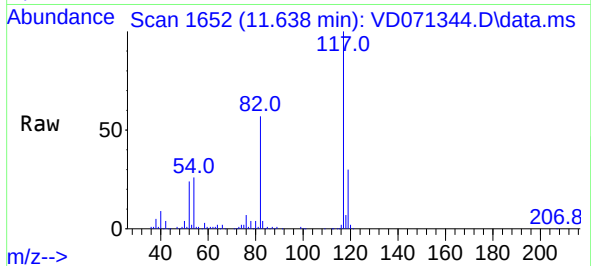

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. -0.006 min
Lab File: VD071344.D
Acq: 15 Dec 2021 15:56

Tgt Ion:152 Resp: 292912
Ion Ratio Lower Upper
152 100
115 62.8 29.8 89.3
150 159.1 0.0 349.2

