

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121523\
 Data File : VD077922.D
 Acq On : 16 Dec 2023 01:50
 Operator : RP/MD
 Sample : 05758-37
 Misc : 4.70G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SP-COMP-5

Quant Time: Dec 16 05:12:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	165411	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	302261	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	280032	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	117657	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	71503	36.685	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	73.360%
35) Dibromofluoromethane	7.805	113	88522	41.810	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	83.620%
50) Toluene-d8	10.269	98	388177	45.777	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	91.560%
62) 4-Bromofluorobenzene	12.575	95	105050	41.436	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	82.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121523\
Data File : VD077922.D
Acq On : 16 Dec 2023 01:50
Operator : RP/MD
Sample : 05758-37
Misc : 4.70G/5.0ml/MSVOA_D/SOIL
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SP-COMP-5

Quant Time: Dec 16 05:12:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration



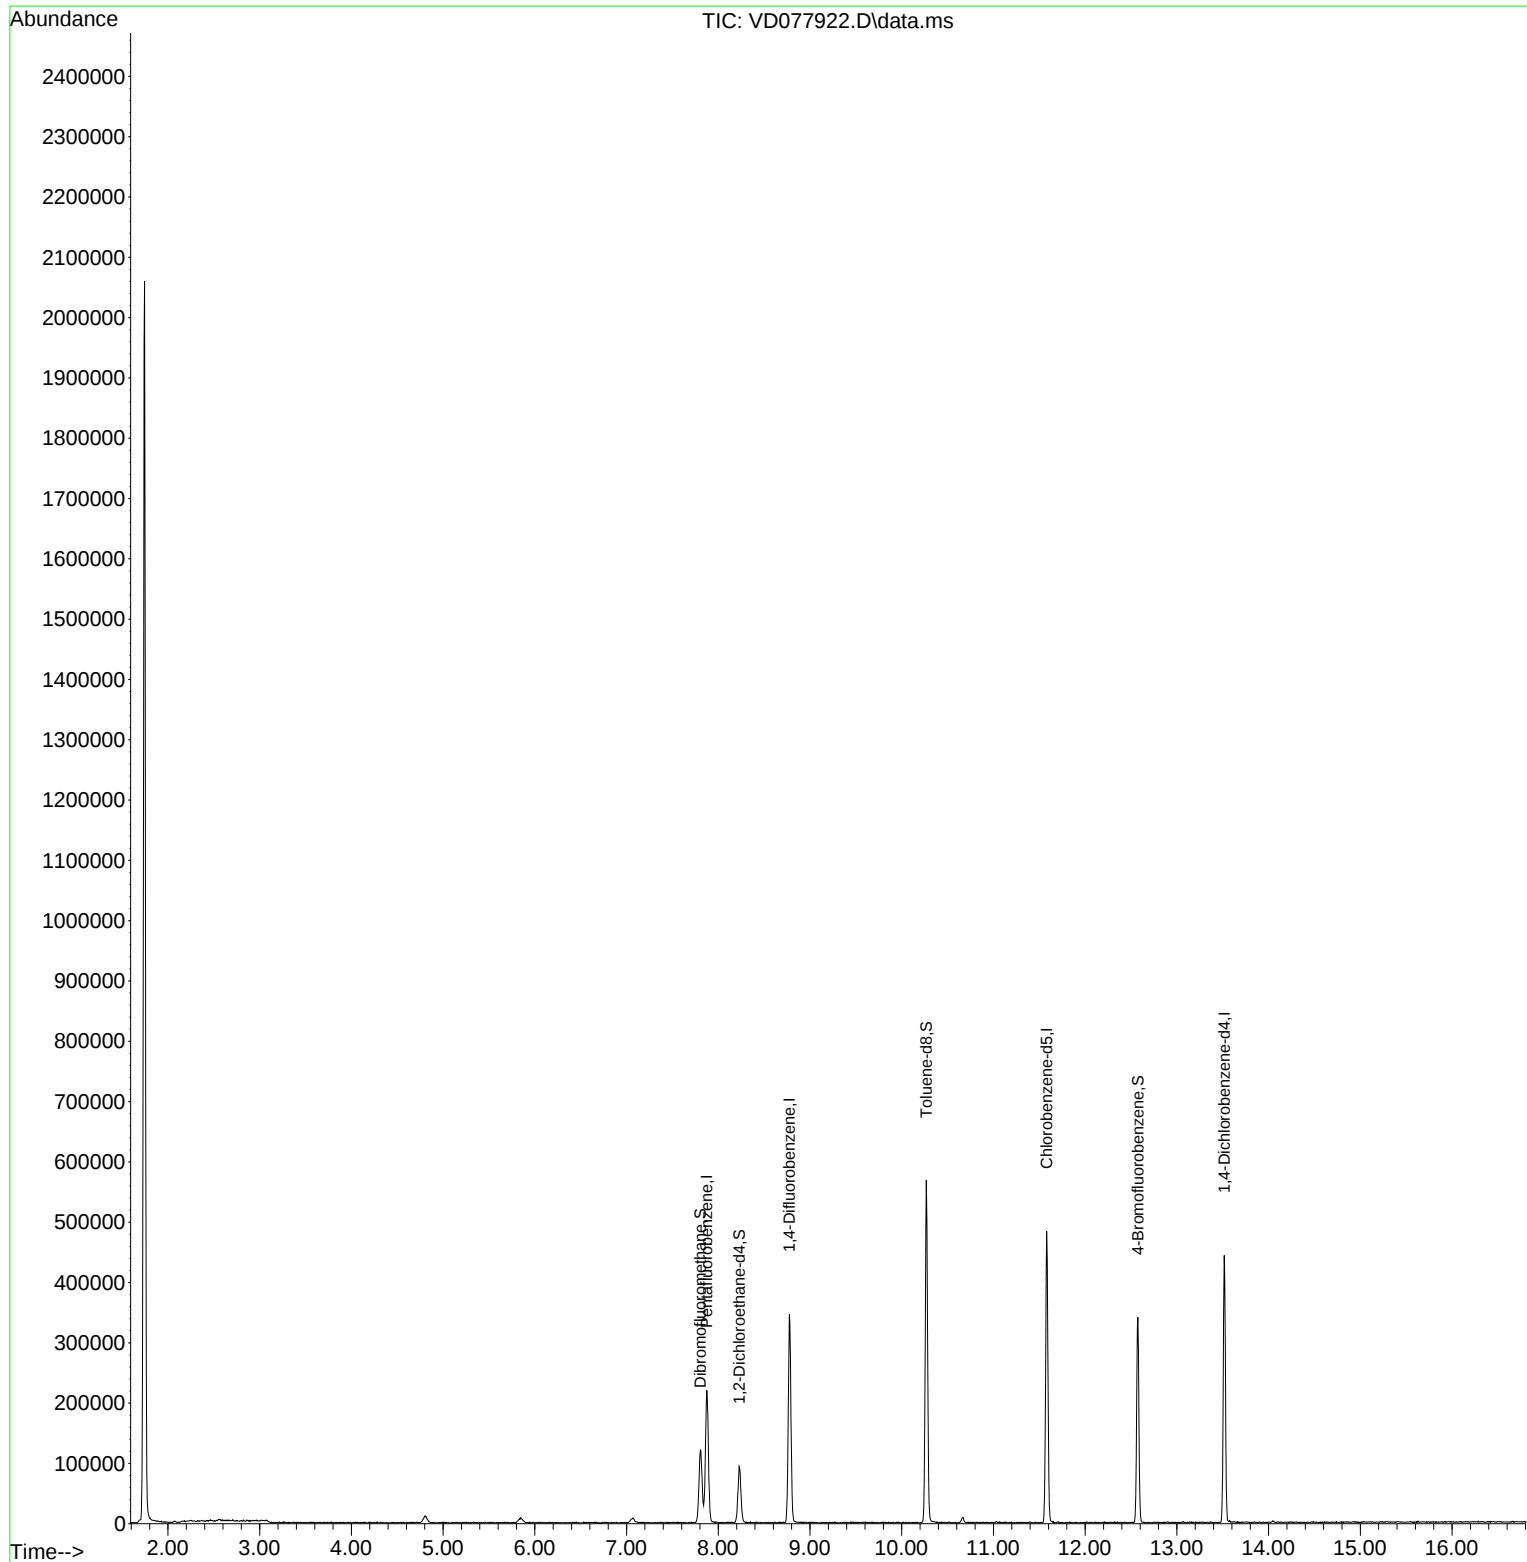


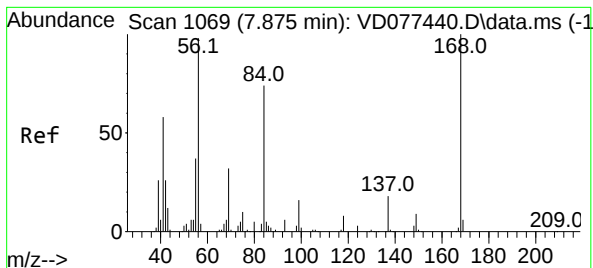

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50




Instrument :
MSVOA_D
ClientSampleId :
SP-COMP-5


Tgt Ion:168 Resp: 165411
Ion Ratio Lower Upper
168 100
99 55.6 36.7 55.1#

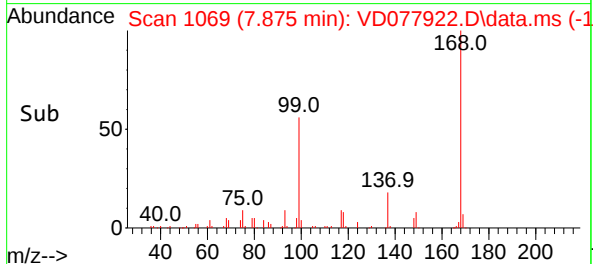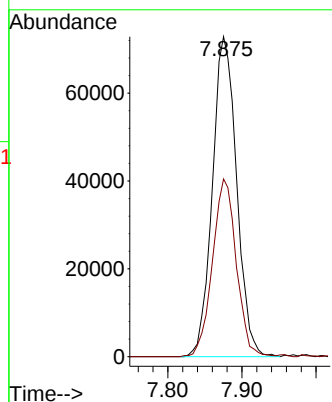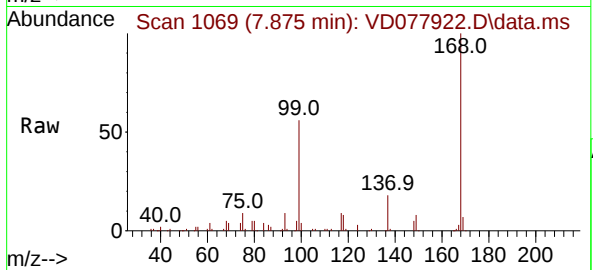

#33
1,2-Dichloroethane-d4
Concen: 36.685 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. 0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50

Tgt Ion: 65 Resp: 71503
Ion Ratio Lower Upper
65 100
67 55.7 0.0 115.0

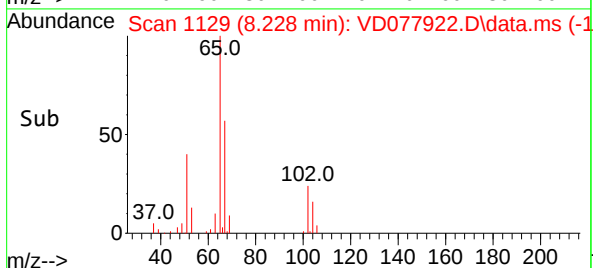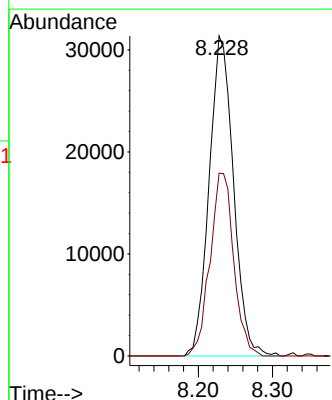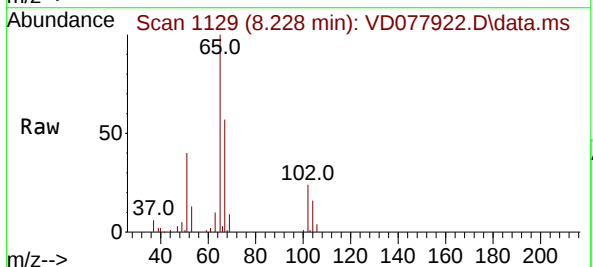

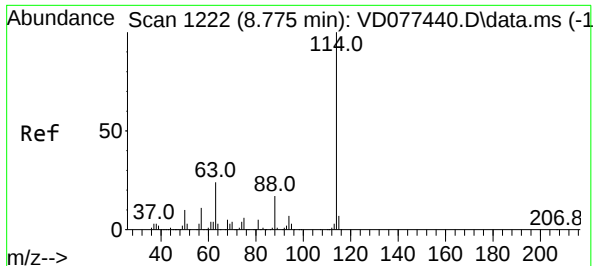

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD077922.D

Acq: 16 Dec 2023 01:50

Instrument :

MSVOA_D

ClientSampleId :

SP-COMP-5





Tgt Ion:114 Resp: 302261

Ion Ratio Lower Upper

114 100

63 20.2 0.0 33.4

88 15.4 0.0 26.2

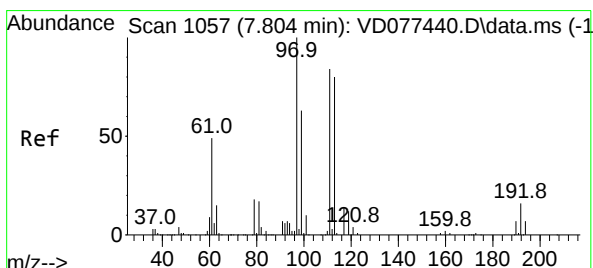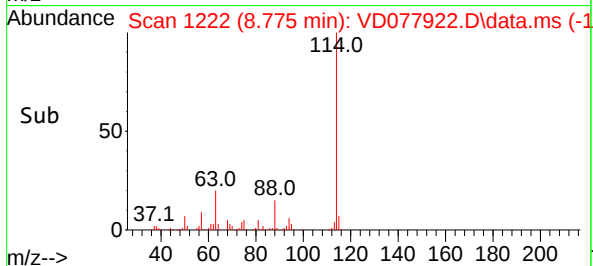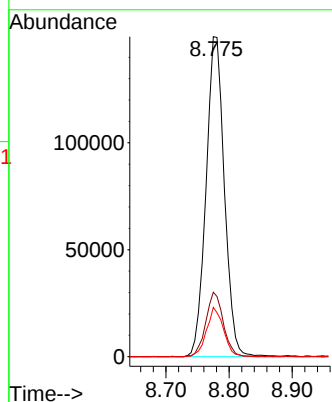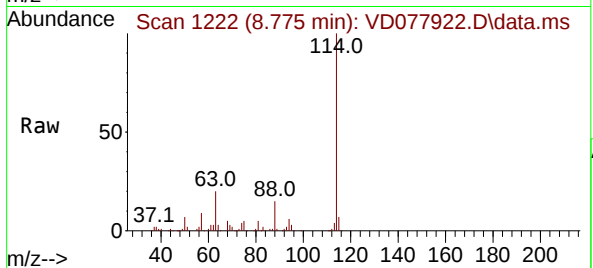

#35

Dibromofluoromethane

Concen: 41.810 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. 0.000 min

Lab File: VD077922.D

Acq: 16 Dec 2023 01:50




Tgt Ion:113 Resp: 88522


Ion Ratio Lower Upper

113 100

111 102.1 84.7 127.1

192 18.1 16.8 25.2


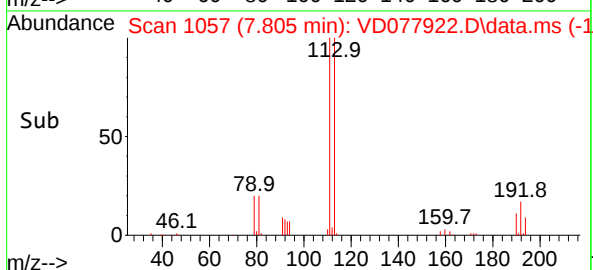
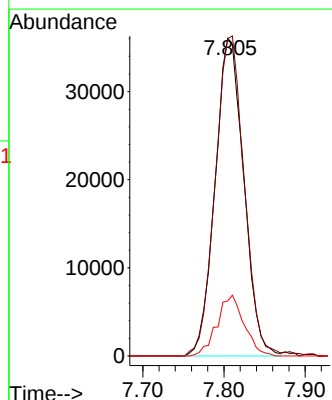
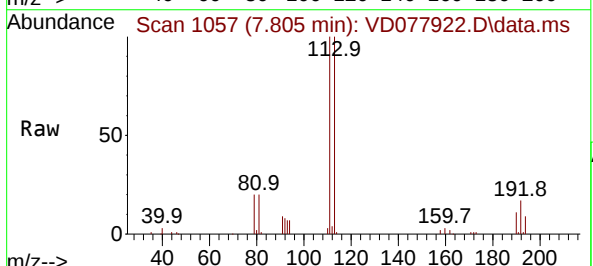


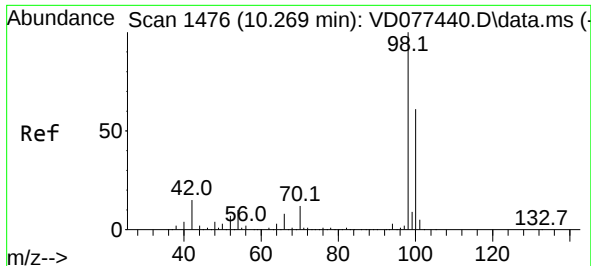

#50
Toluene-d8
Concen: 45.777 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50




Instrument :
MSVOA_D
ClientSampleId :
SP-COMP-5


Tgt Ion: 98 Resp: 388177
Ion Ratio Lower Upper
98 100
100 63.4 50.3 75.5

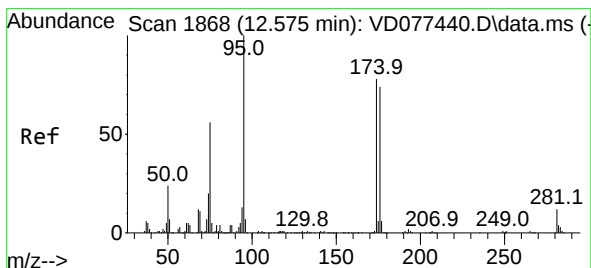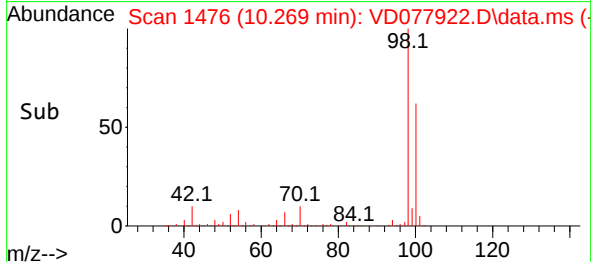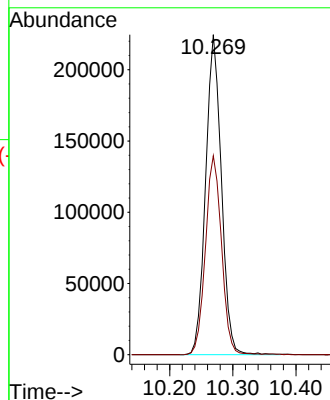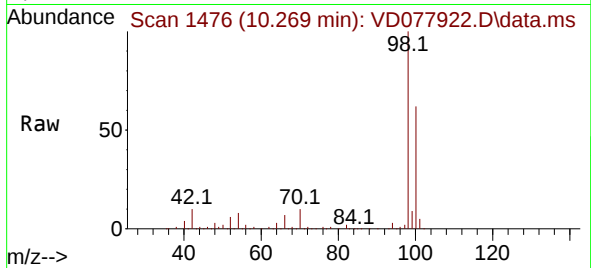

#62
4-Bromofluorobenzene
Concen: 41.436 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50

Tgt Ion: 95 Resp: 105050
Ion Ratio Lower Upper
95 100
174 88.5 0.0 201.8
176 83.5 0.0 191.8


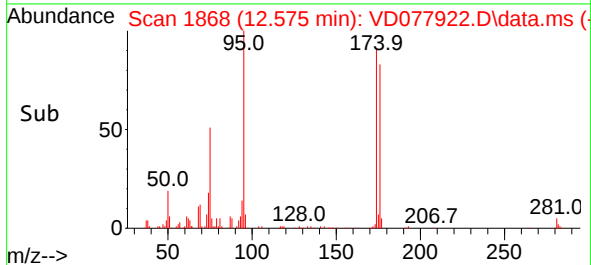
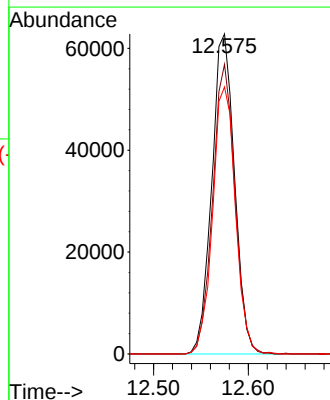
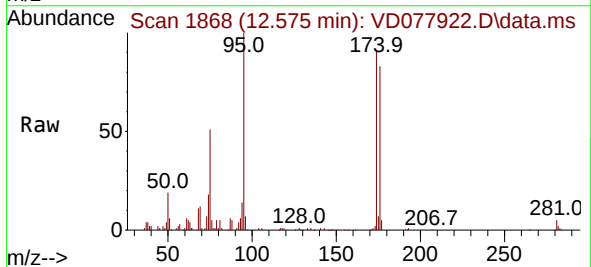


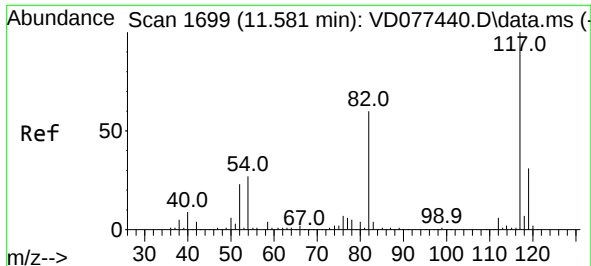

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50

Instrument :
MSVOA_D
ClientSampleId :
SP-COMP-5

Tgt Ion:117 Resp: 280032
Ion Ratio Lower Upper
117 100
82 54.4 38.3 57.5
119 30.7 25.0 37.4

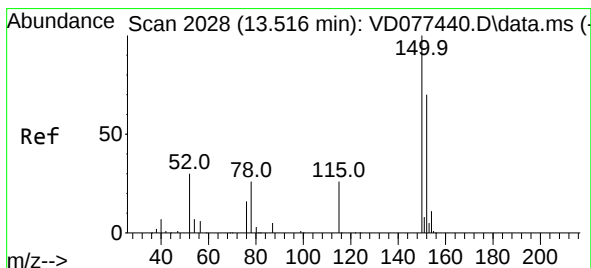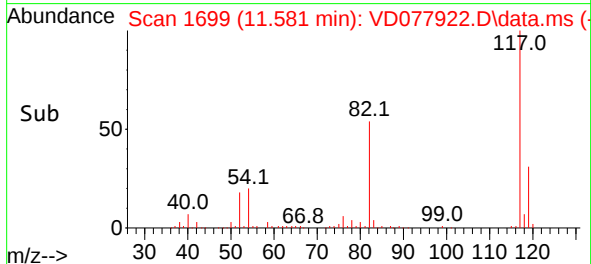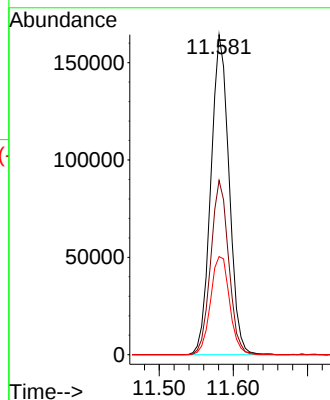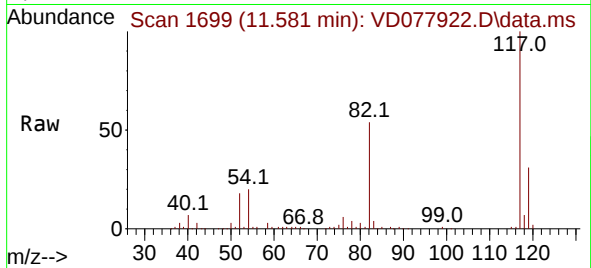

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD077922.D
Acq: 16 Dec 2023 01:50

Tgt Ion:152 Resp: 117657
Ion Ratio Lower Upper
152 100
115 57.1 27.1 81.3
150 156.2 0.0 353.6

