
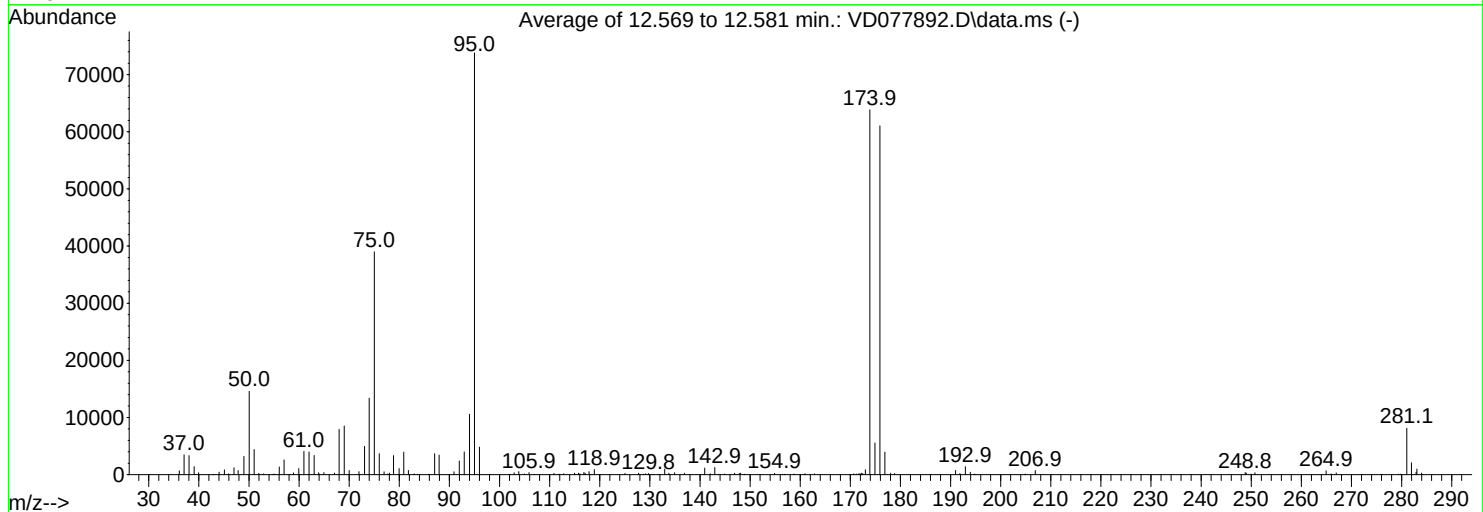


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121523\
Data File : VD077892.D
Acq On : 15 Dec 2023 08:33
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

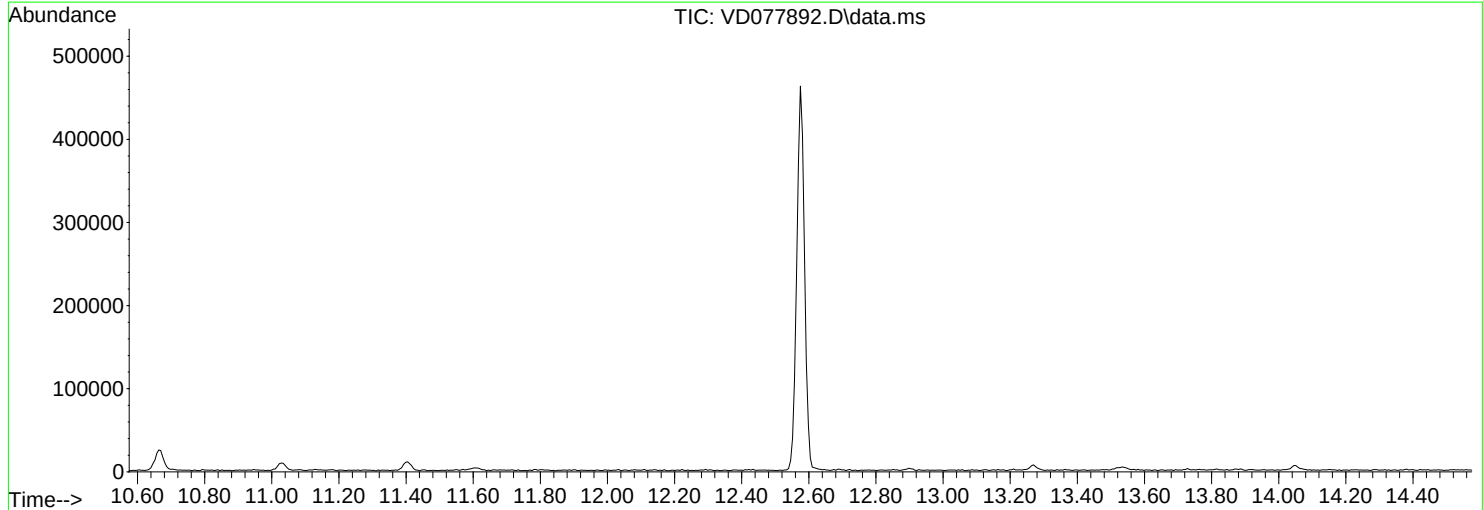

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	14602	PASS
75	95	30	60	52.8	39011	PASS
95	95	100	100	100.0	73816	PASS
96	95	5	9	6.5	4831	PASS
173	174	0.00	2	1.3	845	PASS
174	95	50	100	86.5	63848	PASS
175	174	5	9	8.7	5554	PASS
176	174	95	101	95.6	61043	PASS
177	176	5	9	6.5	3950	PASS