
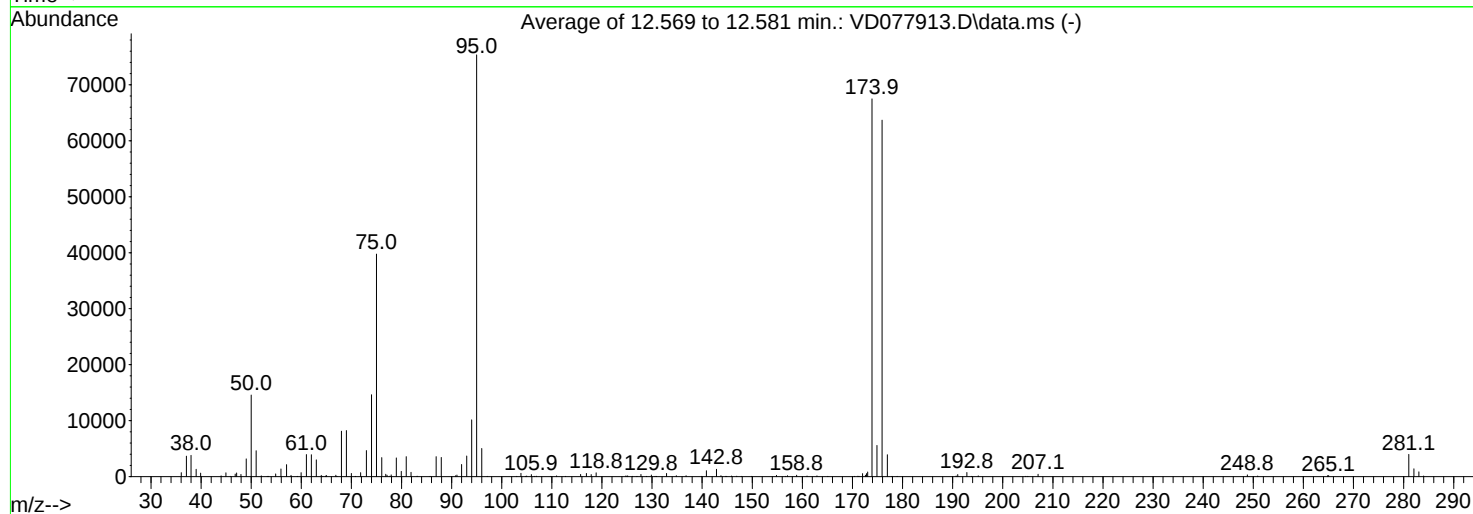


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121523\
Data File : VD077913.D
Acq On : 15 Dec 2023 19:59
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

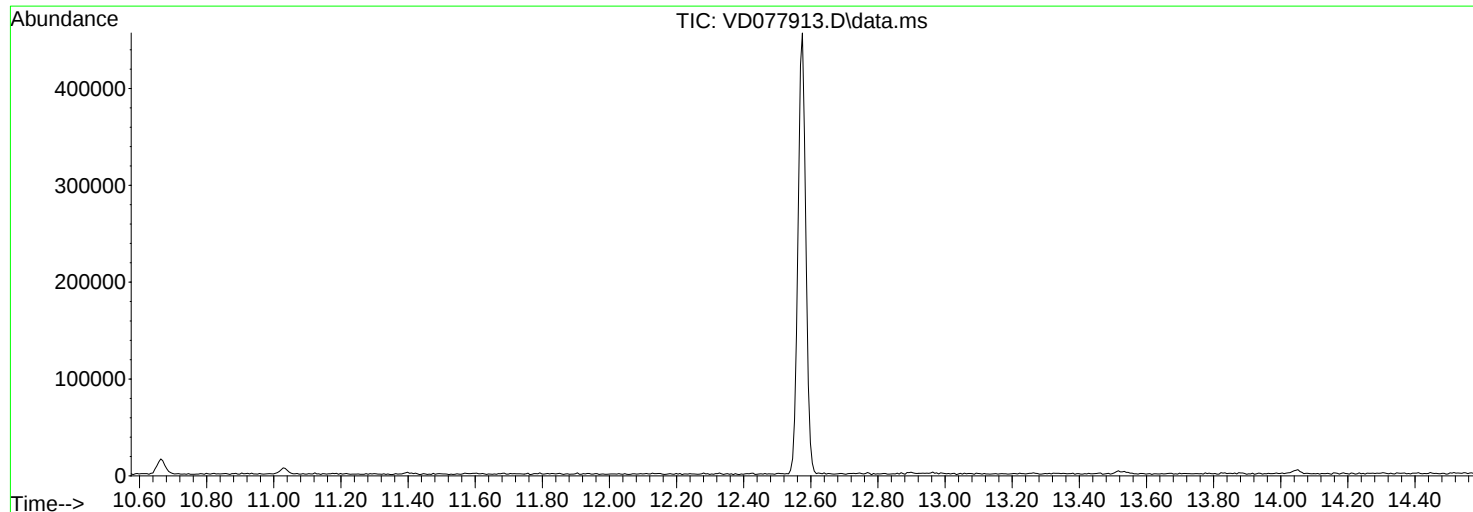

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	14592	PASS
75	95	30	60	52.8	39771	PASS
95	95	100	100	100.0	75349	PASS
96	95	5	9	6.7	5035	PASS
173	174	0.00	2	1.3	846	PASS
174	95	50	100	89.6	67499	PASS
175	174	5	9	8.3	5579	PASS
176	174	95	101	94.3	63685	FAIL*
177	176	5	9	6.2	3928	PASS