


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD121619\
Data File : VD064517.D
Acq On : 16 Dec 2019 09:38
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D112719S.M
Title : SW846 8260
Last Update : Fri Nov 29 07:18:03 2019

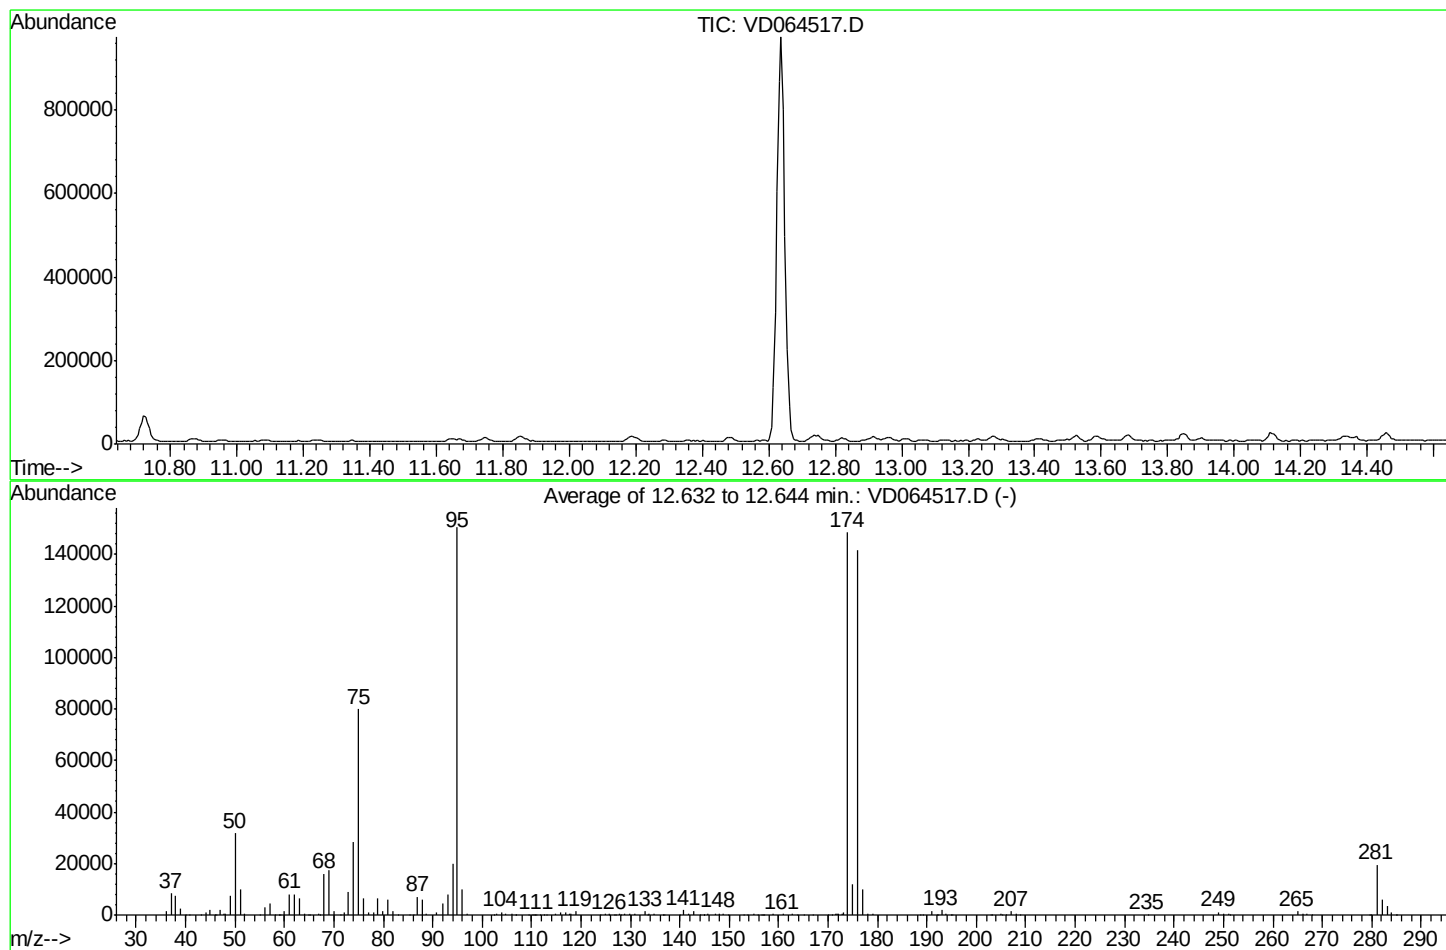

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	31698	PASS
75	95	30	60	53.2	80005	PASS
95	95	100	100	100.0	150506	PASS
96	95	5	9	6.6	9921	PASS
173	174	0.00	2	0.8	1235	PASS
174	95	50	100	98.7	148501	PASS
175	174	5	9	7.9	11755	PASS
176	174	95	101	95.5	141802	PASS
177	176	5	9	6.9	9752	PASS