

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121623\
 Data File : VD077936.D
 Acq On : 16 Dec 2023 16:18
 Operator : RP/MD
 Sample : 05791-08
 Misc : 5.05G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MW-1B-SOIL

Quant Time: Dec 18 02:00:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	127451	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	230702	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	227721	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	102859	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	69437	46.235	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.480%
35) Dibromofluoromethane	7.805	113	71503	44.247	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	88.500%
50) Toluene-d8	10.269	98	293405	45.333	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	90.660%
62) 4-Bromofluorobenzene	12.575	95	89018	46.003	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	92.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121623\
Data File : VD077936.D
Acq On : 16 Dec 2023 16:18
Operator : RP/MD
Sample : 05791-08
Misc : 5.05G/5.0ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MW-1B-SOIL

Quant Time: Dec 18 02:00:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




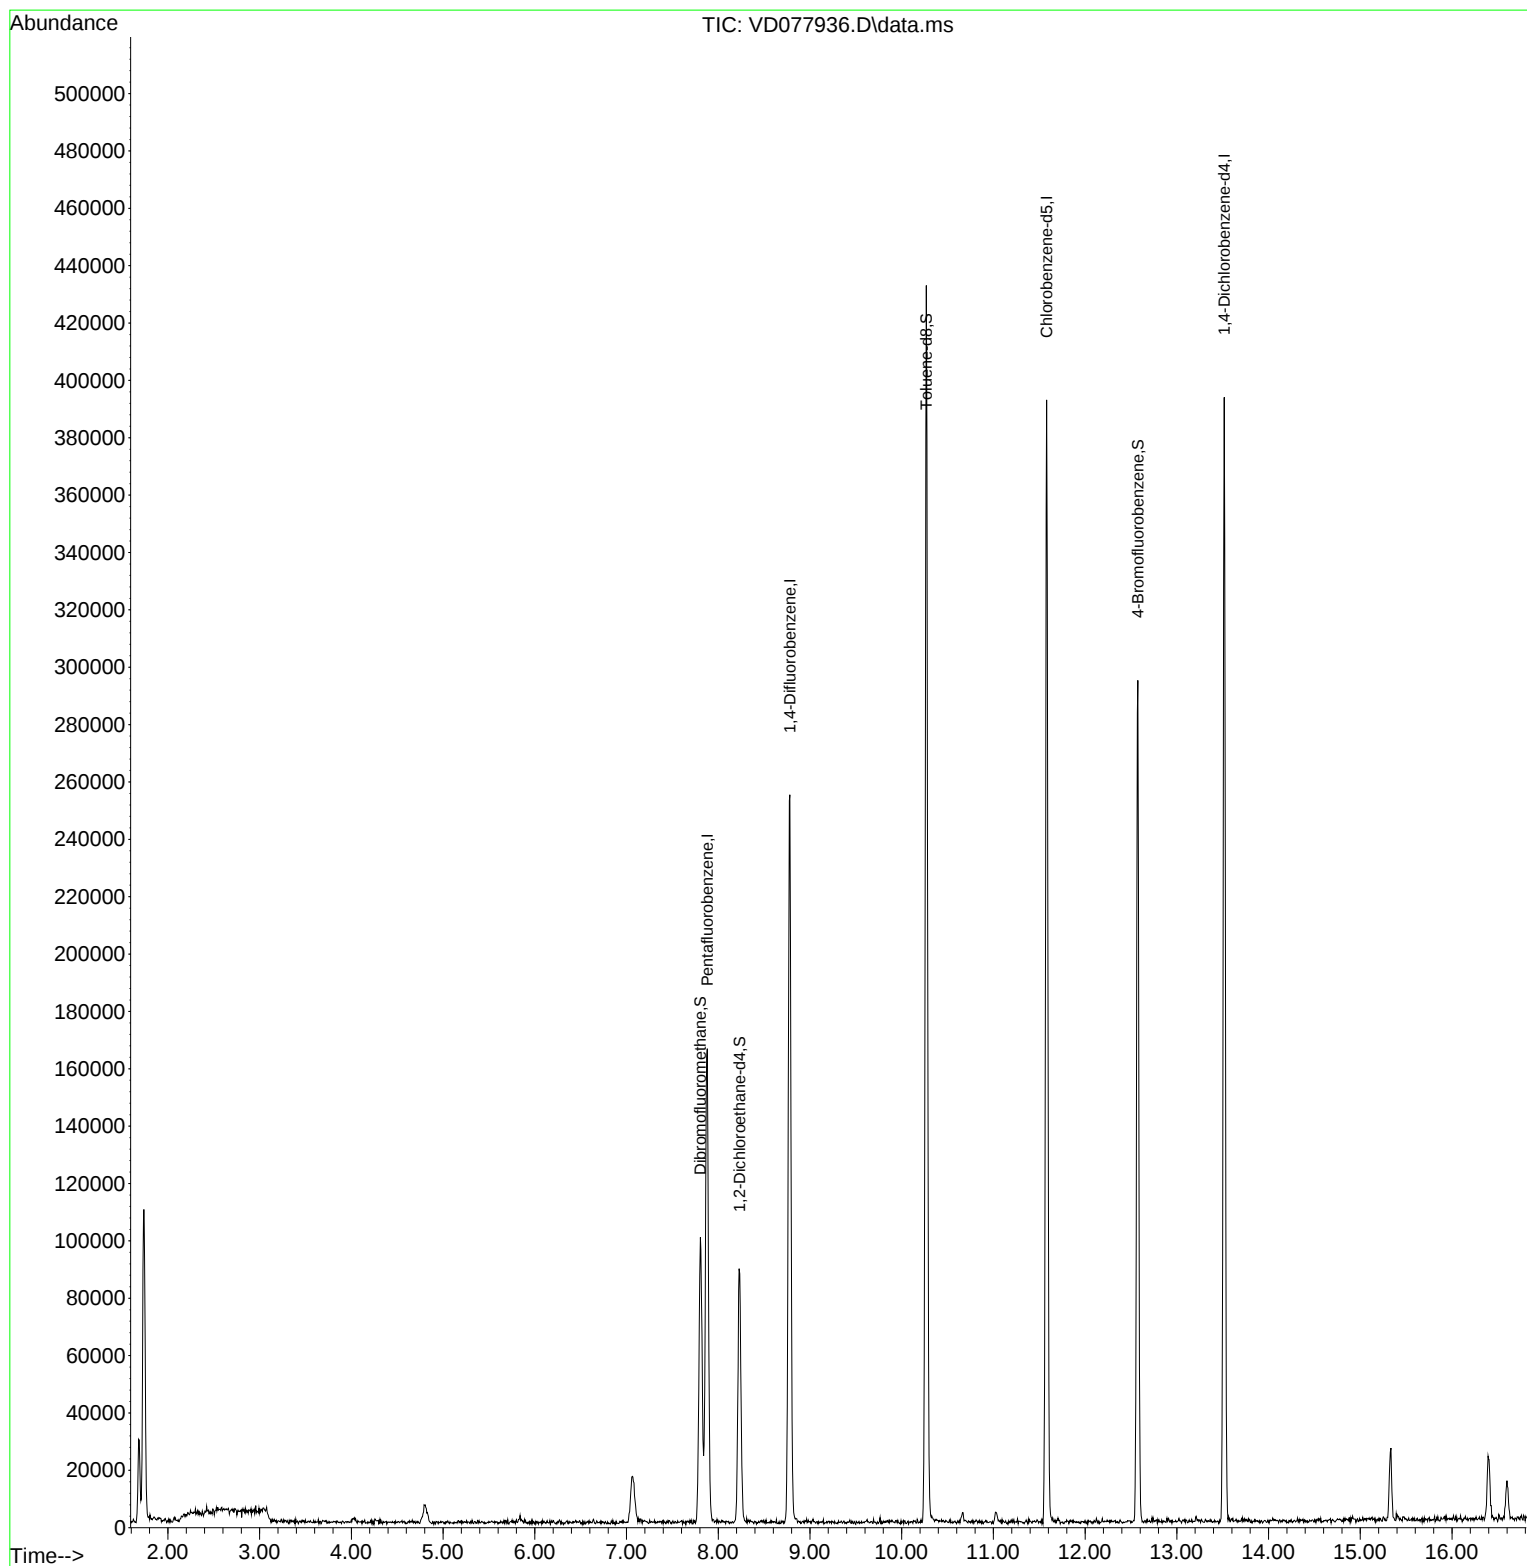


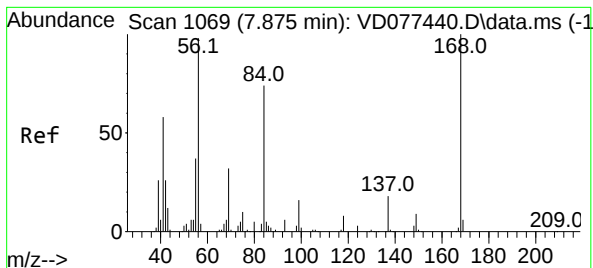

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18




Instrument :
MSVOA_D
ClientSampleId :
MW-1B-SOIL


Tgt Ion:168 Resp: 127451
Ion Ratio Lower Upper
168 100
99 50.6 36.7 55.1

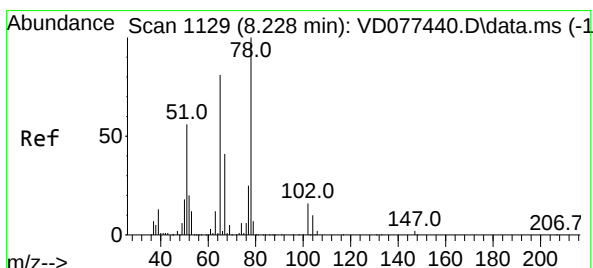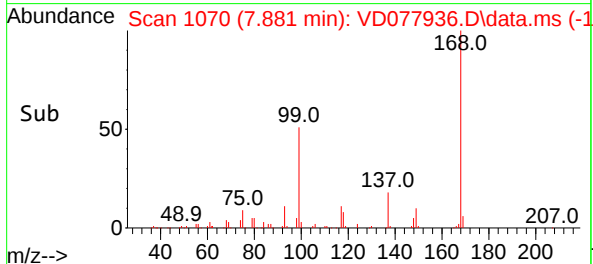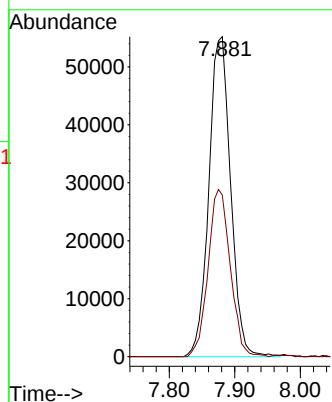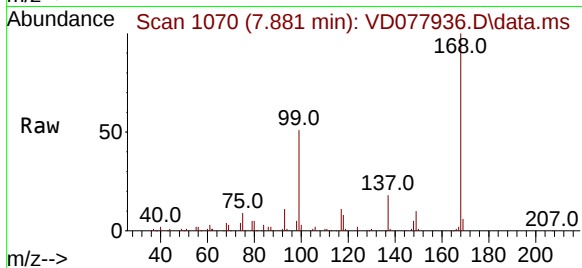

#33
1,2-Dichloroethane-d4
Concen: 46.235 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18

Tgt Ion: 65 Resp: 69437
Ion Ratio Lower Upper
65 100
67 53.7 0.0 115.0

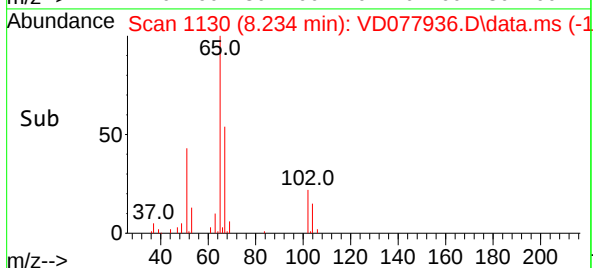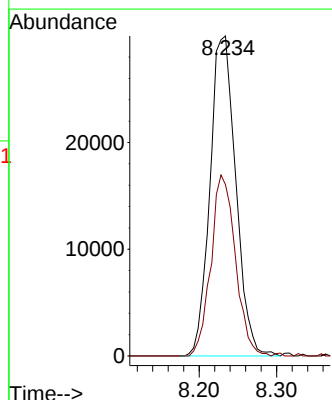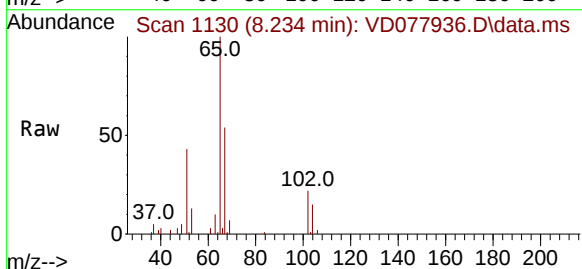

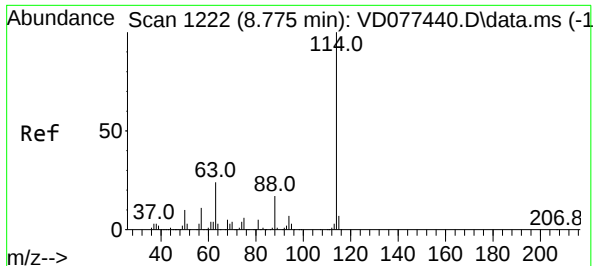

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD077936.D

Acq: 16 Dec 2023 16:18

Instrument :

MSVOA_D

ClientSampleId :

MW-1B-SOIL





Tgt Ion:114 Resp: 230702

Ion Ratio Lower Upper

114 100

63 19.7 0.0 33.4

88 12.9 0.0 26.2

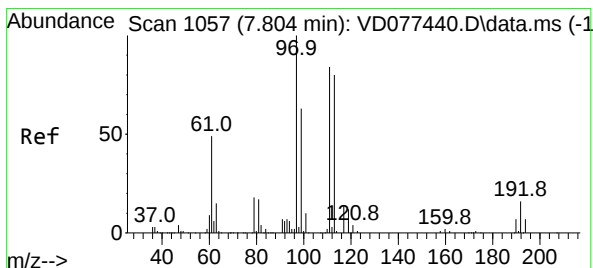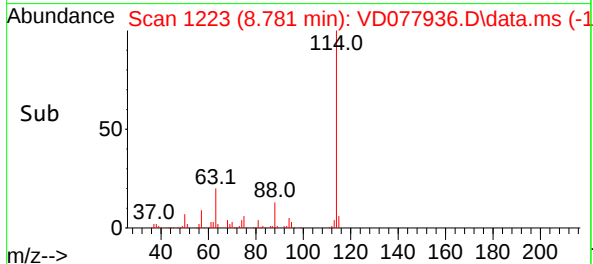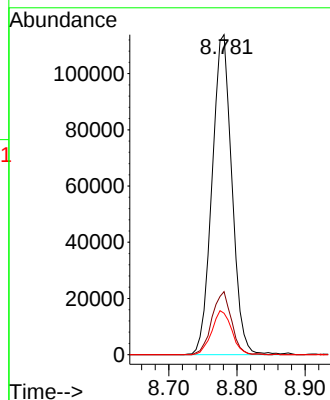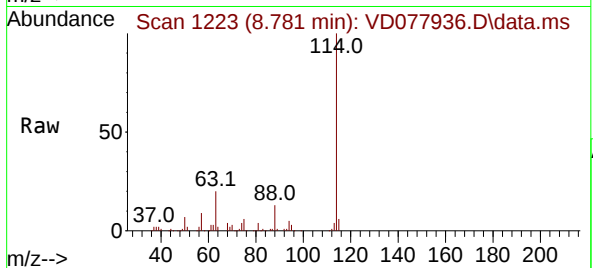

#35

Dibromofluoromethane

Concen: 44.247 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. 0.001 min

Lab File: VD077936.D

Acq: 16 Dec 2023 16:18




Tgt Ion:113 Resp: 71503

Ion Ratio Lower Upper

113 100

111 103.3 84.7 127.1

192 18.4 16.8 25.2

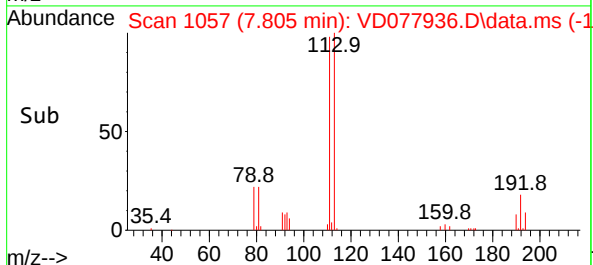
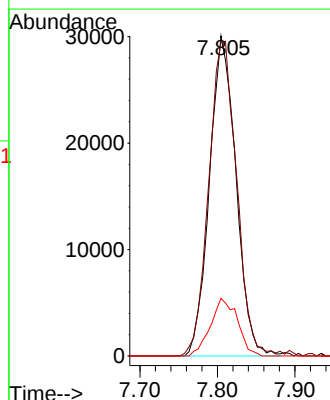
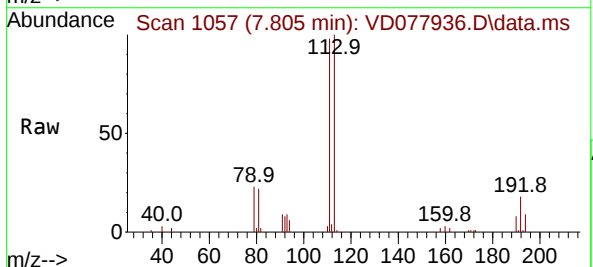




#50
Toluene-d8
Concen: 45.333 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18




Instrument :
MSVOA_D
ClientSampleId :
MW-1B-SOIL


Tgt Ion: 98 Resp: 293405
Ion Ratio Lower Upper
98 100
100 63.5 50.3 75.5

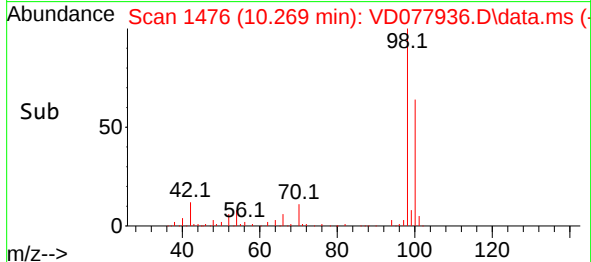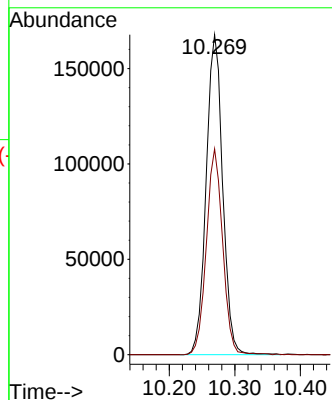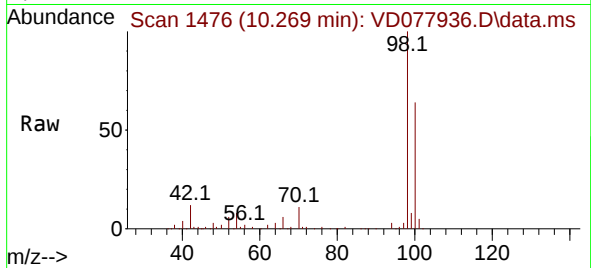

#62
4-Bromofluorobenzene
Concen: 46.003 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18

Tgt Ion: 95 Resp: 89018
Ion Ratio Lower Upper
95 100
174 89.2 0.0 201.8
176 85.2 0.0 191.8


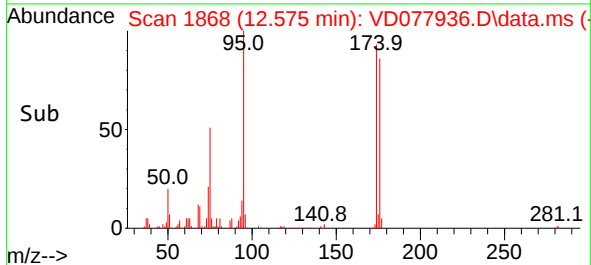
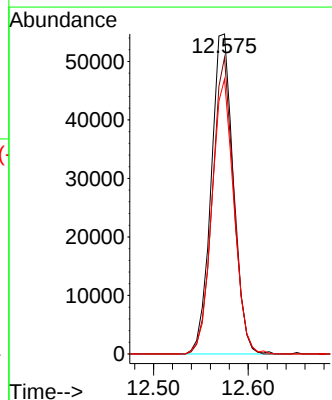
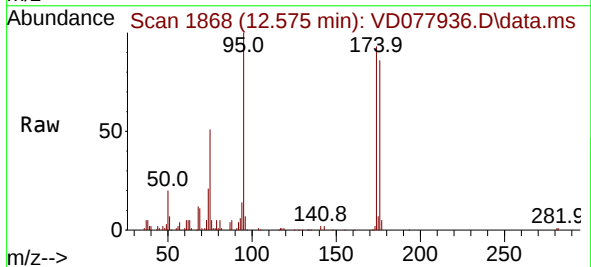


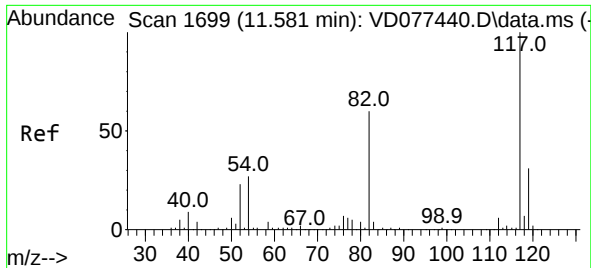

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18

Instrument :
MSVOA_D
ClientSampleId :
MW-1B-SOIL

Tgt Ion:117 Resp: 227721
Ion Ratio Lower Upper
117 100
82 53.4 38.3 57.5
119 31.2 25.0 37.4

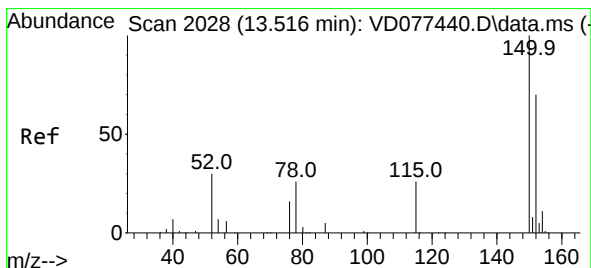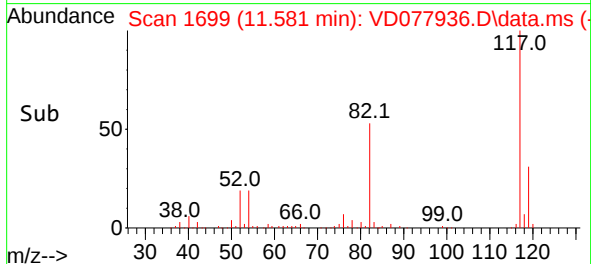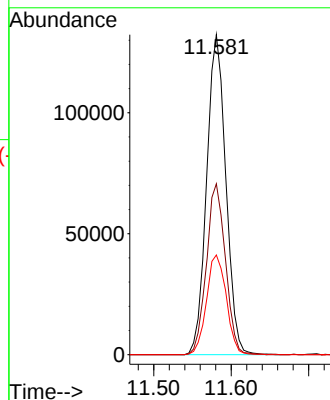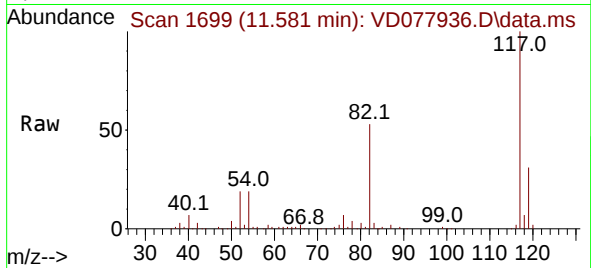

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD077936.D
Acq: 16 Dec 2023 16:18

Tgt Ion:152 Resp: 102859
Ion Ratio Lower Upper
152 100
115 57.0 27.1 81.3
150 157.8 0.0 353.6

