

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD121718\
 Data File : VD060602.D
 Acq On : 17 Dec 2018 16:30
 Operator : VA/AP
 Sample : J6424-02
 Misc : 4.35g/5ml/MSVOA D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EB12_12-14

Quant Time: Dec 18 13:21:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 06 01:49:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.42	168	1399322	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	7.47	114	1988835	50.00	ug/l	0.01
63) Chlorobenzene-d5	11.29	117	1591007	50.00	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.38	152	821831	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.81	65	505854	51.00	ug/l	0.01
Spiked Amount 50.000			Recovery	=	102.00%	
35) Dibromofluoromethane	6.34	113	682313	46.71	ug/l	0.01
Spiked Amount 50.000			Recovery	=	93.42%	
50) Toluene-d8	9.47	98	2008807	47.52	ug/l	0.01
Spiked Amount 50.000			Recovery	=	95.04%	
62) 4-Bromofluorobenzene	12.44	95	707166	46.75	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.50%	
Target Compounds						
16) Acetone	3.18	43	18156	11.420	ug/l	92
52) Toluene	9.56	92	42012	1.353	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD121718\
Data File : VD060602.D
Acq On : 17 Dec 2018 16:30
Operator : VA/AP
Sample : J6424-02
Misc : 4.35g/5ml/MSVOA D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EB12_12-14

Quant Time: Dec 18 13:21:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D120518S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 06 01:49:20 2018
Response via : Initial Calibration

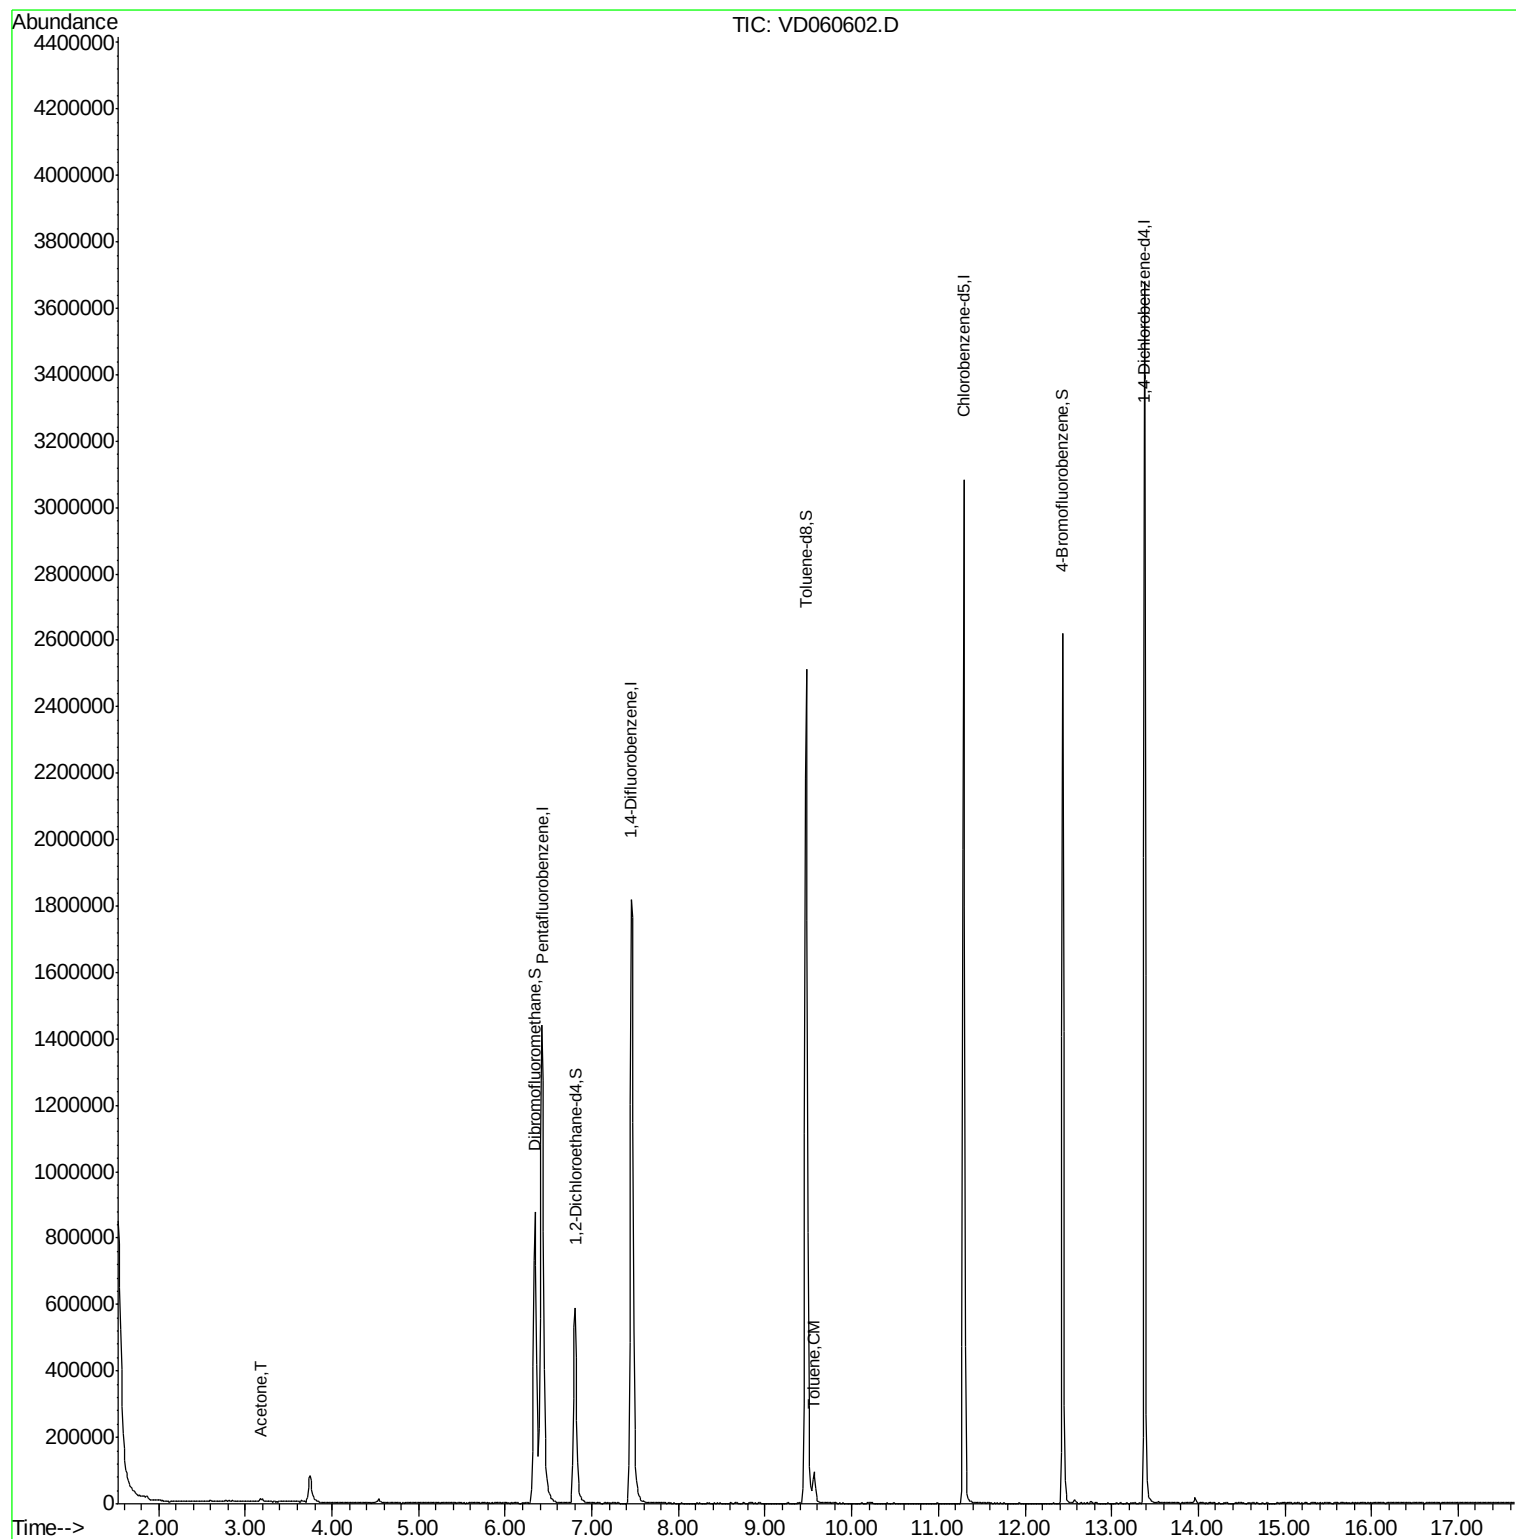

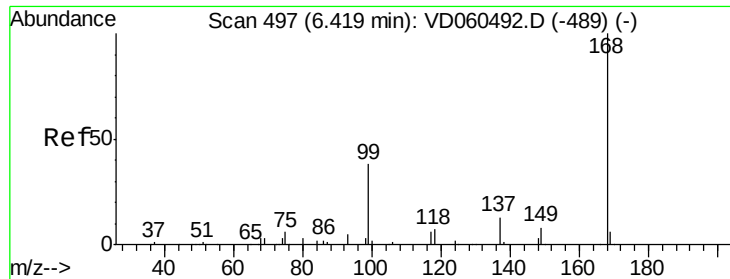

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 6.42 min Scan# 498

Delta R.T. 0.00 min

Lab File: VD060602.D

Acq: 17 Dec 2018 16:30

Instrument :

MSVOA_D

ClientSampleId :


EB12_12-14

Tot Ion:168 Resp: 1399322

Ion Ratio Lower Upper

168 100

99 48.7 35.6 53.4

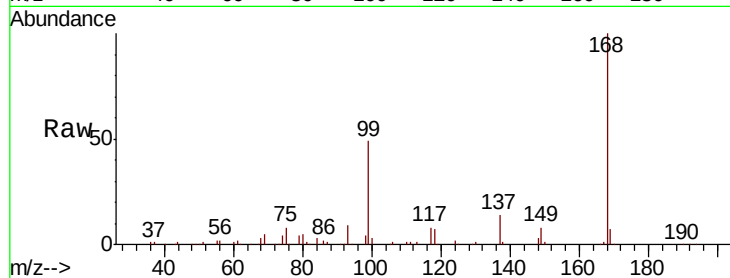

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

6.42

500000

400000



300000

200000

100000

0

Time-->

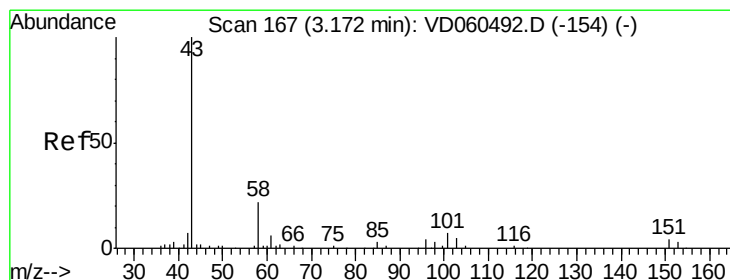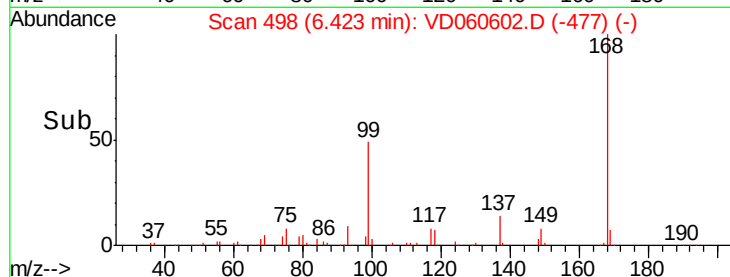

#16

Acetone

Concen: 11.420 ug/l

RT: 3.18 min Scan# 168

Delta R.T. 0.00 min

Lab File: VD060602.D


Acq: 17 Dec 2018 16:30

Tgt Ion: 43 Resp: 18156

Ion Ratio Lower Upper

43 100

58 17.8 17.3 25.9

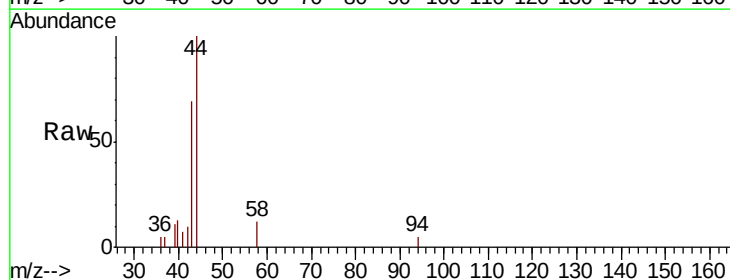

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

3.18

5000

4000


3000


2000

1000

0

Time-->




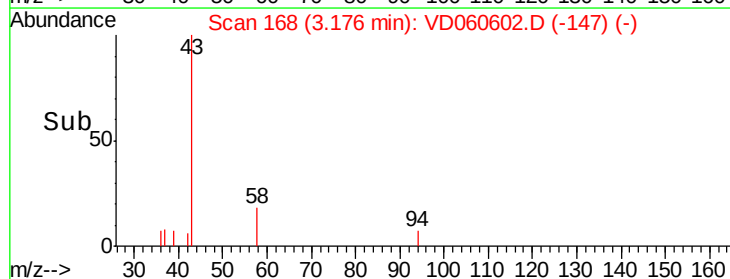


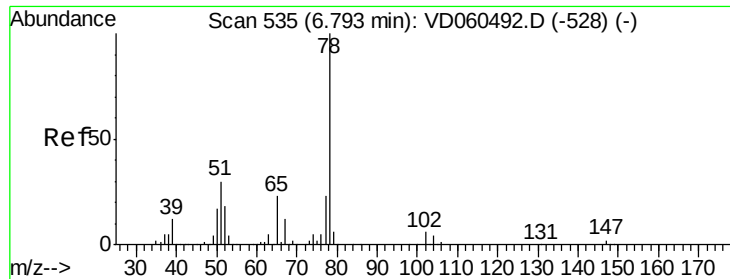

#33
 1,2-Dichloroethane-d4
 Concen: N.D. ug/l
 RT: 6.81 min Scan# 537
 Delta R.T. 0.01 min
 Lab File: VD060602.D
 Acq: 17 Dec 2018 16:30




Instrument :
 MSVOA_D
 ClientSampleId :
 EB12_12-14


Tot Ion: 65 Resp: 505854
 Ion Ratio Lower Upper
 65 100
 67 51.1 0.0 106.8

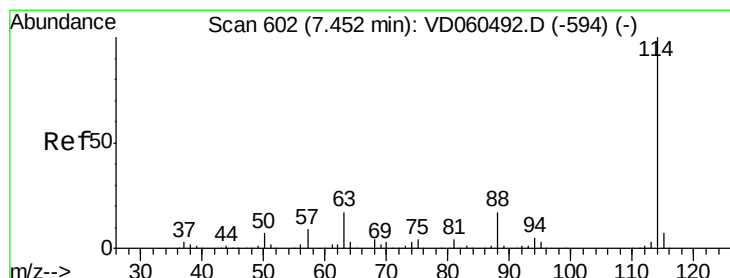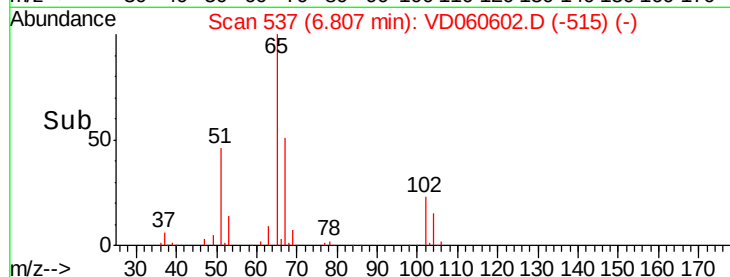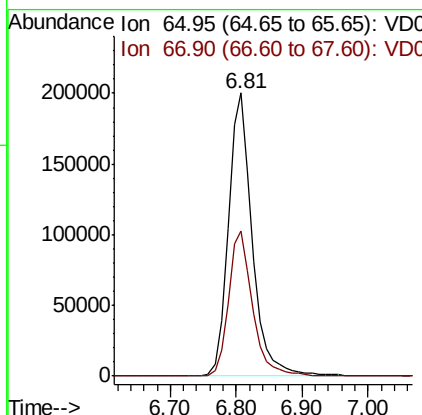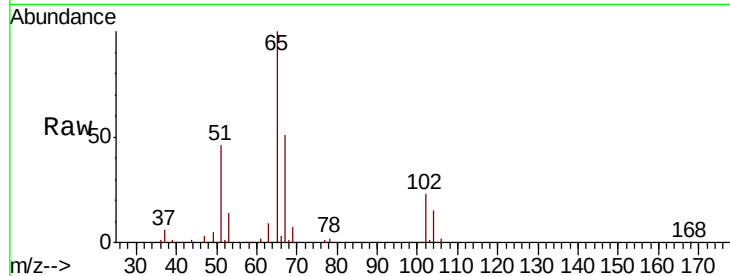

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 7.47 min Scan# 604
 Delta R.T. 0.01 min
 Lab File: VD060602.D
 Acq: 17 Dec 2018 16:30

Tgt Ion:114 Resp: 1988835
 Ion Ratio Lower Upper
 114 100
 63 17.4 0.0 34.2
 88 17.6 0.0 35.0

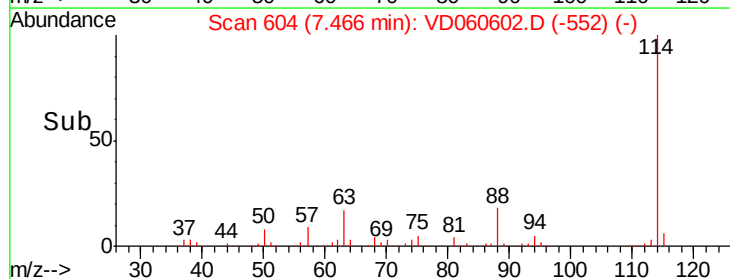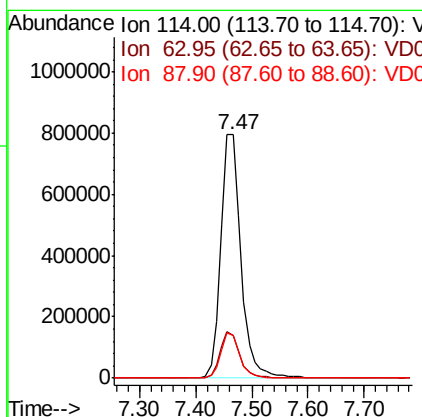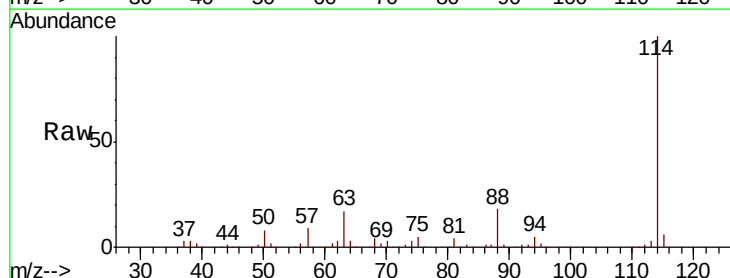

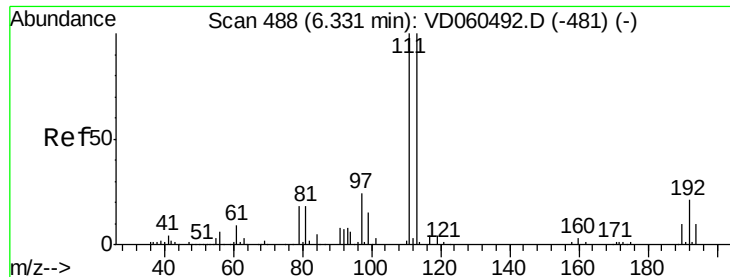

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 6.34 min Scan# 490

Delta R.T. 0.01 min

Lab File: VD060602.D

Acq: 17 Dec 2018 16:30

Instrument :

MSVOA_D

ClientSampleId :

EB12_12-14


Tot Ion:113 Resp: 682313

Ion Ratio Lower Upper

113 100

111 105.5 80.2 120.4




192 21.4 16.6 24.8

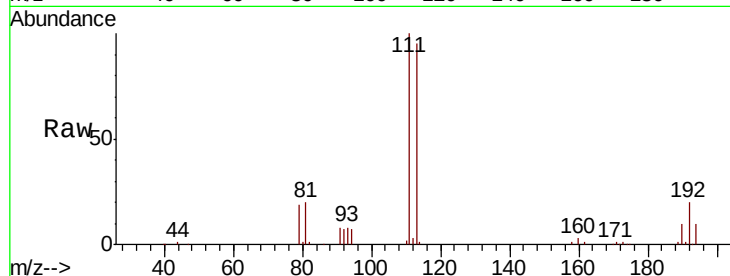

Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

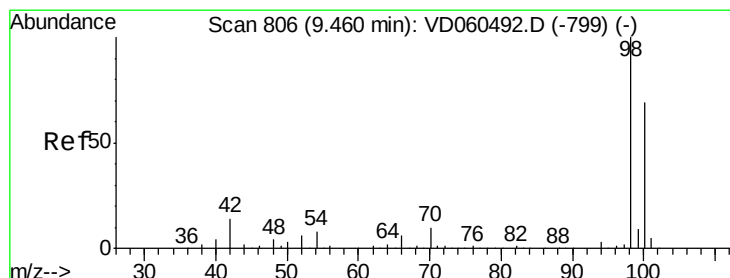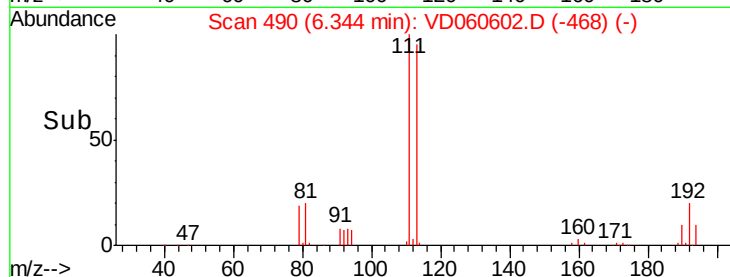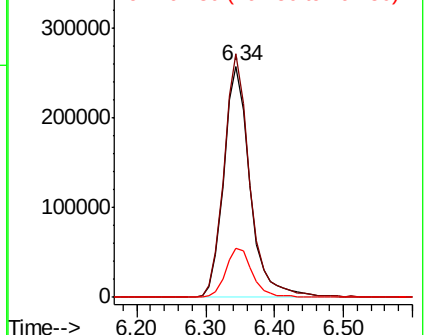

#50

Toluene-d8

Concen: N.D. ug/l

RT: 9.47 min Scan# 808

Delta R.T. 0.01 min

Lab File: VD060602.D


Acq: 17 Dec 2018 16:30

Tgt Ion: 98 Resp: 2008807

Ion Ratio Lower Upper



98 100


100 69.2 55.7 83.5

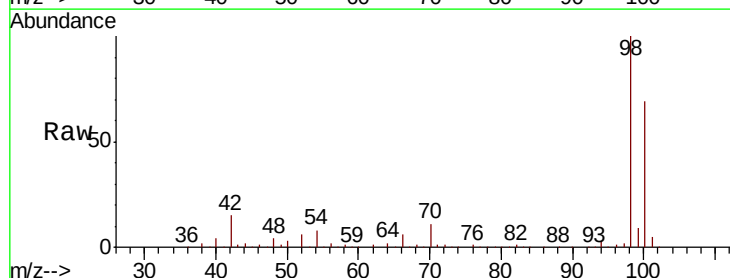

Abundance Ion 98.05 (97.75 to 98.75): V

Ion 100.05 (99.75 to 100.75): V

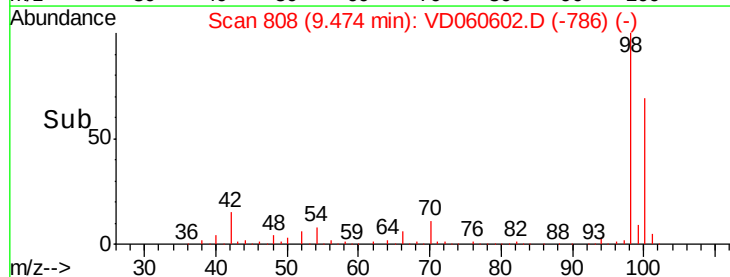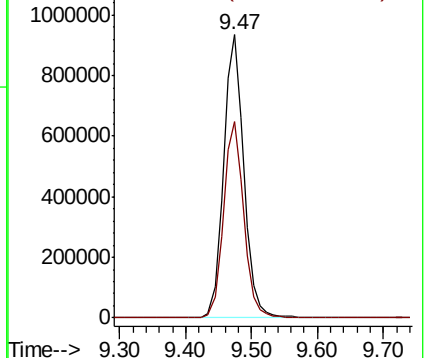

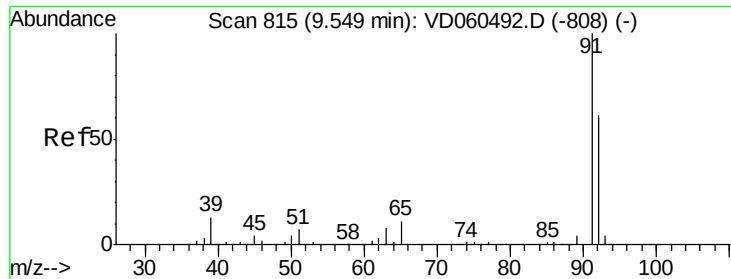

#52

Toluene

Concen: 1.353 ug/l

RT: 9.56 min Scan# 817

Delta R.T. 0.01 min

Lab File: VD060602.D

Acq: 17 Dec 2018 16:30

Instrument :

MSVOA_D

ClientSampleId :





EB12_12-14

Tot Ion: 92 Resp: 42012

Ion Ratio Lower Upper

92 100

91 175.3 131.7 197.5

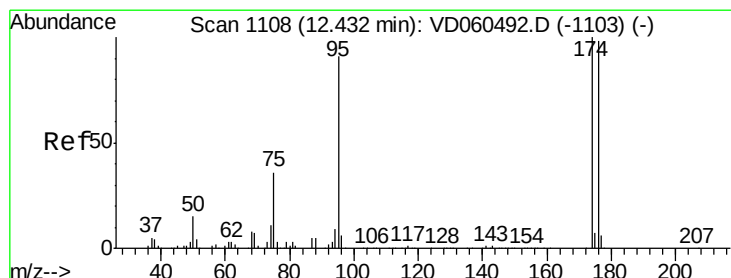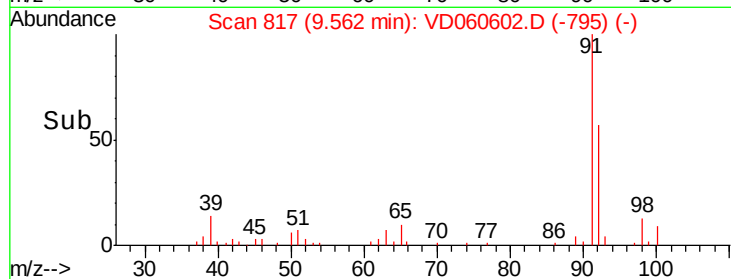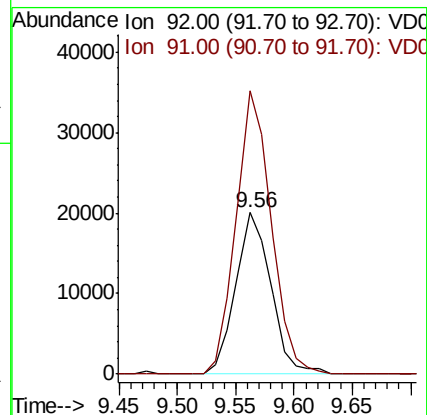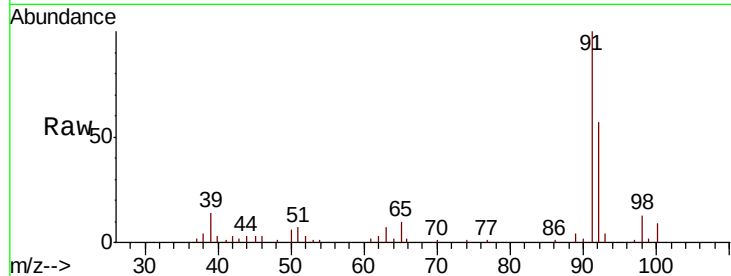

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.44 min Scan# 1109

Delta R.T. 0.00 min

Lab File: VD060602.D

Acq: 17 Dec 2018 16:30




Tgt Ion: 95 Resp: 707166


Ion Ratio Lower Upper

95 100

174 97.4 0.0 219.4

176 96.0 0.0 214.6

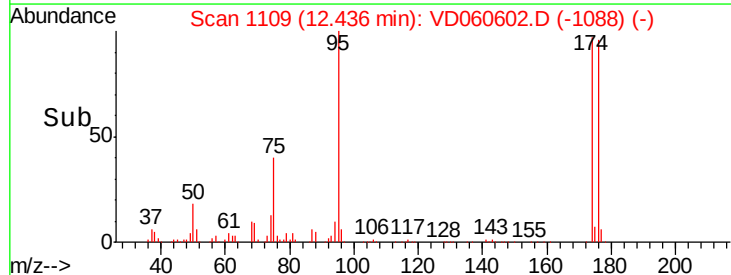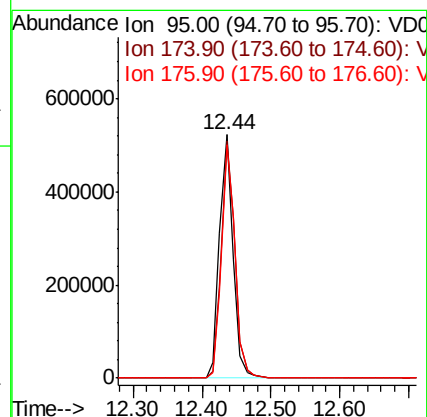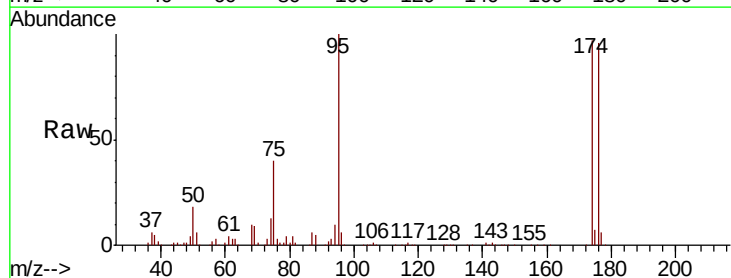


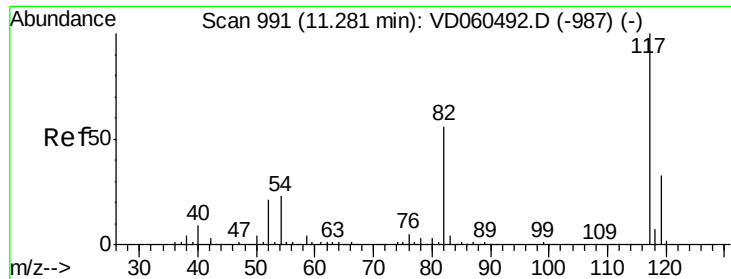




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.29 min Scan# 993
Delta R.T. 0.01 min
Lab File: VD060602.D
Acq: 17 Dec 2018 16:30

Instrument :
MSVOA_D
ClientSampled :
EB12_12-14

Tot Ion:117 Resp: 1591007
Ion Ratio Lower Upper
117 100
82 53.8 45.2 67.8
119 33.1 26.1 39.1

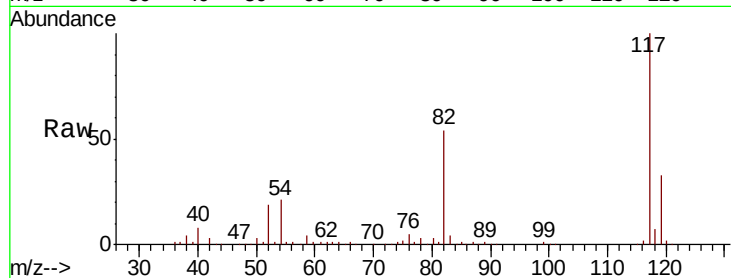


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

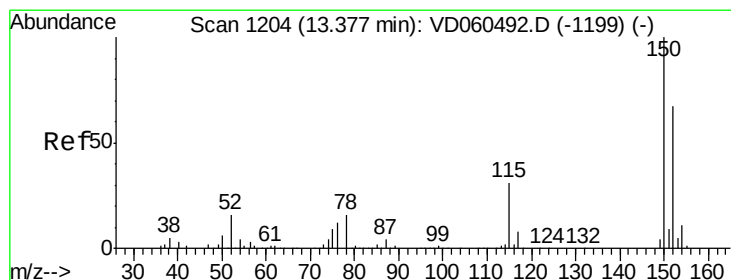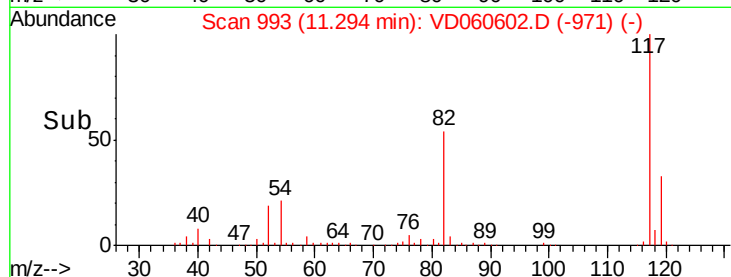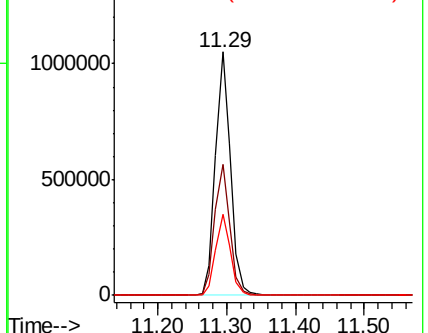

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.38 min Scan# 1205
Delta R.T. 0.00 min
Lab File: VD060602.D
Acq: 17 Dec 2018 16:30

Tgt Ion:152 Resp: 821831
Ion Ratio Lower Upper
152 100
115 50.4 24.6 74.0
150 152.4 0.0 309.0

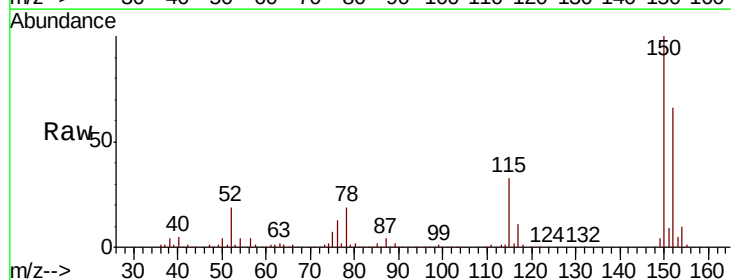

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

