
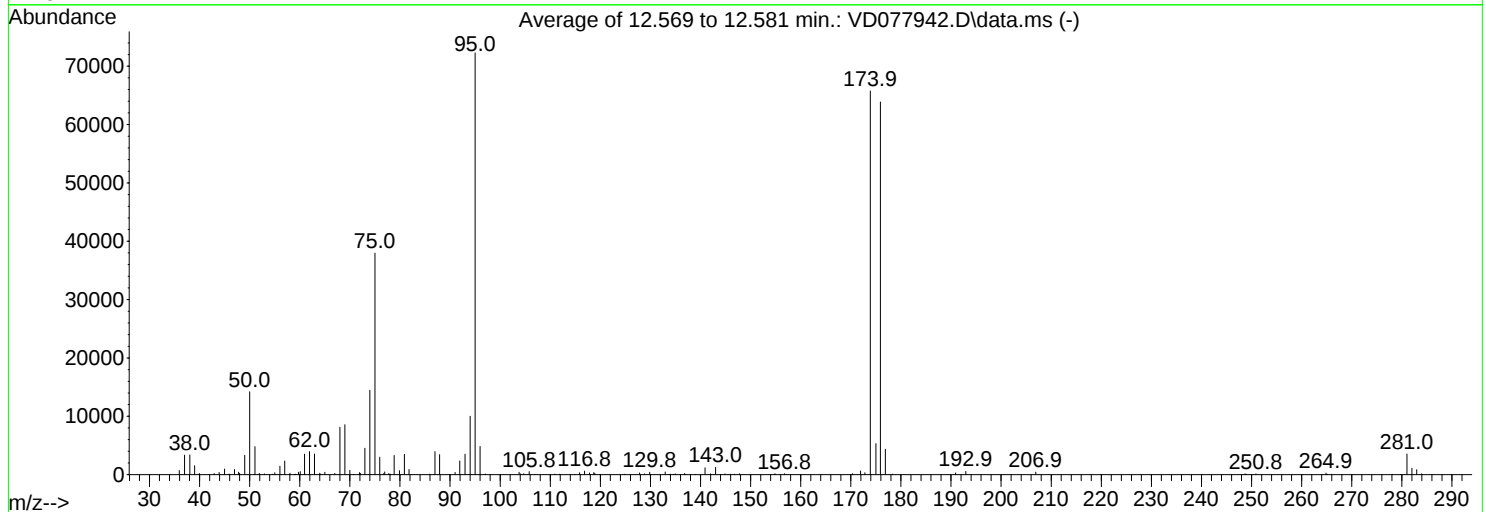


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121823\
Data File : VD077942.D
Acq On : 18 Dec 2023 11:22
Operator : RP/MD
Sample : BFB194
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB194

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM112923SMA.M
Title : SFAM01.0
Last Update : Mon Dec 18 23:16:23 2023

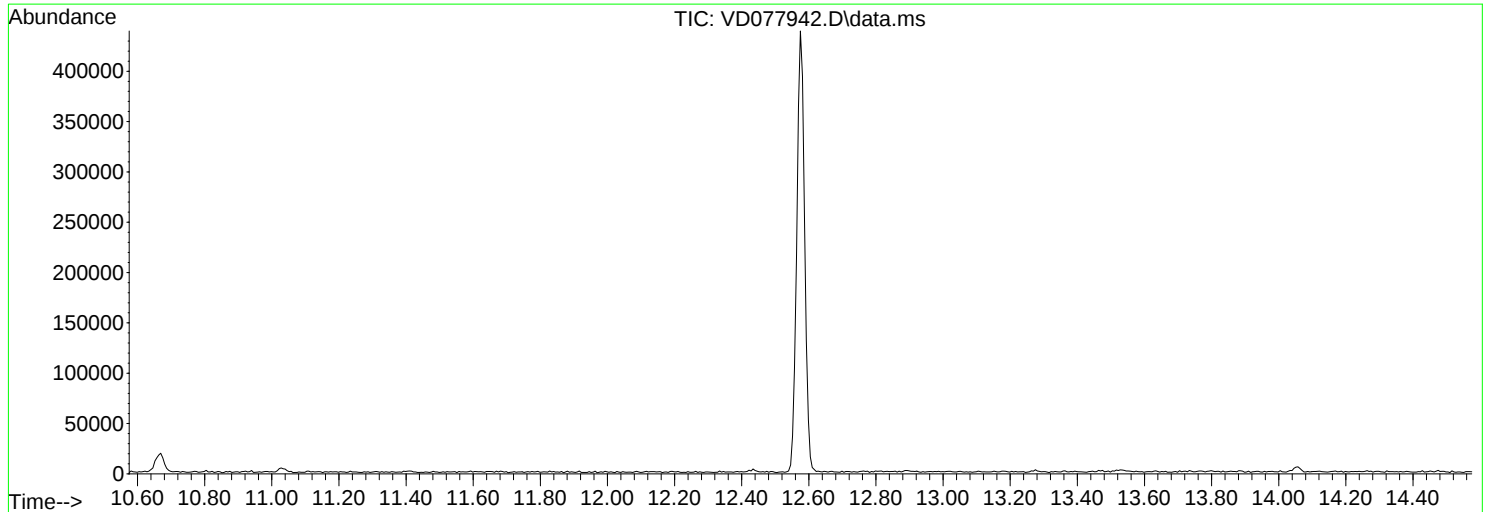

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	14208	PASS
75	95	30	80	52.5	37987	PASS
95	95	100	100	100.0	72293	PASS
96	95	5	9	6.7	4817	PASS
173	174	0.00	2	0.5	343	PASS
174	95	50	120	91.0	65768	PASS
175	174	5	9	8.1	5322	PASS
176	174	95	105	97.1	63867	PASS
177	176	5	10	6.8	4362	PASS

m/z	Abundance
39.90	648.0
42.00	183.0
43.90	657.0
75.90	187.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194

m/z	Abundance
35.90	807.0
37.00	3386.0
38.00	2759.0
39.00	1359.0
40.00	905.0
44.00	1252.0
45.00	923.0
47.00	806.0
47.80	557.0
49.00	2995.0
50.00	13060.0
51.10	4444.0
51.90	200.0
53.00	207.0
54.60	242.0
55.20	238.0
56.10	1421.0
57.00	2010.0
58.10	221.0
59.70	634.0
60.20	622.0
61.00	3906.0
62.00	4132.0
63.00	3960.0
64.00	296.0
65.00	262.0
67.00	200.0
68.00	7877.0
69.00	8701.0
70.00	799.0
71.90	512.0
73.00	4661.0
74.00	13842.0
75.00	36576.0
76.00	2831.0
76.70	482.0
77.00	411.0
78.10	254.0
78.80	3432.0
80.00	735.0
80.90	3789.0
81.80	692.0
87.00	3860.0
87.90	3712.0
91.00	364.0
92.00	2107.0
93.00	2928.0
94.00	9201.0
95.00	65888.0
96.00	3803.0
103.80	328.0
104.70	175.0
105.80	544.0
115.90	319.0
116.90	690.0
117.90	233.0
118.70	555.0
127.90	171.0
128.80	226.0
129.80	562.0
132.90	320.0
134.90	204.0
136.90	258.0
141.00	1190.0
143.00	1095.0
147.80	241.0
154.80	157.0
170.40	213.0
172.00	601.0
173.90	57664.0
175.00	4396.0
175.90	56000.0
176.90	4164.0
191.00	261.0
193.00	477.0
206.90	433.0
250.80	159.0
264.90	181.0
281.10	2405.0
282.00	600.0
283.10	504.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194

m/z	Abundance
36.00	771.0
37.00	3377.0
38.00	3980.0
39.00	1884.0
40.00	1001.0
42.90	376.0
43.90	1027.0
45.00	1141.0
46.90	922.0
47.80	664.0
49.00	3786.0
50.00	14742.0
51.10	5653.0
51.90	189.0
55.00	314.0
56.00	1572.0
57.00	2535.0
58.00	269.0
59.20	237.0
60.00	946.0
61.00	3814.0
61.90	3868.0
63.00	3614.0
64.00	474.0
65.00	371.0
67.00	222.0
68.00	9025.0
69.00	9009.0
70.10	669.0
71.90	586.0
73.00	4131.0
74.00	15525.0
75.00	40928.0
76.00	3168.0
76.90	498.0
78.90	3225.0
79.80	726.0
80.90	3763.0
81.80	1132.0
87.00	4125.0
87.90	3579.0
91.00	577.0
92.00	2658.0
93.00	4089.0
94.00	10802.0
95.00	82640.0
96.00	5895.0
97.00	180.0
103.90	489.0
104.60	160.0
105.70	558.0
106.90	163.0
110.90	250.0
111.90	281.0
114.90	199.0
115.80	259.0
116.90	521.0
117.90	348.0
118.90	660.0
127.80	417.0
129.90	296.0
132.00	170.0
133.00	615.0
134.00	266.0
135.00	213.0
136.70	345.0
139.00	175.0
140.90	990.0
142.00	290.0
143.00	1118.0
144.00	211.0
145.00	238.0
145.50	204.0
146.00	254.0
146.80	221.0
147.70	218.0
154.90	351.0
156.70	232.0
157.10	166.0
170.30	306.0
171.90	568.0
173.90	73320.0
175.00	5751.0
175.90	70864.0
176.90	5115.0
178.30	219.0
190.90	365.0
193.00	559.0
207.00	455.0
248.70	410.0
264.90	297.0
278.10	177.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194

279.70	177.0
281.10	3884.0
282.00	1122.0
283.00	713.0
284.00	155.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194

m/z	Abundance
36.00	587.0
37.00	3294.0
38.10	3400.0
39.00	1338.0
40.00	696.0
42.90	172.0
43.90	822.0
45.00	824.0
45.90	345.0
46.90	931.0
48.00	655.0
49.00	3190.0
50.00	14822.0
51.00	4313.0
51.90	237.0
52.90	212.0
54.90	425.0
56.10	1342.0
57.00	2434.0
58.00	261.0
58.90	171.0
59.80	640.0
60.90	2842.0
62.00	3876.0
62.90	3013.0
64.20	295.0
65.00	631.0
67.00	233.0
68.00	7490.0
69.00	7928.0
69.90	719.0
70.80	170.0
72.10	695.0
73.00	4769.0
74.00	13974.0
75.00	36456.0
76.00	3525.0
76.90	532.0
77.80	592.0
78.90	3184.0
79.90	630.0
80.90	2908.0
81.80	783.0
82.90	183.0
85.90	245.0
87.00	3842.0
87.90	3009.0
90.90	249.0
91.90	2278.0
93.00	3507.0
94.00	10010.0
95.00	68352.0
96.00	4752.0
97.10	152.0
103.70	427.0
104.10	453.0
104.80	174.0
105.90	497.0
115.80	452.0
116.80	573.0
117.70	309.0
118.70	541.0
124.90	291.0
127.90	290.0
128.80	192.0
129.90	411.0
133.00	494.0
133.70	214.0
134.60	169.0
137.00	171.0
140.80	1379.0
142.00	151.0
143.00	1590.0
144.80	184.0
156.80	280.0
171.90	728.0
172.80	1028.0
173.90	66320.0
175.00	5820.0
175.90	64736.0
176.90	3807.0
190.80	303.0
192.90	630.0
206.80	470.0
248.90	254.0
250.90	272.0
264.80	334.0
265.10	296.0
266.00	242.0
280.90	4298.0
282.00	1569.0
282.90	1330.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194

283.90

254.0

Instrument :
MSVOA_D
ClientSampleId :
BFB194