


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD121918\  
Data File : VD060630.D  
Acq On : 19 Dec 2018 9:53  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00g/5ml/MSVOA\_D/SOIL  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampled :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D120518S.M  
Title : SW846 8260  
Last Update : Thu Dec 06 01:49:20 2018

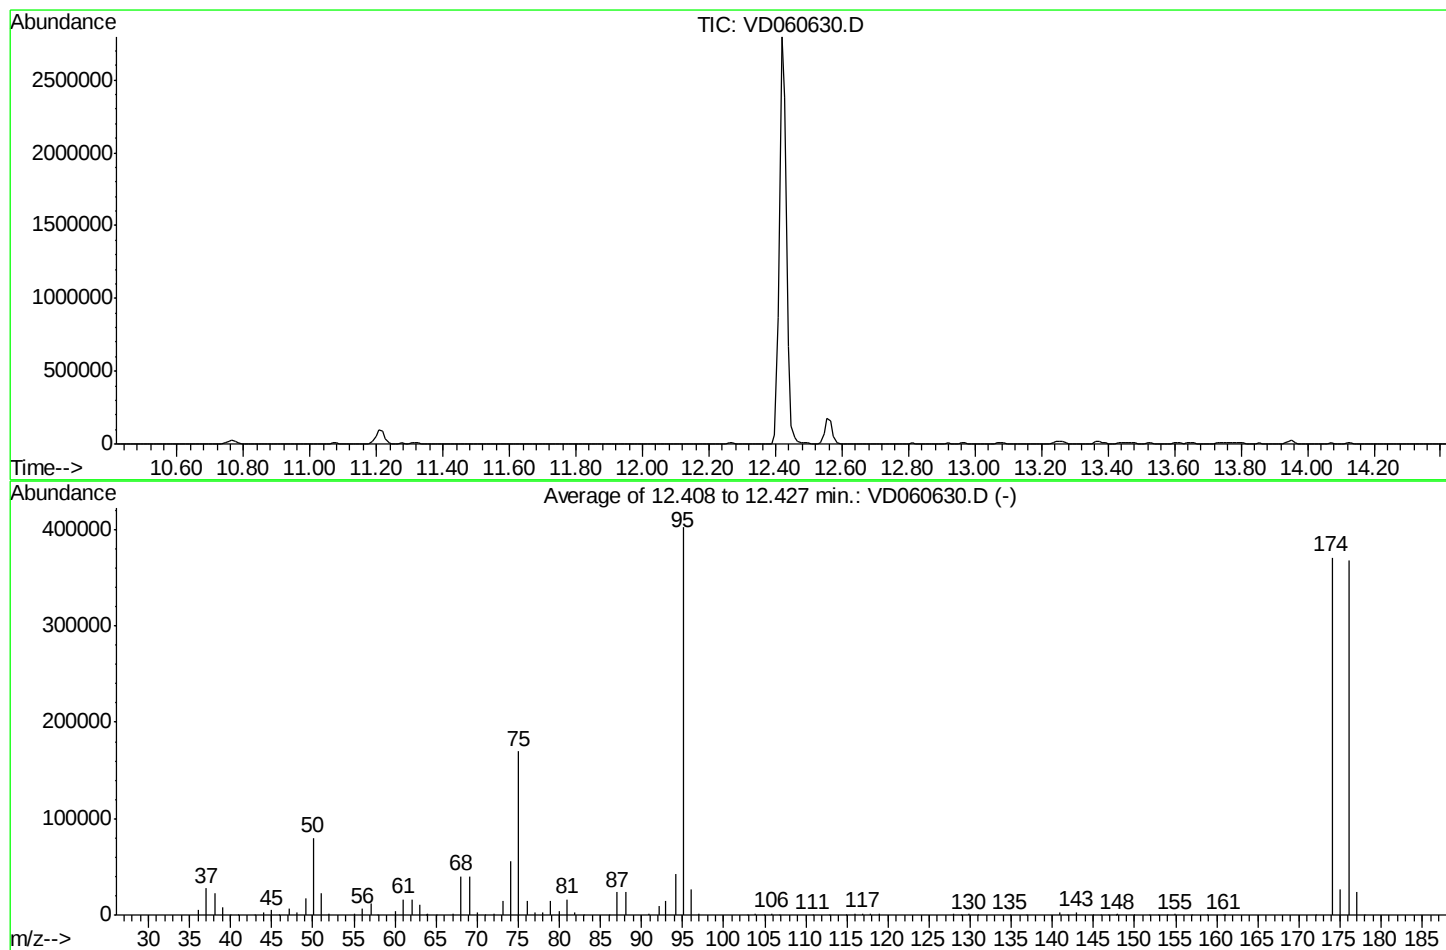

AutoFind: Scans 1106, 1107, 1108; Background Corrected with Scan 1102

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.8      | 79754   | PASS             |
| 75          | 95           | 30           | 60           | 42.2      | 169906  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 402282  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 26009   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 92.1      | 370634  | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 26689   | PASS             |
| 176         | 174          | 95           | 101          | 99.4      | 368584  | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 24053   | PASS             |