

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121923\
 Data File : VD077975.D
 Acq On : 19 Dec 2023 15:45
 Operator : RP/MD
 Sample : 05883-03
 Misc : 5.05G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EO-02-121523

Quant Time: Dec 20 02:05:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	169933	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	312151	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	284077	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	116597	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	75109	37.509	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	75.020%
35) Dibromofluoromethane	7.810	113	90318	41.307	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	82.620%
50) Toluene-d8	10.269	98	390737	44.619	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	89.240%
62) 4-Bromofluorobenzene	12.575	95	104607	39.954	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	79.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD121923\
Data File : VD077975.D
Acq On : 19 Dec 2023 15:45
Operator : RP/MD
Sample : 05883-03
Misc : 5.05G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EO-02-121523

Quant Time: Dec 20 02:05:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




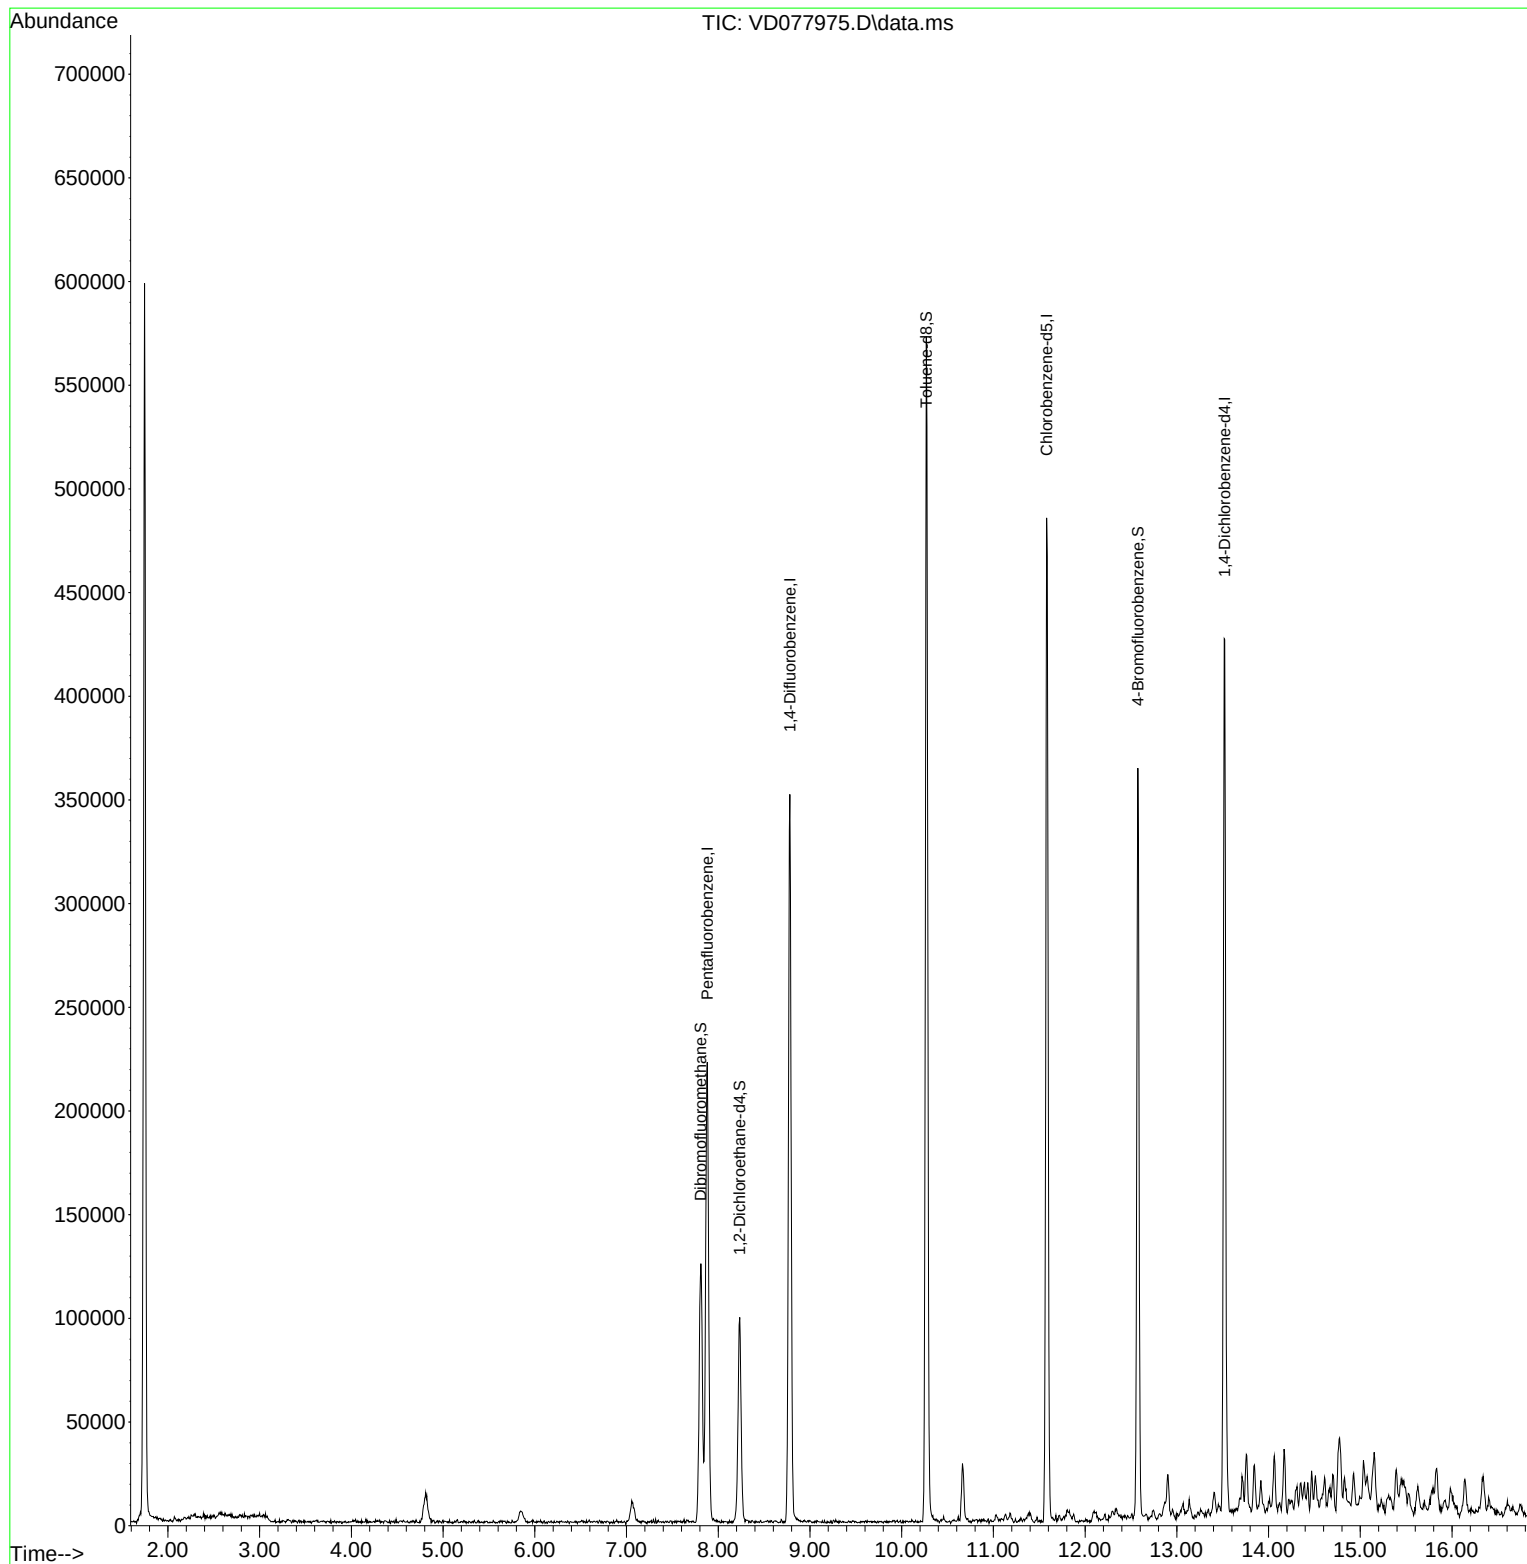


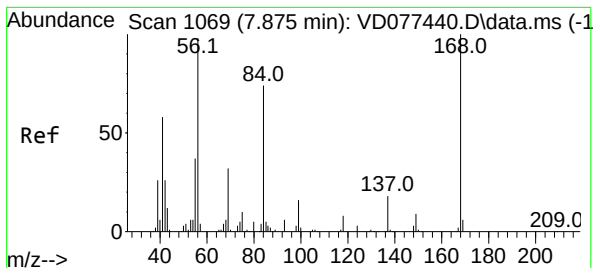

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 110
Delta R.T. 0.006 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45




Instrument :
MSVOA_D
ClientSampleId :
EO-02-121523


Tgt Ion:168 Resp: 169933
Ion Ratio Lower Upper
168 100
99 54.2 36.7 55.1

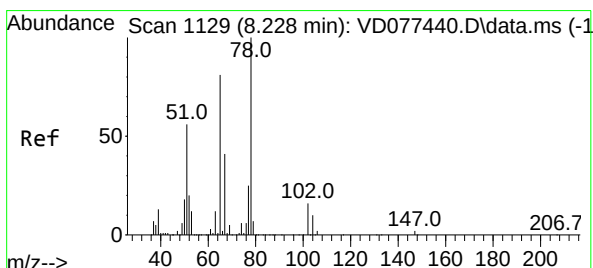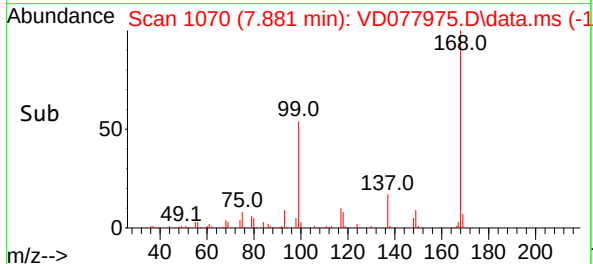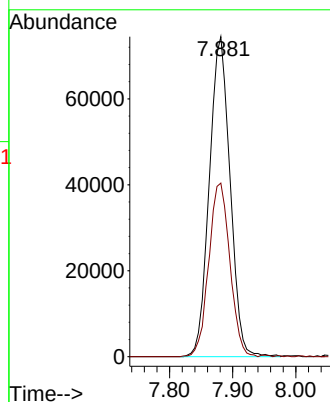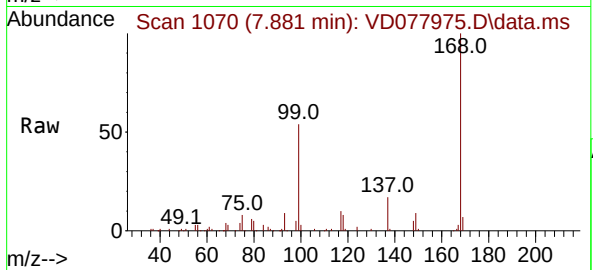

#33
1,2-Dichloroethane-d4
Concen: 37.509 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45

Tgt Ion: 65 Resp: 75109
Ion Ratio Lower Upper
65 100
67 56.1 0.0 115.0

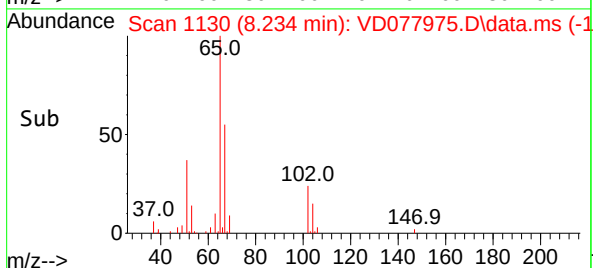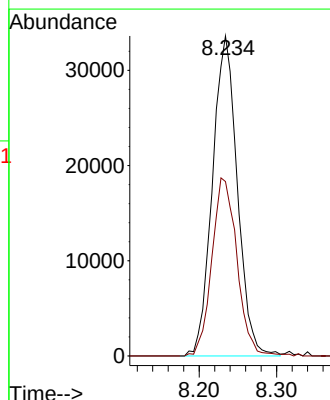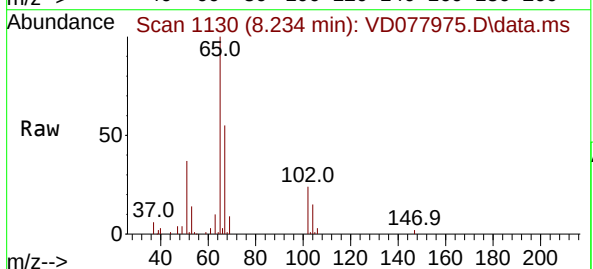

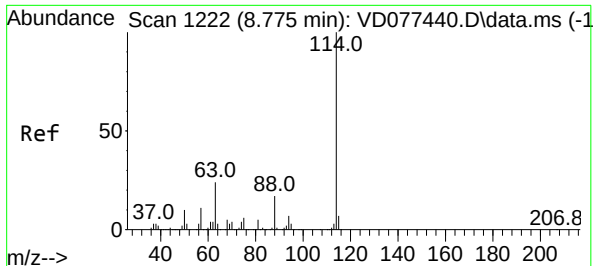

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD077975.D

Acq: 19 Dec 2023 15:45

Instrument :

MSVOA_D

ClientSampleId :

EO-02-121523





Tgt Ion:114 Resp: 312151

Ion Ratio Lower Upper

114 100

63 19.1 0.0 33.4

88 13.5 0.0 26.2

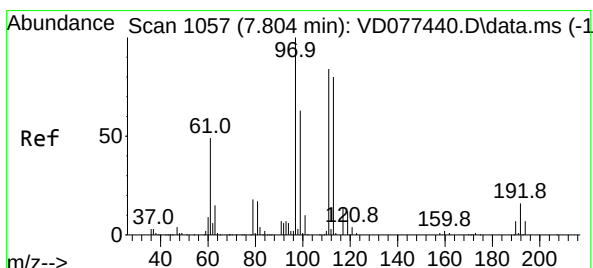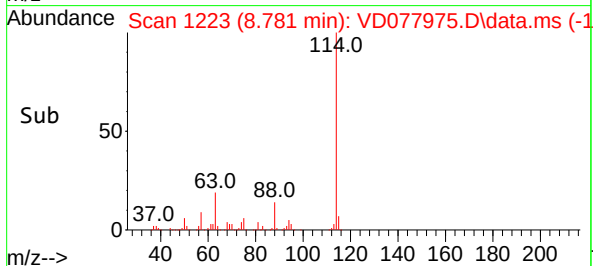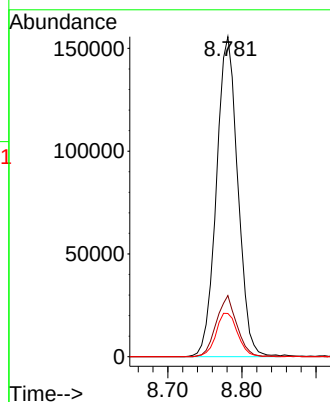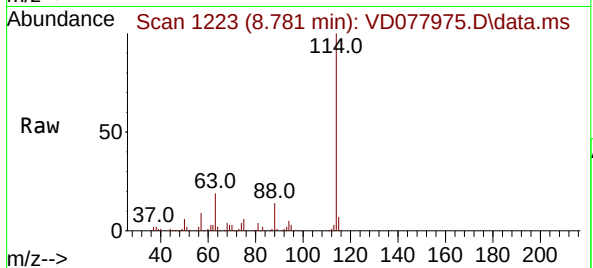

#35

Dibromofluoromethane

Concen: 41.307 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD077975.D

Acq: 19 Dec 2023 15:45




Tgt Ion:113 Resp: 90318


Ion Ratio Lower Upper

113 100

111 105.9 84.7 127.1

192 19.2 16.8 25.2


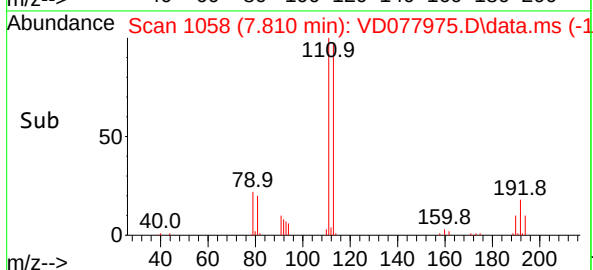
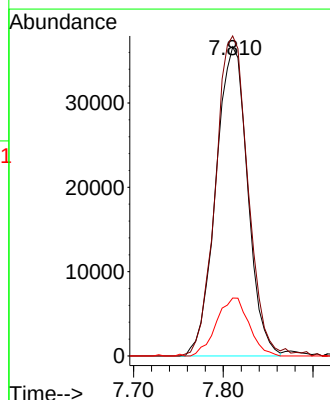
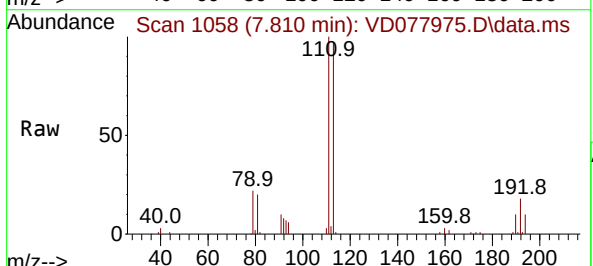


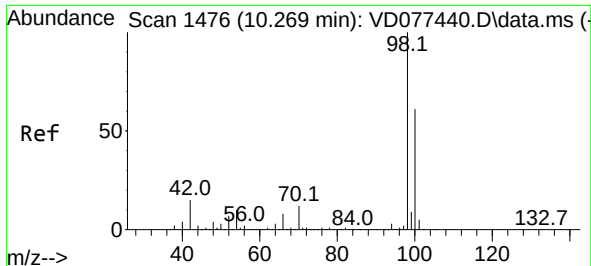

#50
Toluene-d8
Concen: 44.619 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45




Instrument :
MSVOA_D
ClientSampleId :
EO-02-121523


Tgt Ion: 98 Resp: 390737
Ion Ratio Lower Upper
98 100
100 63.4 50.3 75.5

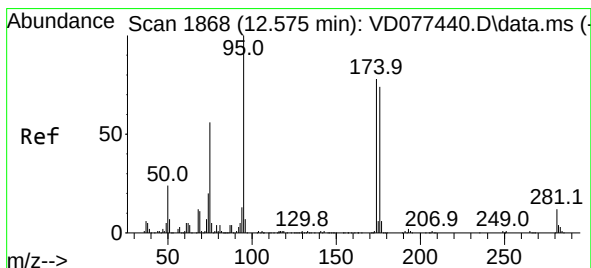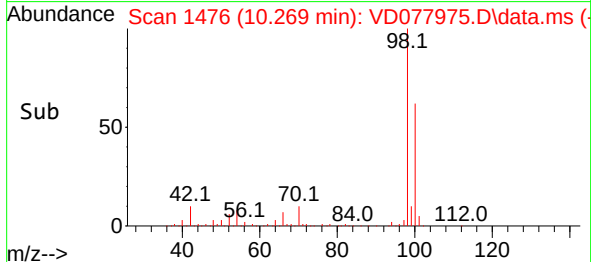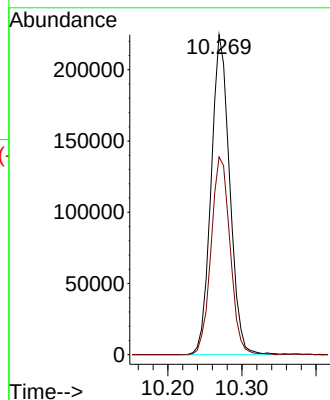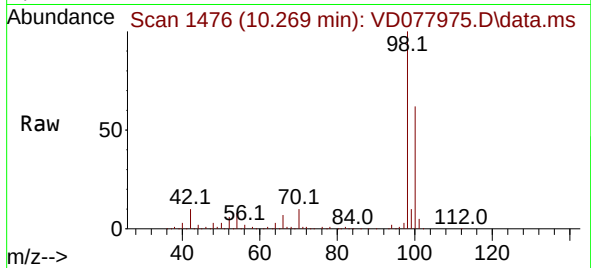

#62
4-Bromofluorobenzene
Concen: 39.954 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45

Tgt Ion: 95 Resp: 104607
Ion Ratio Lower Upper
95 100
174 92.2 0.0 201.8
176 85.7 0.0 191.8


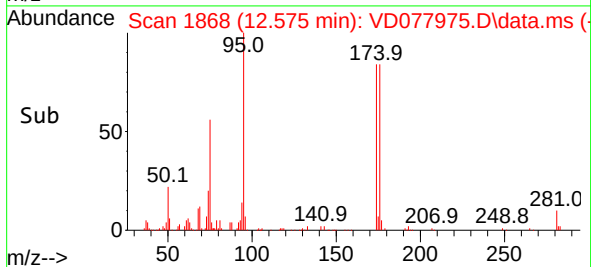
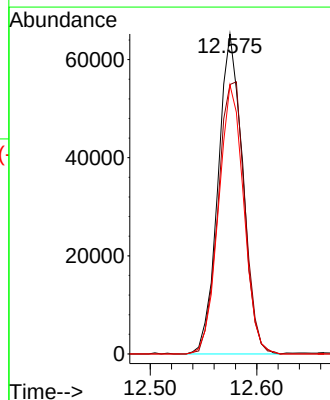
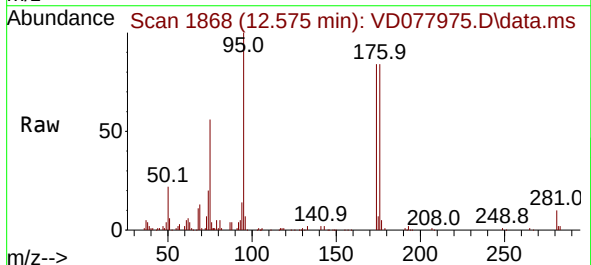


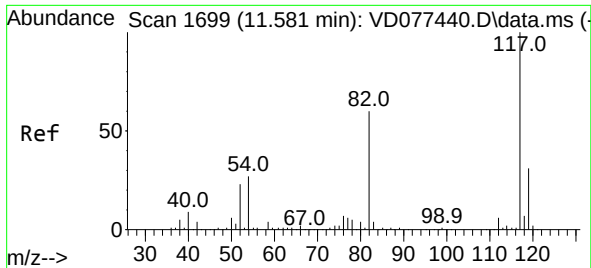

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45

Instrument :
MSVOA_D
ClientSampleId :
EO-02-121523

Tgt Ion:117 Resp: 284077
Ion Ratio Lower Upper
117 100
82 51.9 38.3 57.5
119 31.8 25.0 37.4

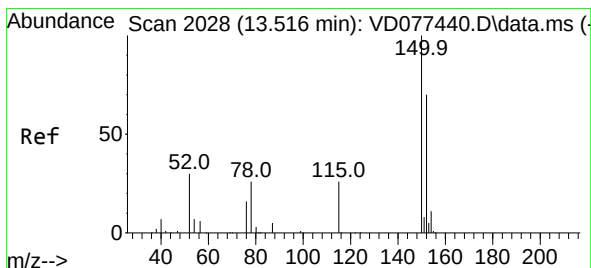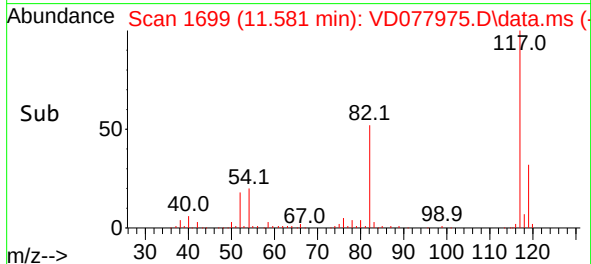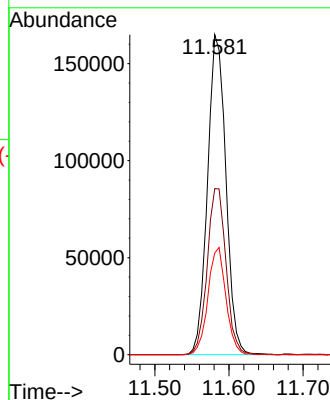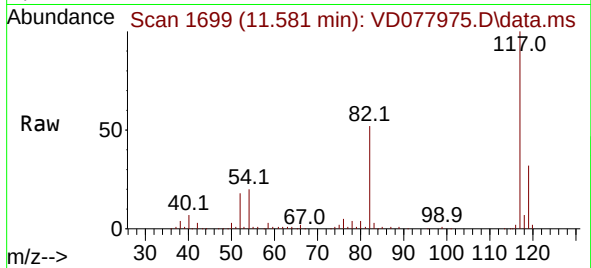

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD077975.D
Acq: 19 Dec 2023 15:45

Tgt Ion:152 Resp: 116597
Ion Ratio Lower Upper
152 100
115 56.0 27.1 81.3
150 154.8 0.0 353.6

