


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD122018\
Data File : VD060652.D
Acq On : 20 Dec 2018 9:45
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
Title : SW846 8260
Last Update : Fri Dec 21 17:37:47 2018

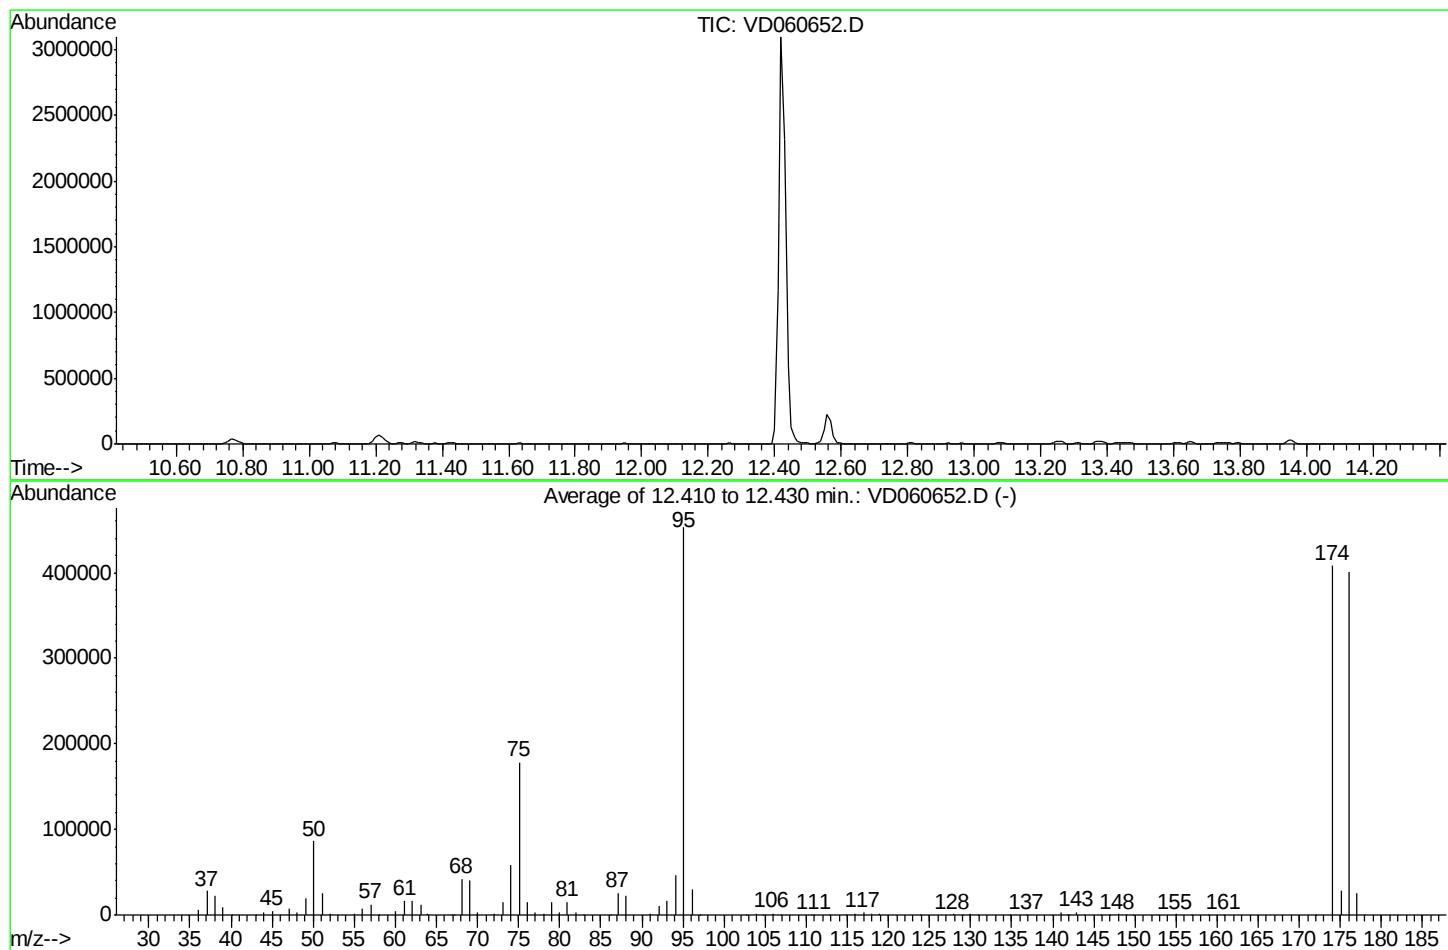

AutoFind: Scans 1208, 1209, 1210; Background Corrected with Scan 1203

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	86138	PASS
75	95	30	60	39.4	178570	PASS
95	95	100	100	100.0	452992	PASS
96	95	5	9	6.7	30314	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.1	408000	PASS
175	174	5	9	7.1	29112	PASS
176	174	95	101	98.4	401578	PASS
177	176	5	9	6.5	26005	PASS