

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
 Data File : VD077992.D
 Acq On : 20 Dec 2023 13:41
 Operator : RP/MD
 Sample : 05827-05RE
 Misc : 5.07G/5.0ml/MSVOA_D/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 RT-SB-08-13.5-14.5RE

Quant Time: Dec 21 05:23:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	167603	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	314127	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	297131	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	127790	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	77366	39.173	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	78.340%
35) Dibromofluoromethane	7.810	113	93874	42.663	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.320%
50) Toluene-d8	10.269	98	399000	45.276	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	90.560%
62) 4-Bromofluorobenzene	12.575	95	110964	42.115	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	84.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
Data File : VD077992.D
Acq On : 20 Dec 2023 13:41
Operator : RP/MD
Sample : 05827-05RE
Misc : 5.07G/5.0ml/MSVOA_D/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
RT-SB-08-13.5-14.5RE

Quant Time: Dec 21 05:23:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration

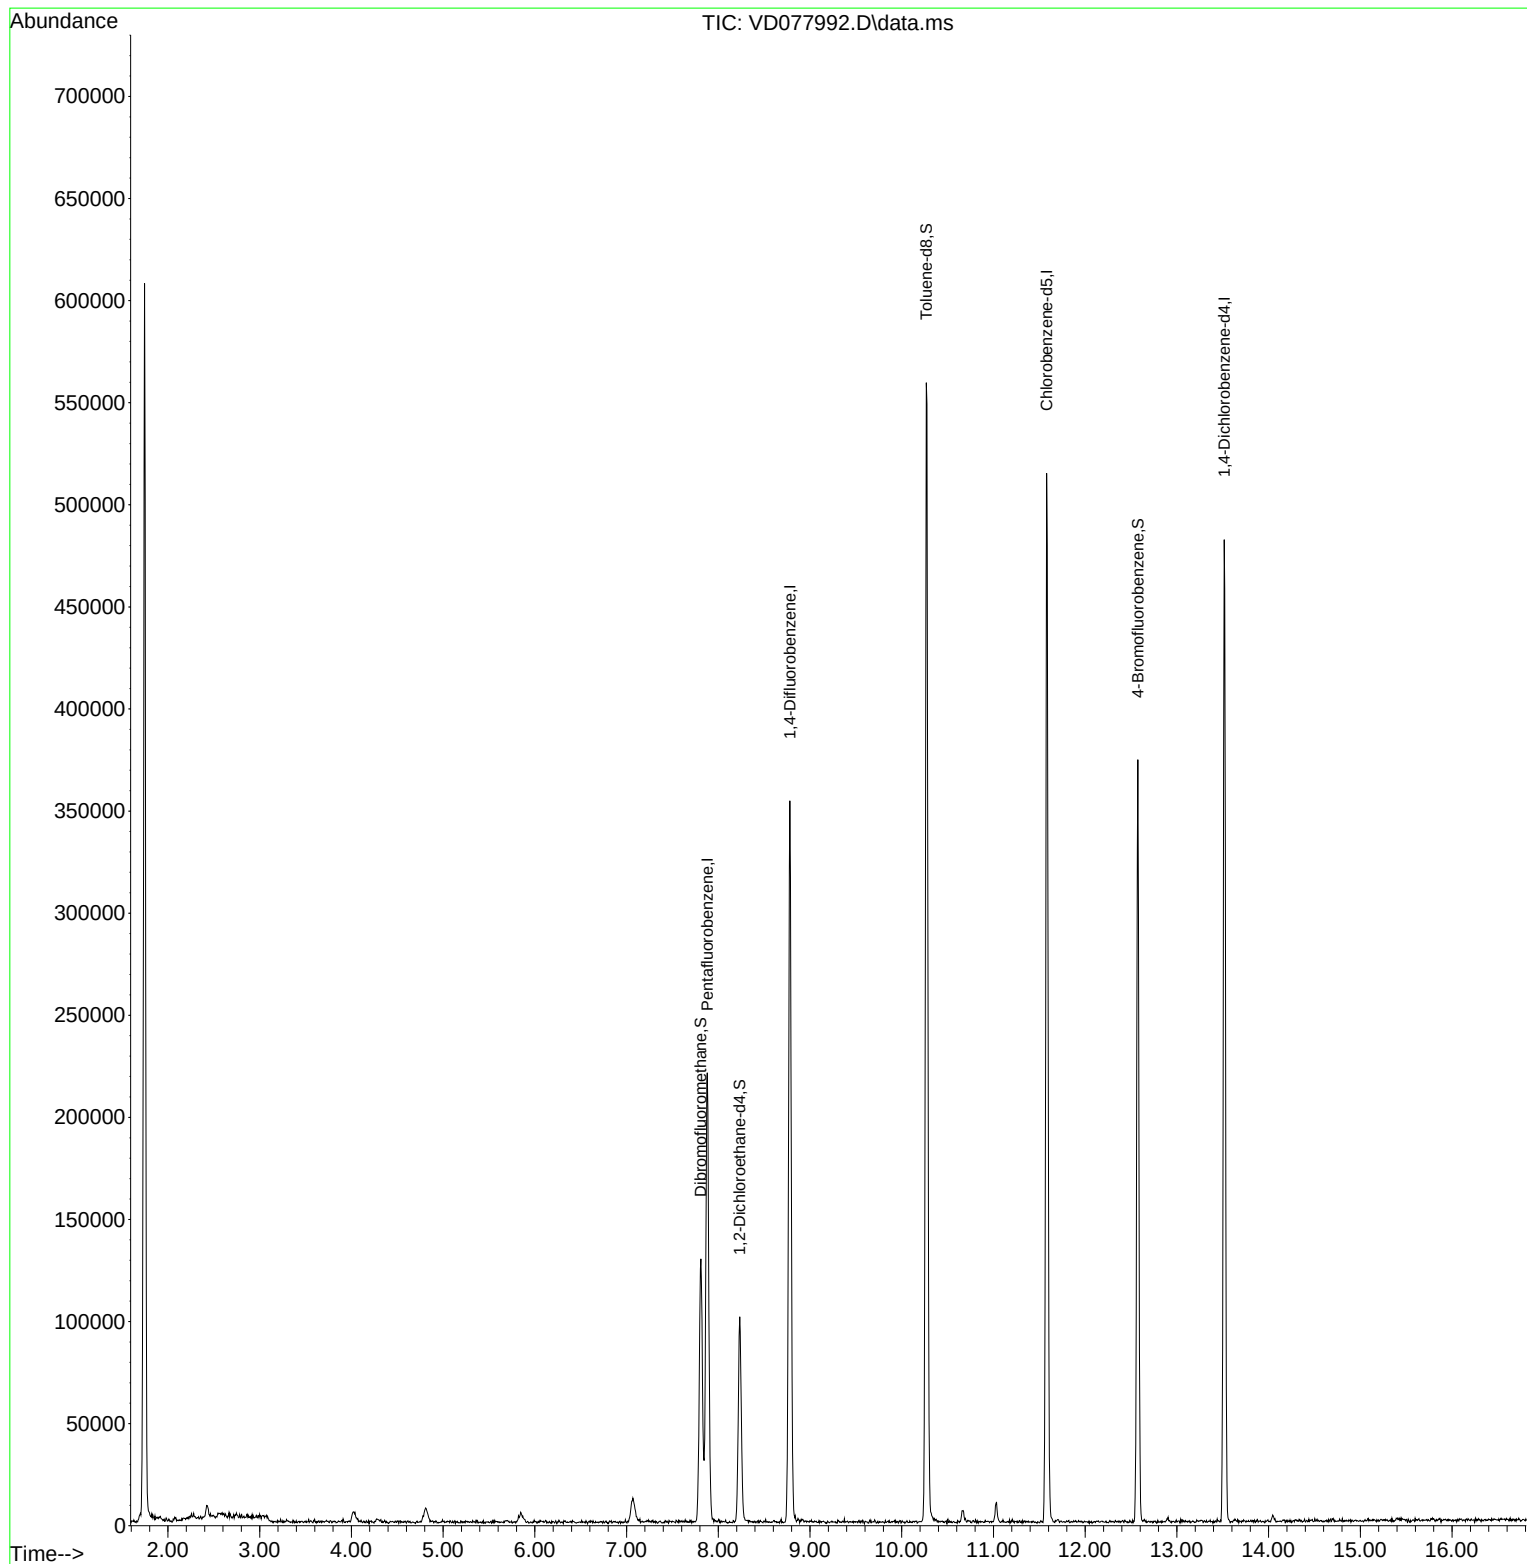

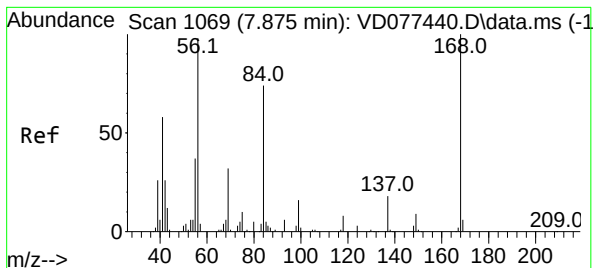

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.881 min Scan# 1107

Delta R.T. 0.006 min

Lab File: VD077992.D

Acq: 20 Dec 2023 13:41

Instrument :

MSVOA_D

ClientSampleId :





RT-SB-08-13.5-14.5RE

Tgt Ion:168 Resp: 167603

Ion Ratio Lower Upper

168 100

99 49.5 36.7 55.1

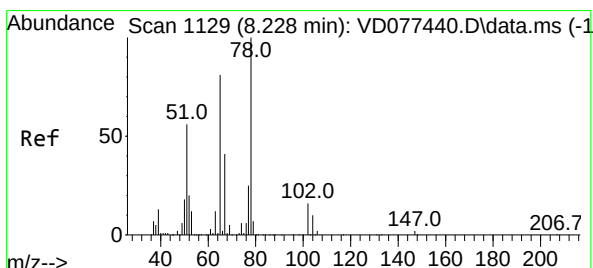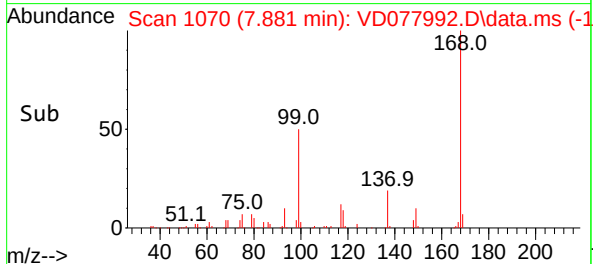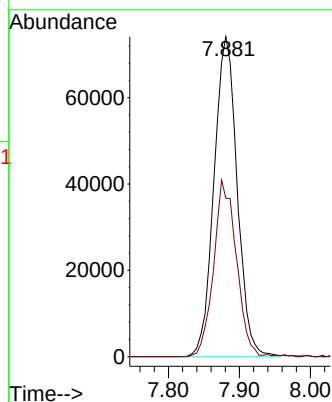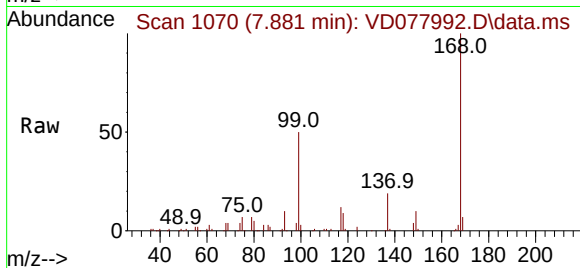

#33

1,2-Dichloroethane-d4

Concen: 39.173 ug/l

RT: 8.234 min Scan# 1130

Delta R.T. 0.006 min

Lab File: VD077992.D




Acq: 20 Dec 2023 13:41


Tgt Ion: 65 Resp: 77366

Ion Ratio Lower Upper

65 100

67 54.3 0.0 115.0

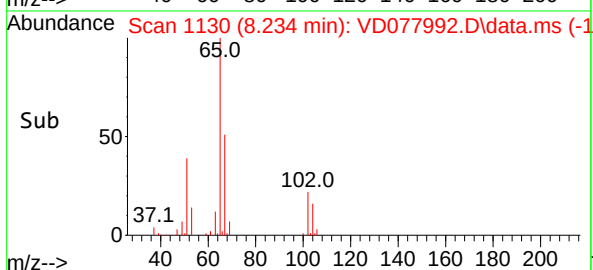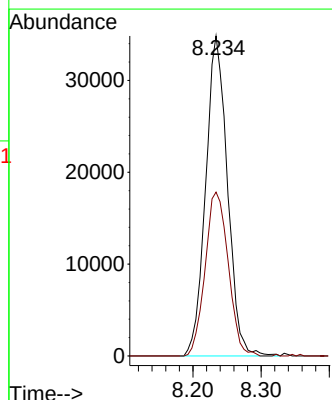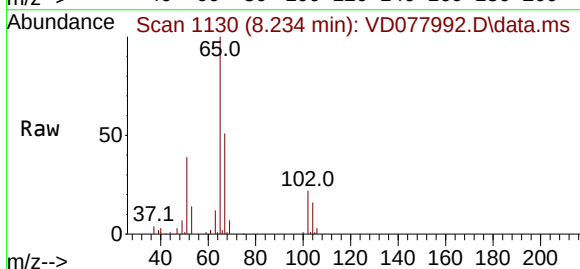

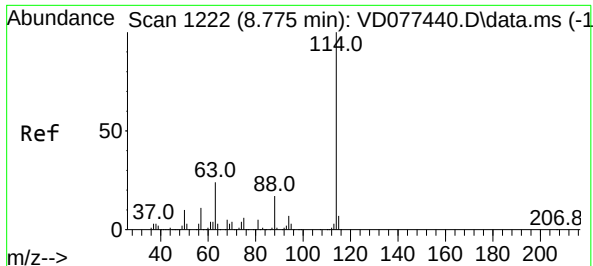

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD077992.D

Acq: 20 Dec 2023 13:41

Instrument :

MSVOA_D

ClientSampleId :

RT-SB-08-13.5-14.5RE





Tgt Ion:114 Resp: 314127

Ion Ratio Lower Upper

114 100

63 17.9 0.0 33.4

88 14.0 0.0 26.2

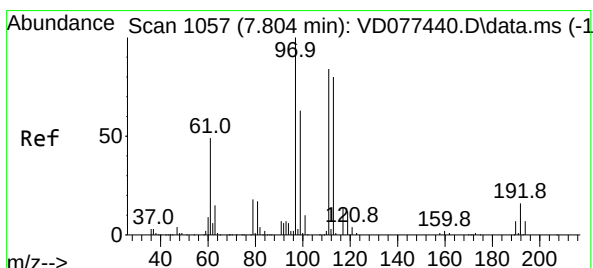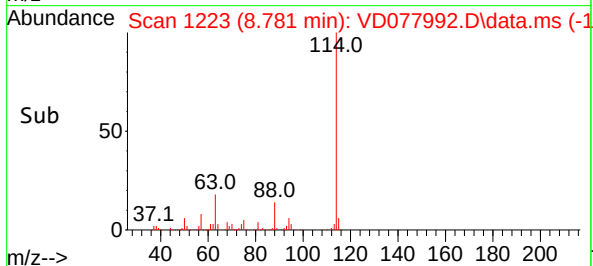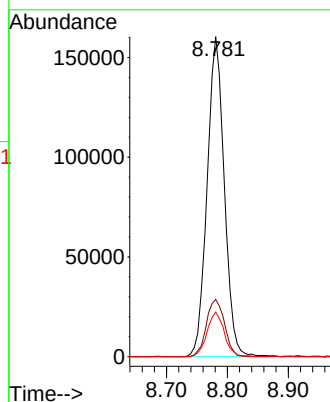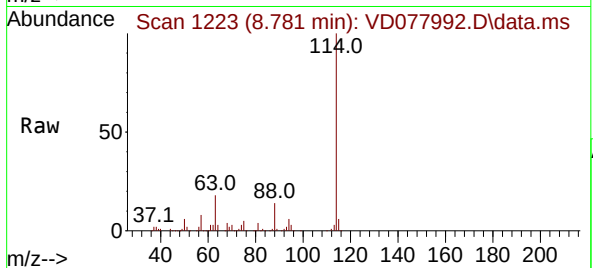

#35

Dibromofluoromethane

Concen: 42.663 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD077992.D

Acq: 20 Dec 2023 13:41




Tgt Ion:113 Resp: 93874


Ion Ratio Lower Upper

113 100

111 101.8 84.7 127.1

192 19.2 16.8 25.2


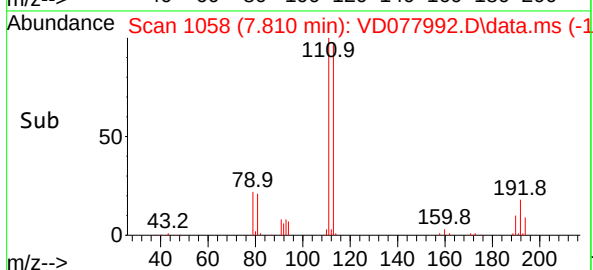
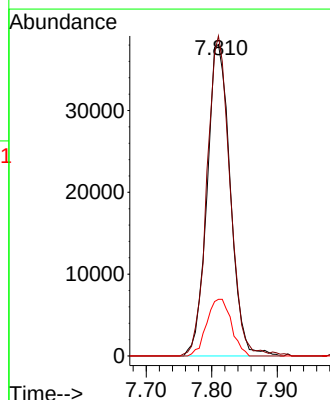
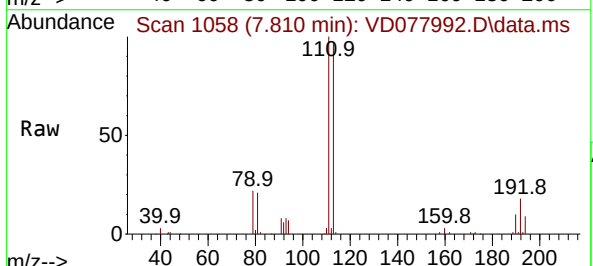


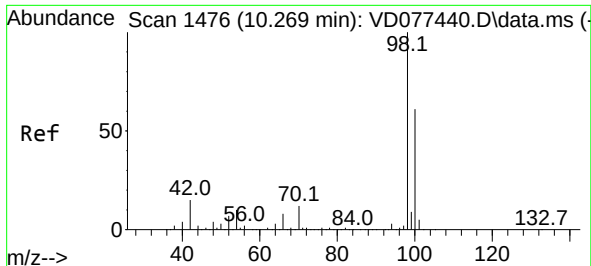

#50
Toluene-d8
Concen: 45.276 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD077992.D
Acq: 20 Dec 2023 13:41




Instrument :
MSVOA_D
ClientSampleId :
RT-SB-08-13.5-14.5RE


Tgt Ion: 98 Resp: 399000
Ion Ratio Lower Upper
98 100
100 63.6 50.3 75.5

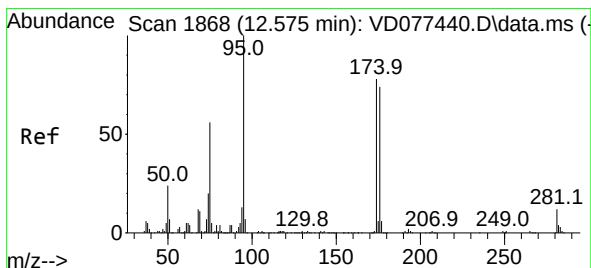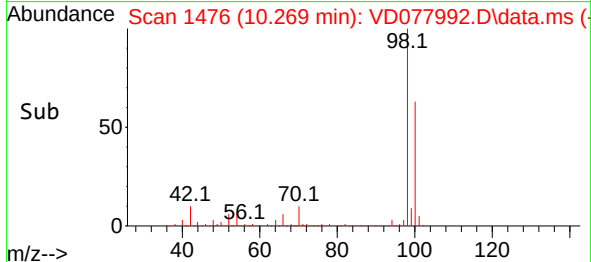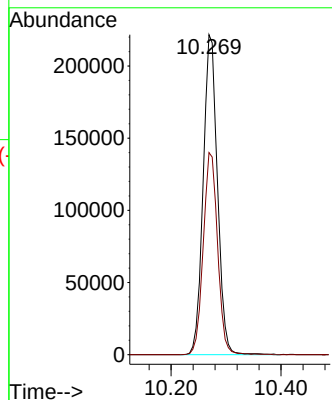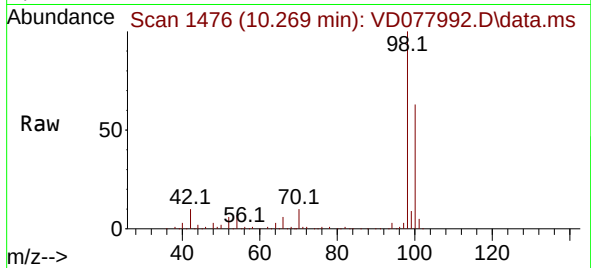

#62
4-Bromofluorobenzene
Concen: 42.115 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD077992.D
Acq: 20 Dec 2023 13:41

Tgt Ion: 95 Resp: 110964
Ion Ratio Lower Upper
95 100
174 90.2 0.0 201.8
176 87.1 0.0 191.8


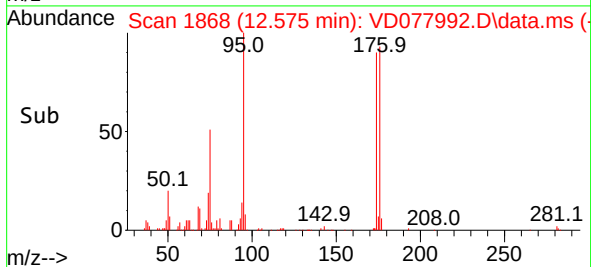
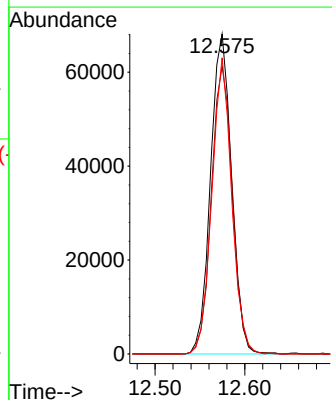
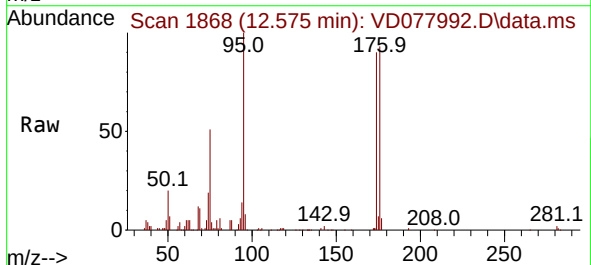


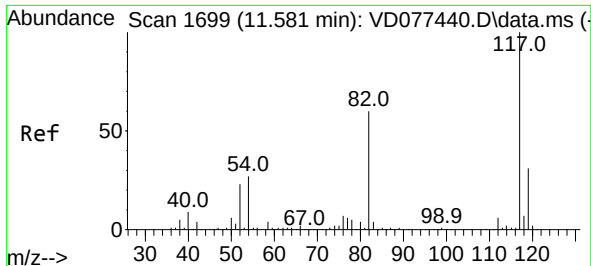

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD077992.D
Acq: 20 Dec 2023 13:41

Instrument :
MSVOA_D
ClientSampleId :
RT-SB-08-13.5-14.5RE

Tgt Ion:117 Resp: 297131
Ion Ratio Lower Upper
117 100
82 51.4 38.3 57.5
119 29.9 25.0 37.4

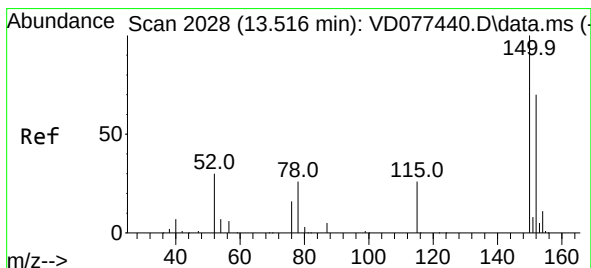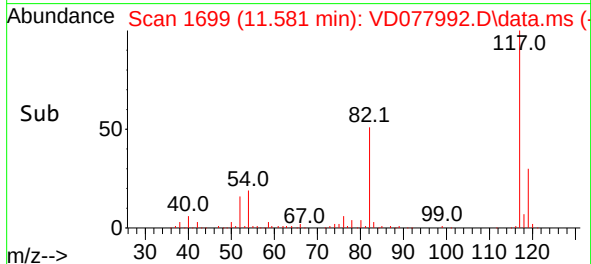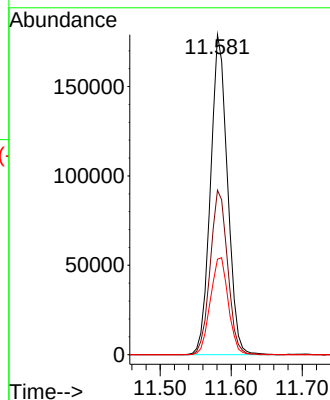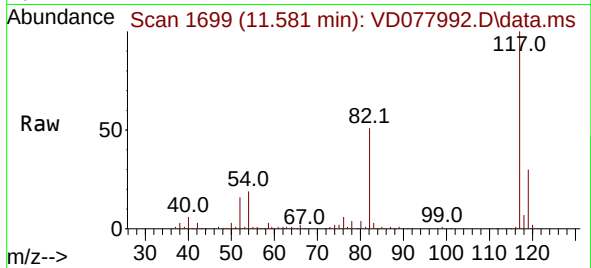

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD077992.D
Acq: 20 Dec 2023 13:41

Tgt Ion:152 Resp: 127790
Ion Ratio Lower Upper
152 100
115 57.2 27.1 81.3
150 158.0 0.0 353.6

