

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
 Data File : VD078000.D
 Acq On : 20 Dec 2023 17:16
 Operator : RP/MD
 Sample : 05796-04RE
 Misc : 5.03G/5.0ml/MSVOA_D/SOIL/B
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 RT-SB-04-13-14RE

Quant Time: Dec 21 05:26:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	161068	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	290803	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	257879	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	79764	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	77584	40.878	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	81.760%
35) Dibromofluoromethane	7.810	113	87379	42.896	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.800%
50) Toluene-d8	10.269	98	357968	43.877	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	87.760%
62) 4-Bromofluorobenzene	12.575	95	90182	36.973	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	73.940%


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
Data File : VD078000.D
Acq On : 20 Dec 2023 17:16
Operator : RP/MD
Sample : 05796-04RE
Misc : 5.03G/5.0ml/MSVOA_D/SOIL/B
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
RT-SB-04-13-14RE

Quant Time: Dec 21 05:26:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




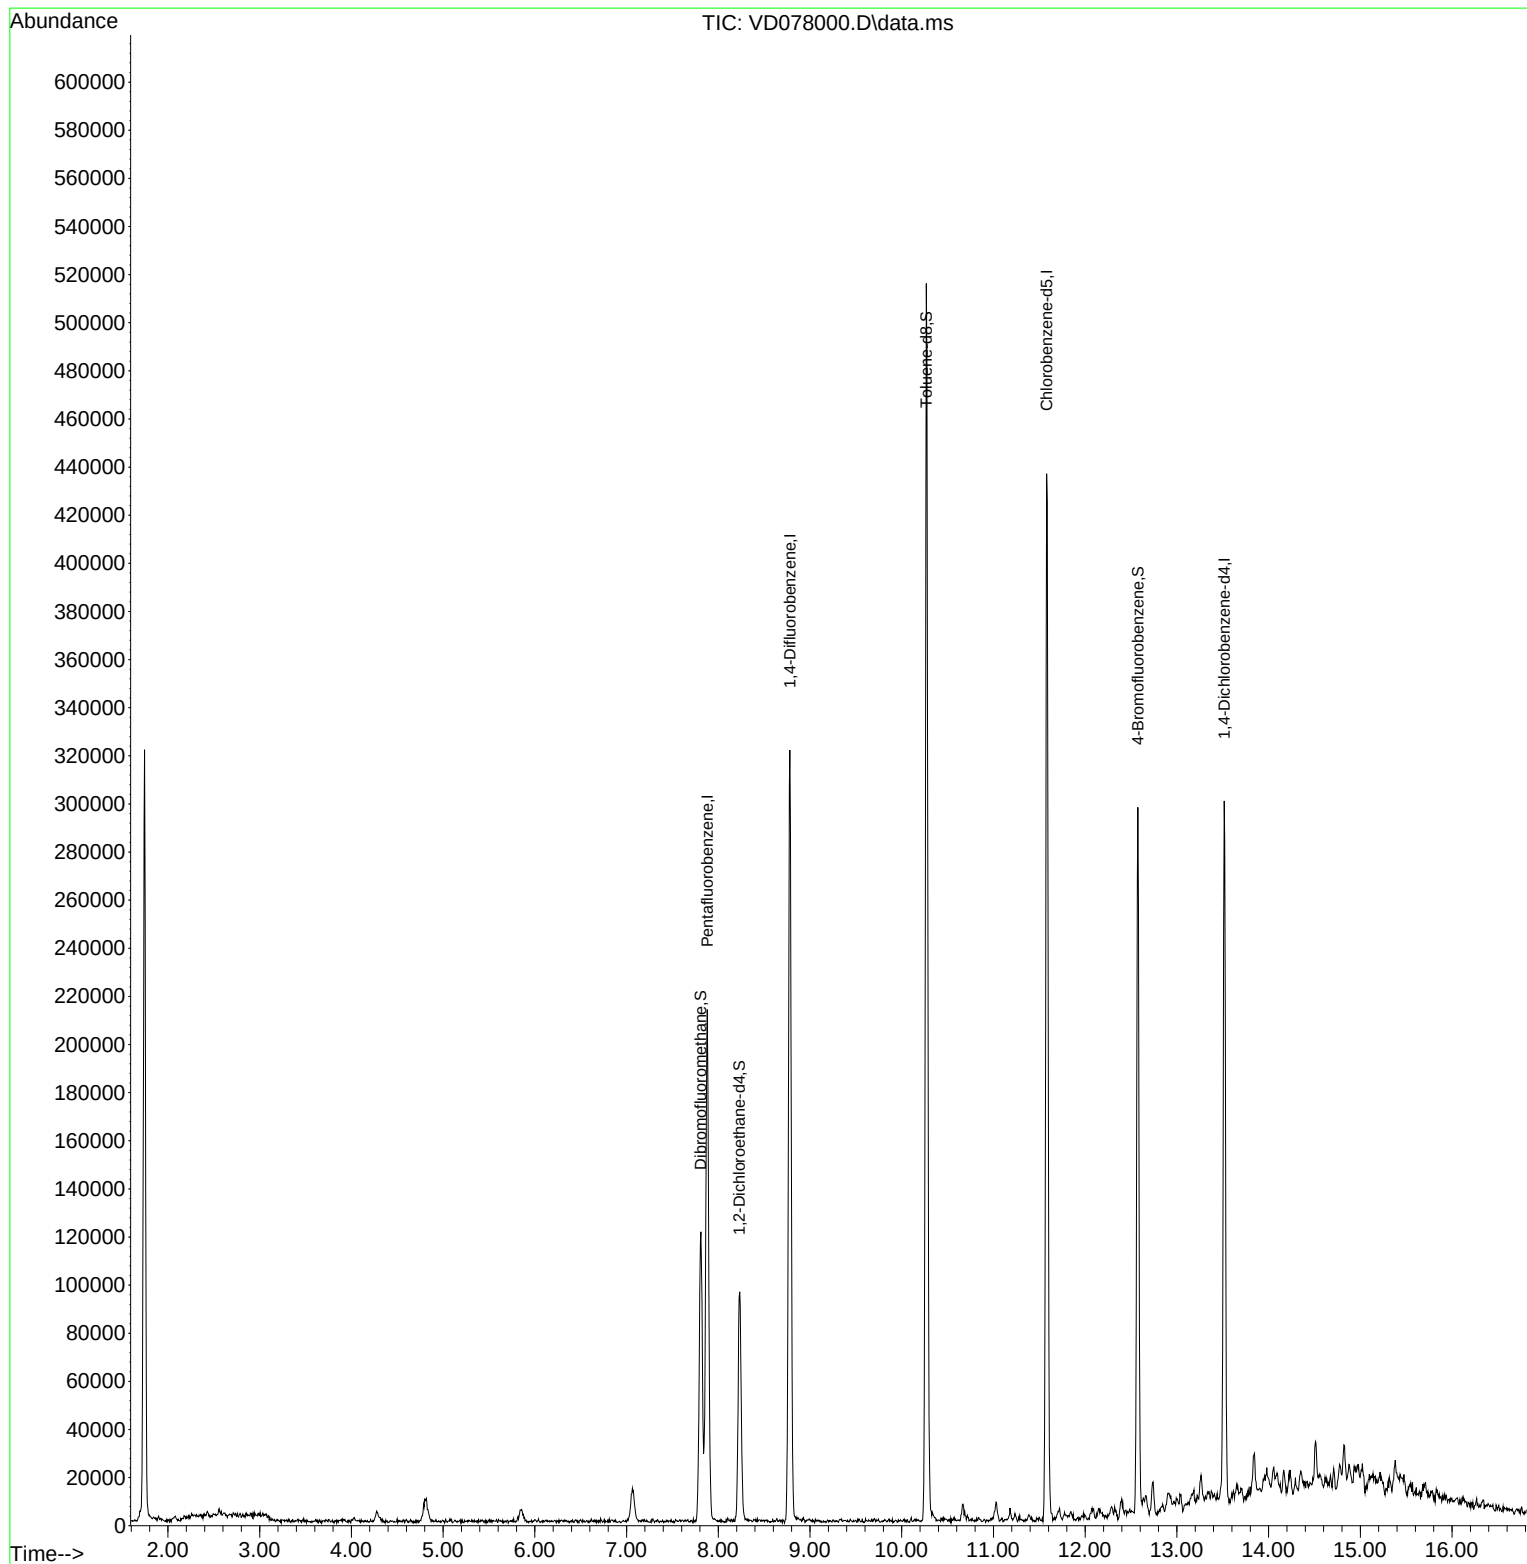


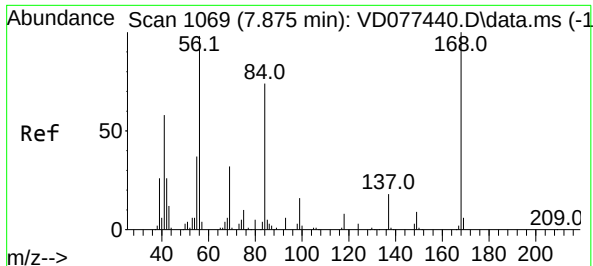

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16




Instrument :
MSVOA_D
ClientSampleId :
RT-SB-04-13-14RE


Tgt Ion:168 Resp: 161068
Ion Ratio Lower Upper
168 100
99 51.3 36.7 55.1

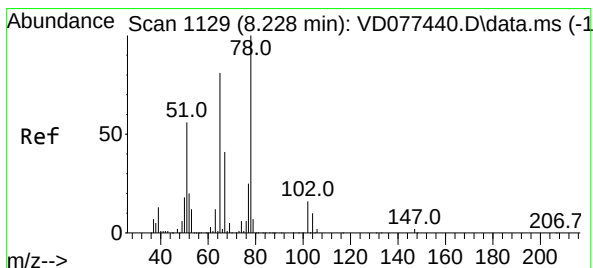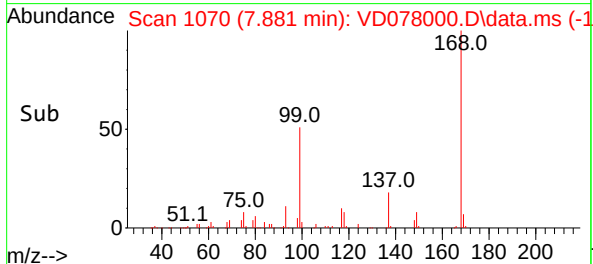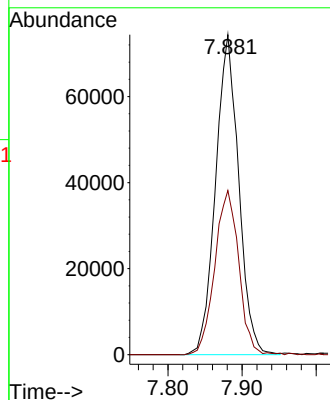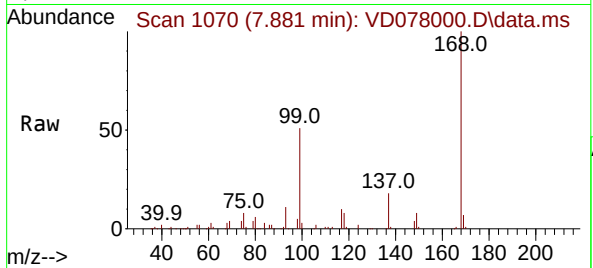

#33
1,2-Dichloroethane-d4
Concen: 40.878 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16

Tgt Ion: 65 Resp: 77584
Ion Ratio Lower Upper
65 100
67 53.7 0.0 115.0

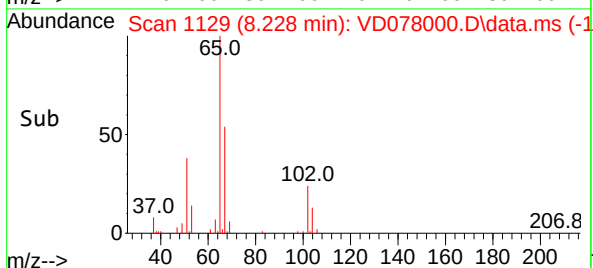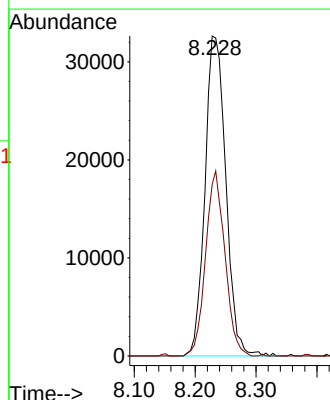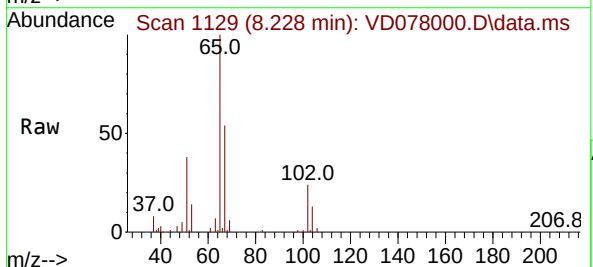

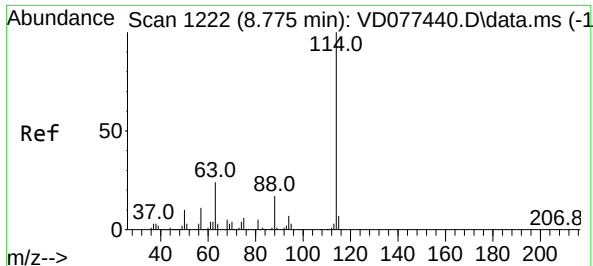

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 114

Delta R.T. 0.006 min

Lab File: VD078000.D

Acq: 20 Dec 2023 17:16

Instrument :

MSVOA_D

ClientSampleId :

RT-SB-04-13-14RE





Tgt Ion:114 Resp: 290803

Ion Ratio Lower Upper

114 100

63 18.5 0.0 33.4

88 13.5 0.0 26.2

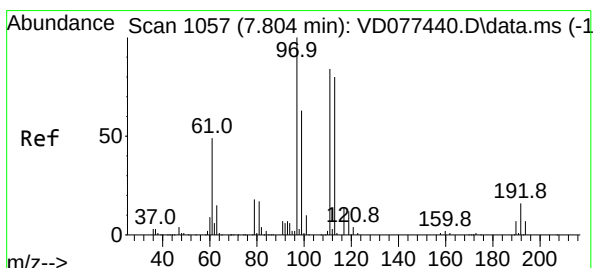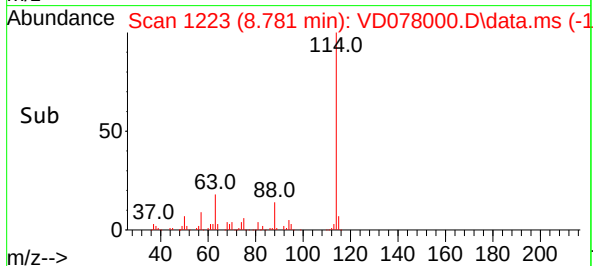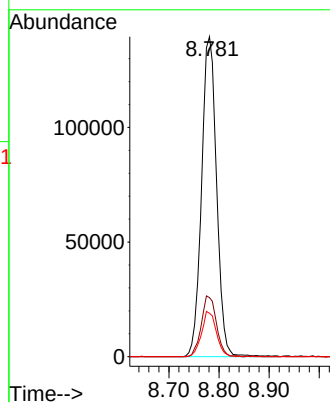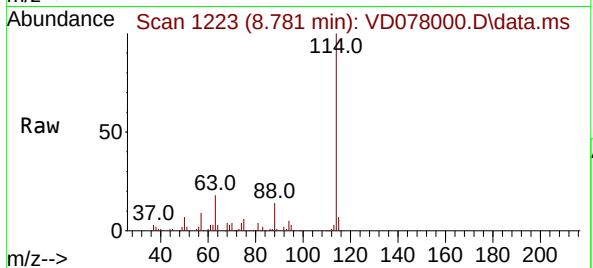

#35

Dibromofluoromethane

Concen: 42.896 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078000.D

Acq: 20 Dec 2023 17:16




Tgt Ion:113 Resp: 87379


Ion Ratio Lower Upper

113 100

111 103.6 84.7 127.1

192 18.3 16.8 25.2


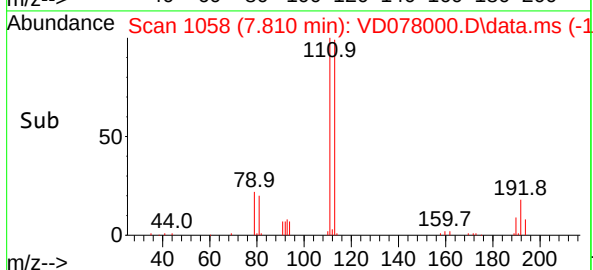
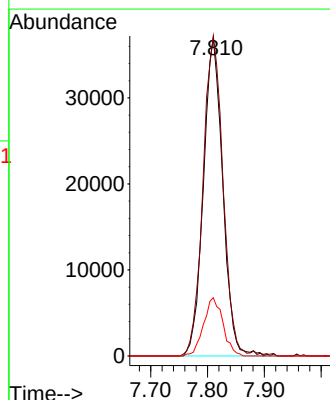
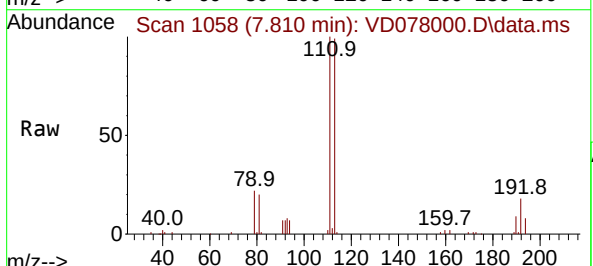


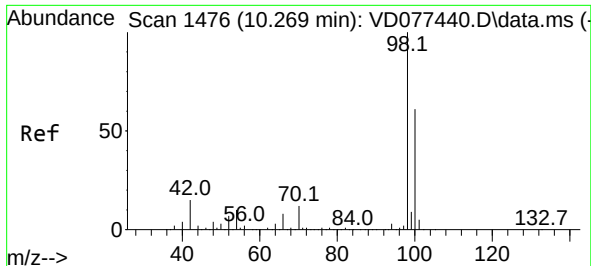

#50
Toluene-d8
Concen: 43.877 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16




Instrument :
MSVOA_D
ClientSampleId :
RT-SB-04-13-14RE


Tgt Ion: 98 Resp: 357968
Ion Ratio Lower Upper
98 100
100 63.5 50.3 75.5

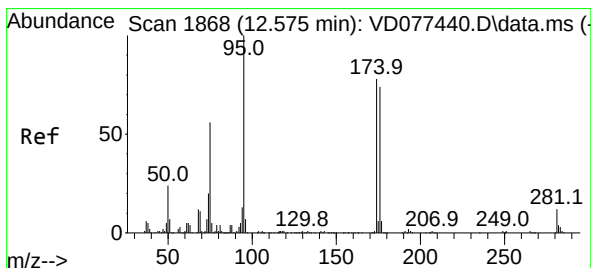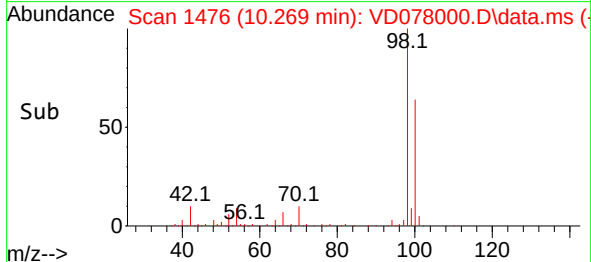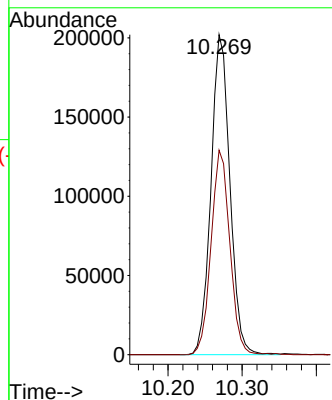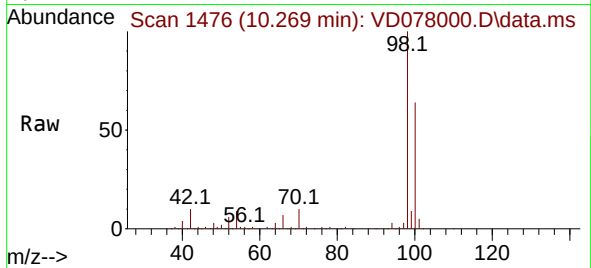

#62
4-Bromofluorobenzene
Concen: 36.973 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16

Tgt Ion: 95 Resp: 90182
Ion Ratio Lower Upper
95 100
174 85.6 0.0 201.8
176 86.4 0.0 191.8


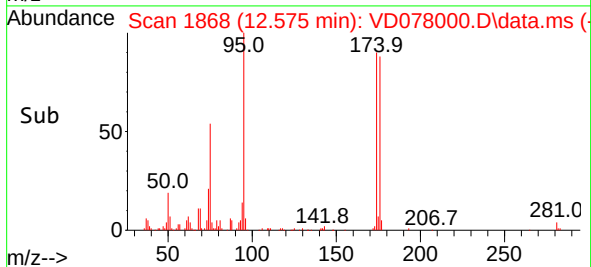
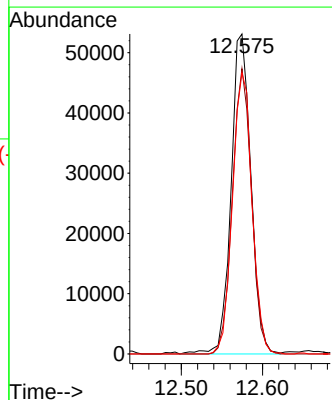
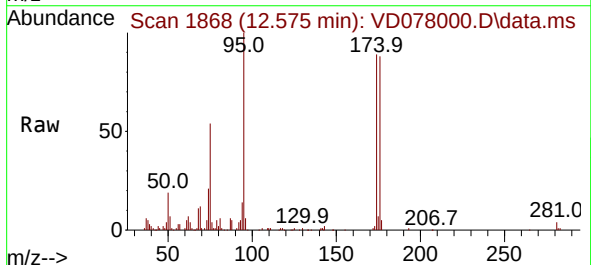


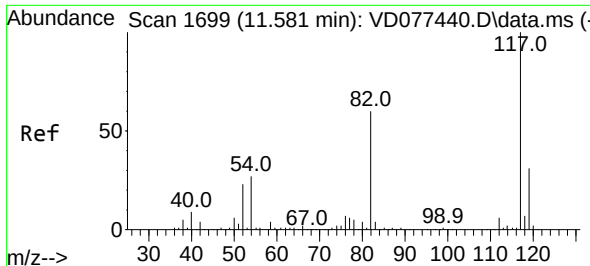

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16

Instrument :
MSVOA_D
ClientSampleId :
RT-SB-04-13-14RE

Tgt Ion:117 Resp: 257879
Ion Ratio Lower Upper
117 100
82 54.1 38.3 57.5
119 31.3 25.0 37.4

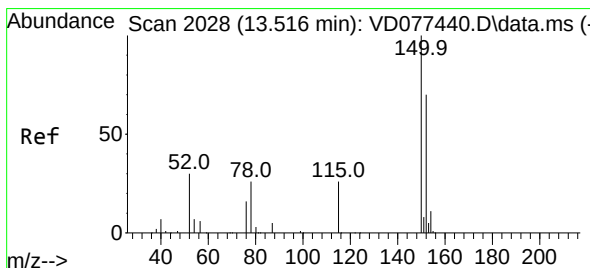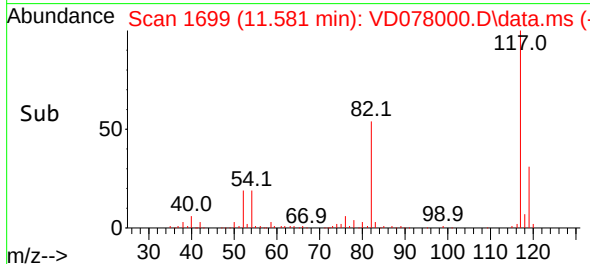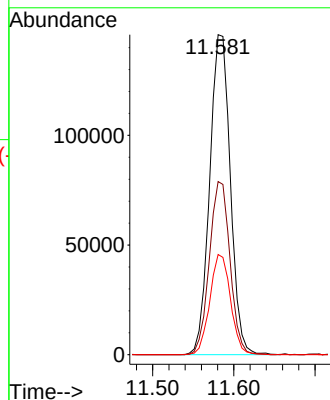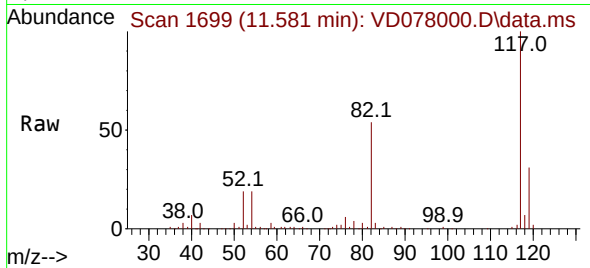

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD078000.D
Acq: 20 Dec 2023 17:16

Tgt Ion:152 Resp: 79764
Ion Ratio Lower Upper
152 100
115 57.5 27.1 81.3
150 155.7 0.0 353.6

