
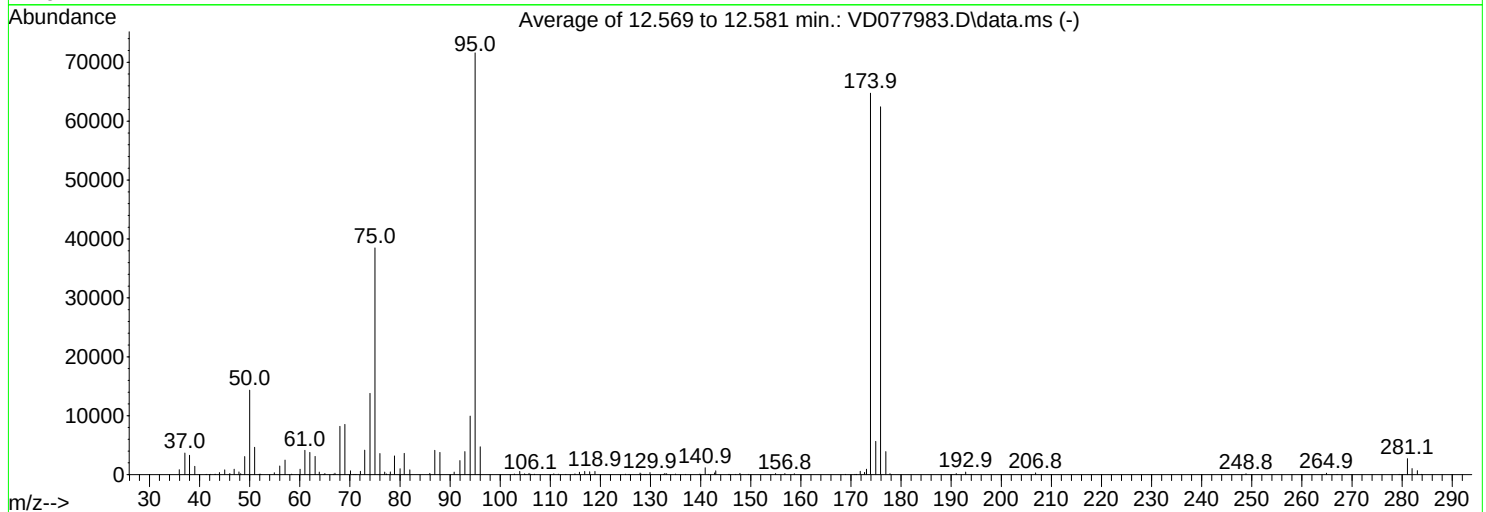


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
Data File : VD077983.D
Acq On : 20 Dec 2023 08:48
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

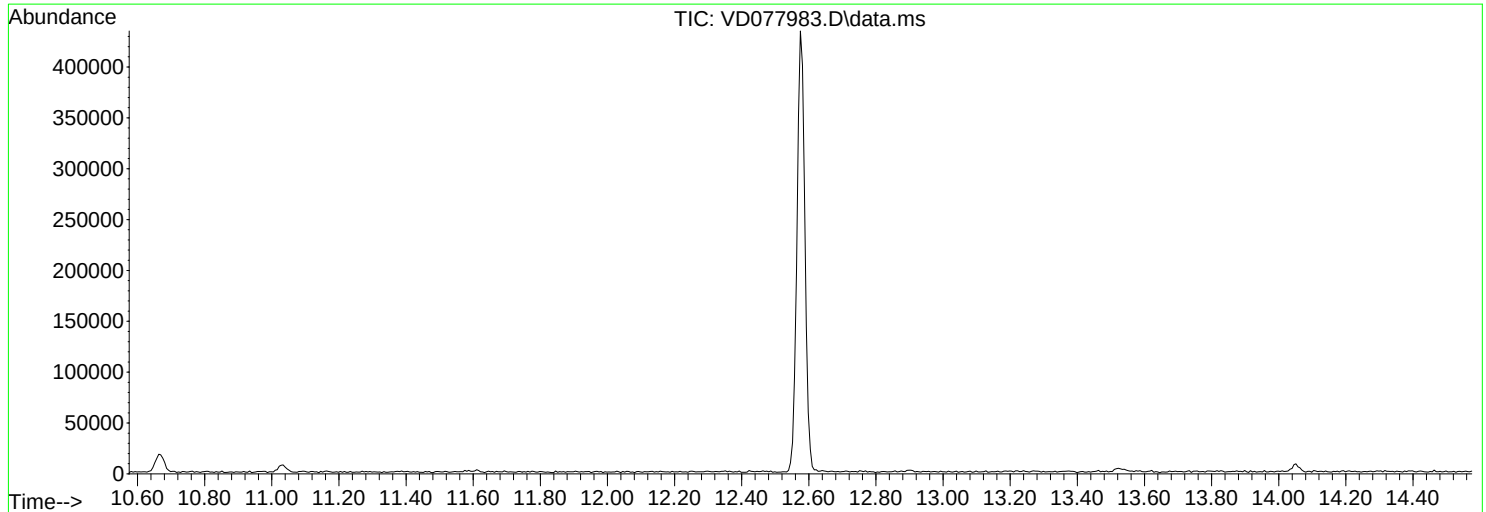

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	14335	PASS
75	95	30	60	53.8	38491	PASS
95	95	100	100	100.0	71600	PASS
96	95	5	9	6.6	4725	PASS
173	174	0.00	2	1.4	913	PASS
174	95	50	100	90.4	64749	PASS
175	174	5	9	8.7	5658	PASS
176	174	95	101	96.5	62453	PASS
177	176	5	9	6.3	3923	PASS