
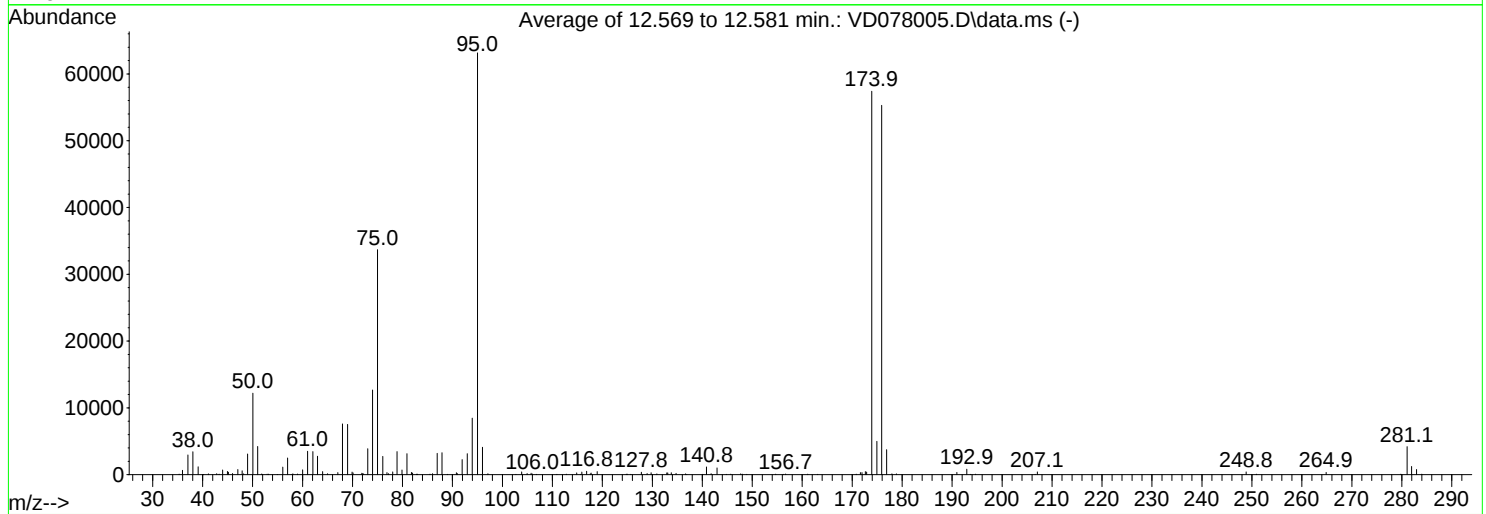


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122023\
Data File : VD078005.D
Acq On : 20 Dec 2023 19:57
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

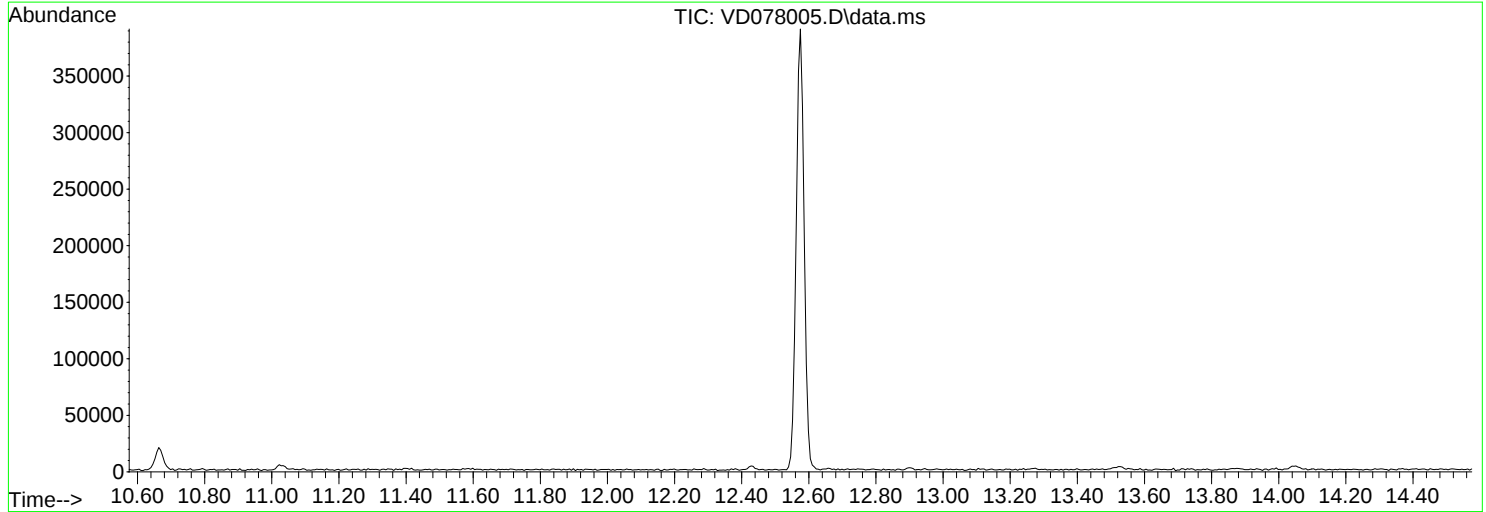

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	12207	PASS
75	95	30	60	53.3	33672	PASS
95	95	100	100	100.0	63157	PASS
96	95	5	9	6.5	4108	PASS
173	174	0.00	2	0.7	385	PASS
174	95	50	100	90.9	57400	PASS
175	174	5	9	8.7	4994	PASS
176	174	95	101	96.3	55296	PASS
177	176	5	9	6.8	3739	PASS