


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122118\
Data File : VD060675.D
Acq On : 21 Dec 2018 10:02
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
Title : SW846 8260
Last Update : Fri Dec 21 17:37:47 2018

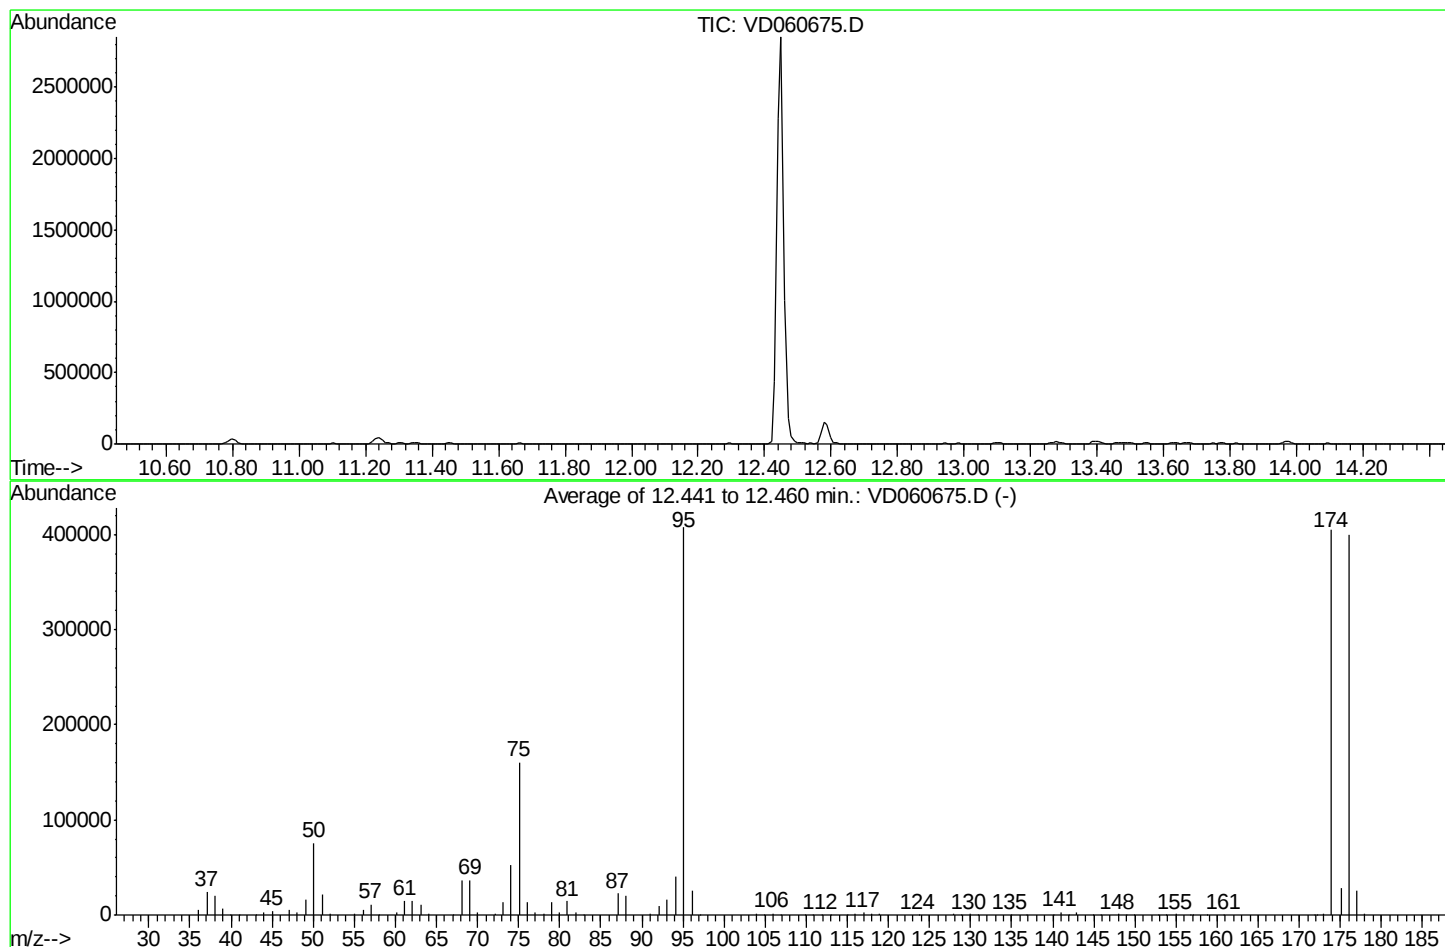

AutoFind: Scans 1140, 1141, 1142; Background Corrected with Scan 1135

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	75805	PASS
75	95	30	60	39.3	160205	PASS
95	95	100	100	100.0	407616	PASS
96	95	5	9	6.3	25540	PASS
173	174	0.00	2	0.2	803	PASS
174	95	50	100	99.5	405461	PASS
175	174	5	9	7.1	28818	PASS
176	174	95	101	98.6	399765	PASS
177	176	5	9	6.3	25194	PASS