

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122121\
 Data File : VD071414.D
 Acq On : 21 Dec 2021 16:53
 Operator : VA/SY
 Sample : M5184-06
 Misc : 7.68G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-6

Quant Time: Dec 21 19:09:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 29 17:54:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	94521	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	174623	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	170641	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	78938	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	90582	81.672	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 163.340%#	
35) Dibromofluoromethane	7.914	113	66356	59.674	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 119.340%	
50) Toluene-d8	10.338	98	218498	51.634	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 103.260%	
62) 4-Bromofluorobenzene	12.626	95	77338	52.724	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 105.440%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122121\
Data File : VD071414.D
Acq On : 21 Dec 2021 16:53
Operator : VA/SY
Sample : M5184-06
Misc : 7.68G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-6

Quant Time: Dec 21 19:09:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Quant Title : SW846 8260
QLast Update : Mon Nov 29 17:54:09 2021
Response via : Initial Calibration




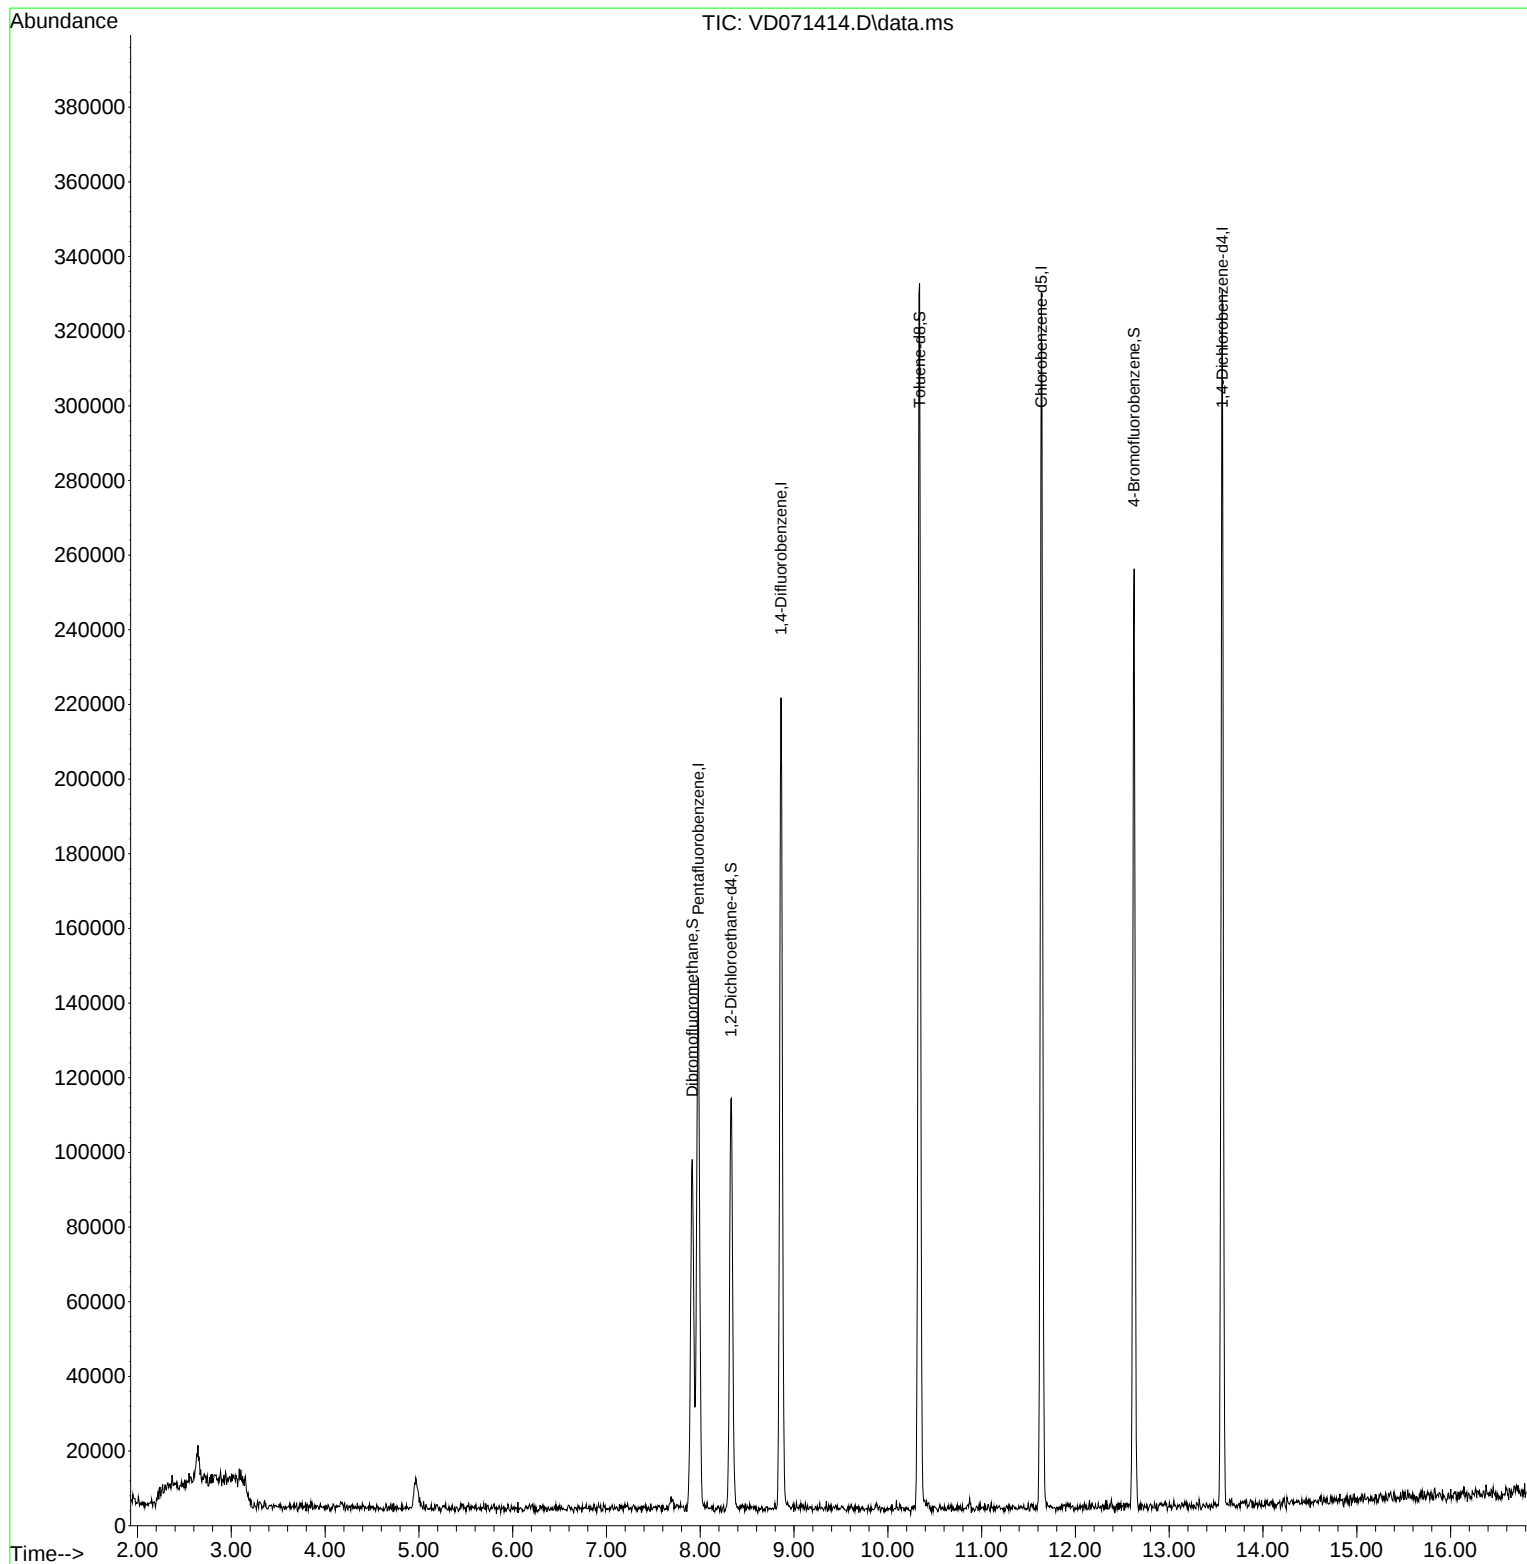


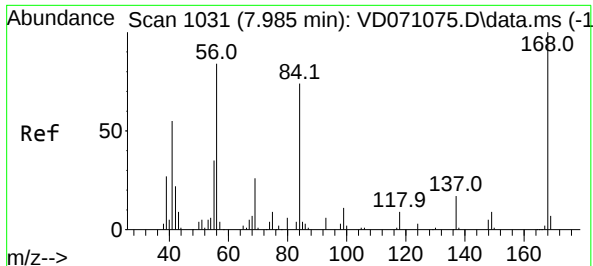

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1031
Delta R.T. -0.006 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53




Instrument :
MSVOA_D
ClientSampleId :
SB-6


Tgt Ion:168 Resp: 94521
Ion Ratio Lower Upper
168 100
99 66.0 46.6 69.8

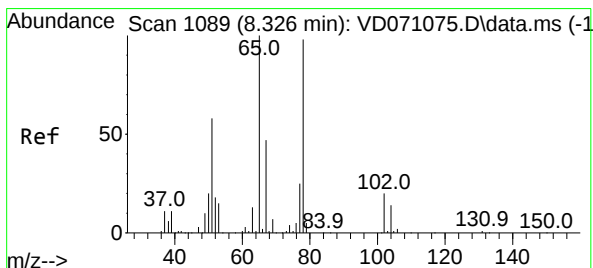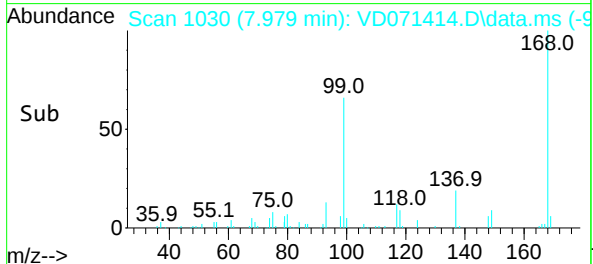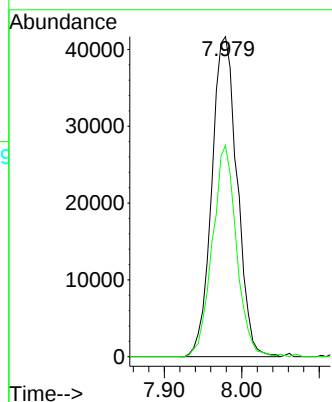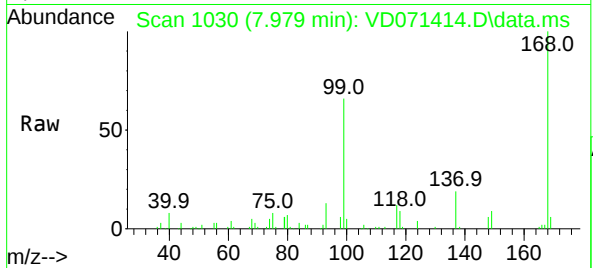

#33
1,2-Dichloroethane-d4
Concen: 81.672 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. -0.000 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53

Tgt Ion: 65 Resp: 90582
Ion Ratio Lower Upper
65 100
67 50.2 0.0 112.2

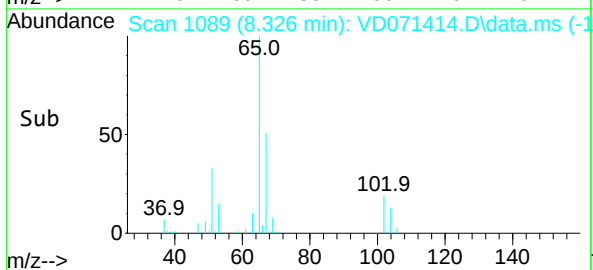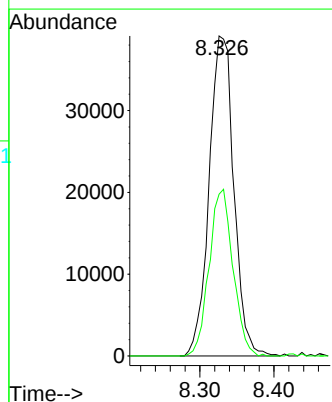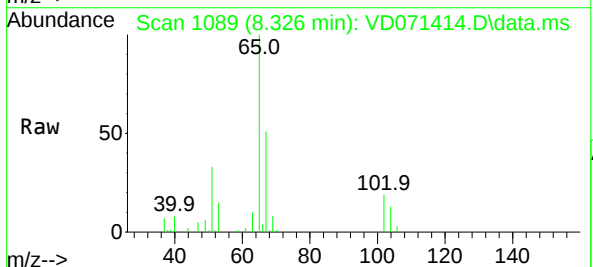

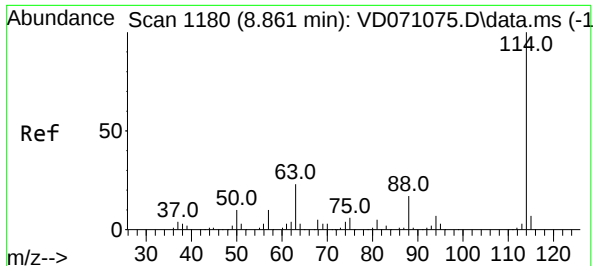

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071414.D

Acq: 21 Dec 2021 16:53

Instrument :

MSVOA_D

ClientSampleId :

SB-6





Tgt Ion:114 Resp: 174623

Ion Ratio Lower Upper

114 100

63 22.8 0.0 41.8

88 17.1 0.0 32.8

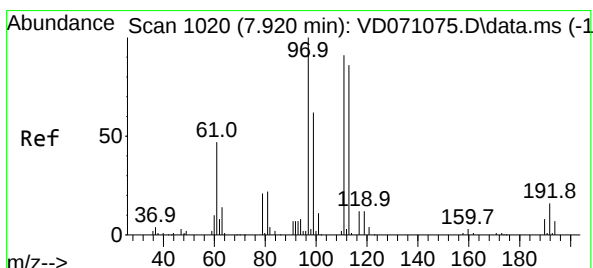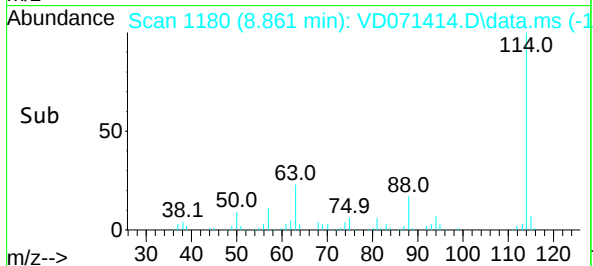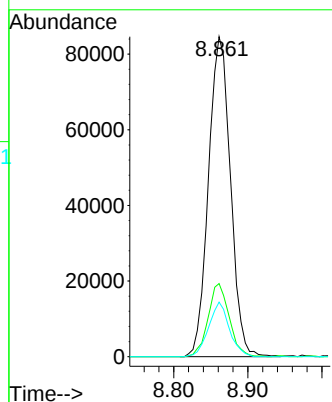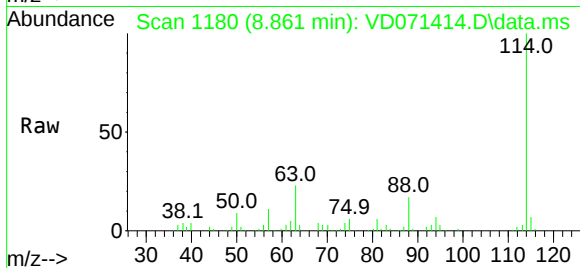

#35

Dibromofluoromethane

Concen: 59.674 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. -0.006 min

Lab File: VD071414.D

Acq: 21 Dec 2021 16:53




Tgt Ion:113 Resp: 66356


Ion Ratio Lower Upper

113 100

111 102.5 82.0 123.0

192 17.3 15.2 22.8


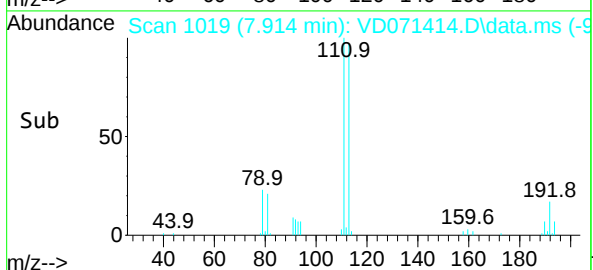
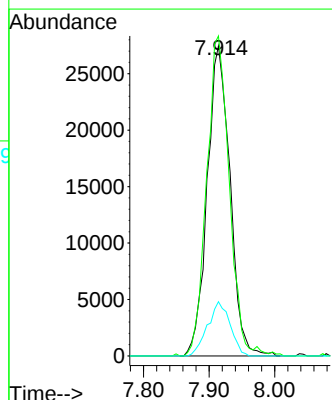
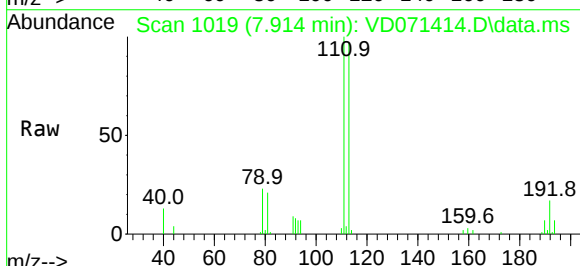


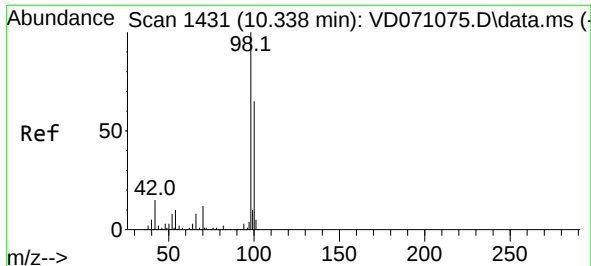

#50
Toluene-d8
Concen: 51.634 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53




Instrument :
MSVOA_D
ClientSampleId :
SB-6


Tgt Ion: 98 Resp: 218498
Ion Ratio Lower Upper
98 100
100 64.1 51.8 77.6

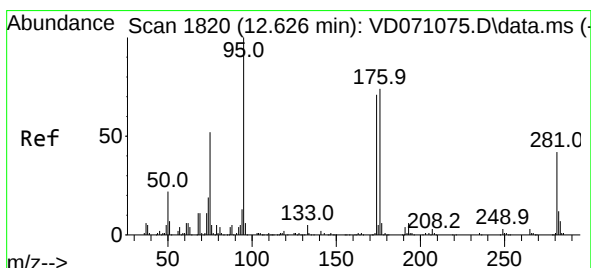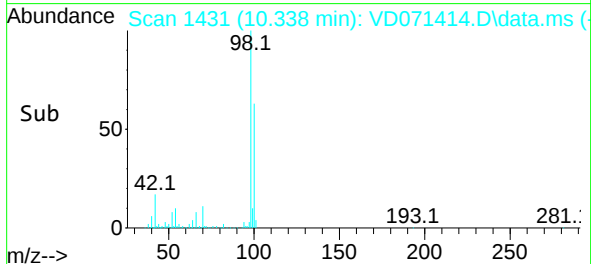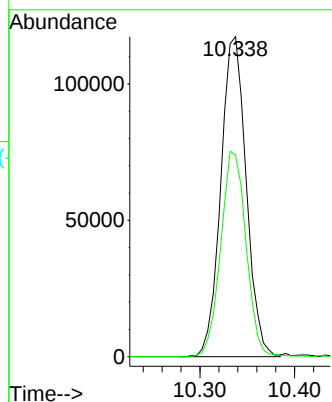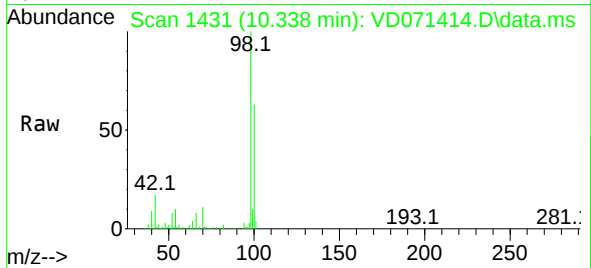

#62
4-Bromofluorobenzene
Concen: 52.724 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53

Tgt Ion: 95 Resp: 77338
Ion Ratio Lower Upper
95 100
174 75.4 0.0 159.4
176 73.6 0.0 154.0


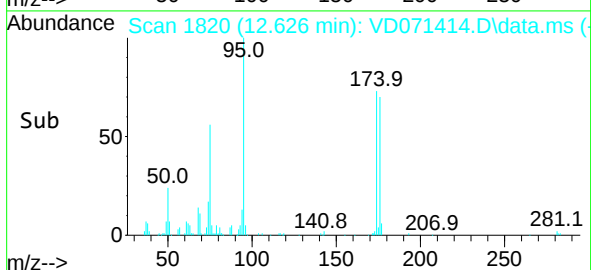
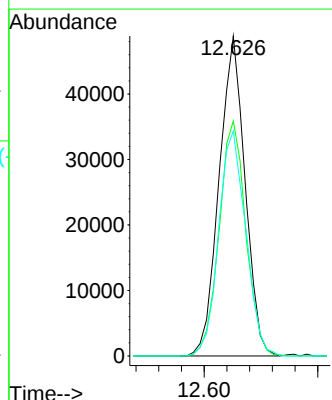
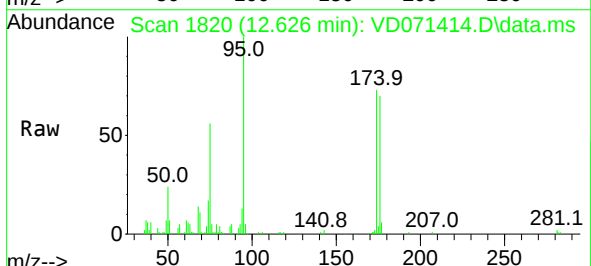


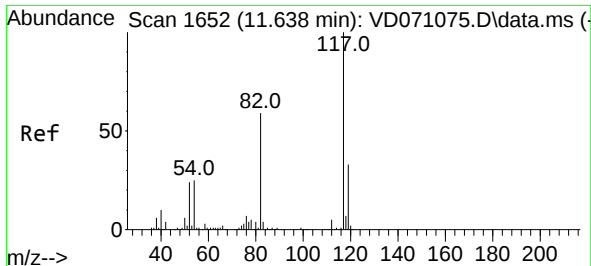

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53

Instrument :
MSVOA_D
ClientSampleId :
SB-6

Tgt Ion:117 Resp: 170641
Ion Ratio Lower Upper
117 100
82 56.2 44.7 67.1
119 28.3 26.2 39.4

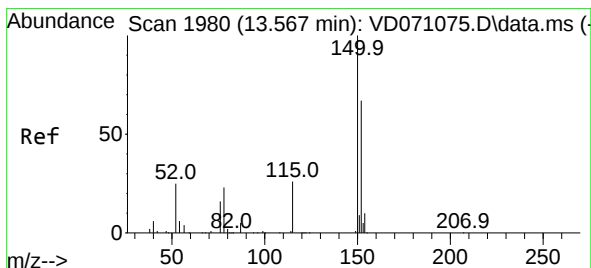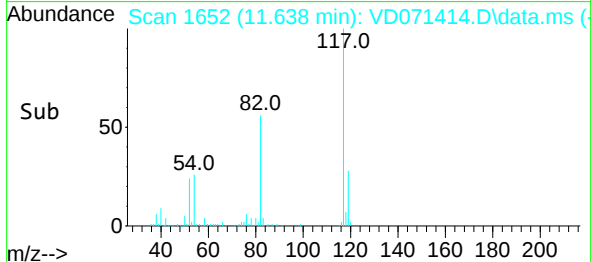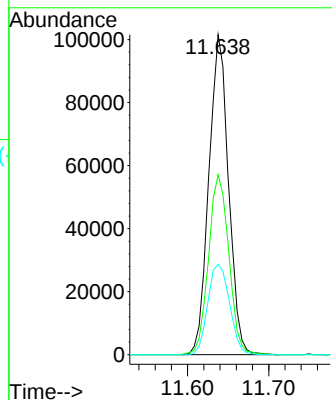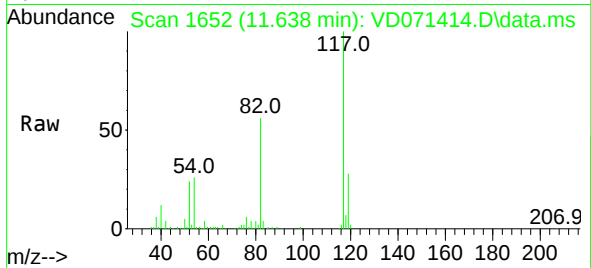

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD071414.D
Acq: 21 Dec 2021 16:53

Tgt Ion:152 Resp: 78938
Ion Ratio Lower Upper
152 100
115 58.6 29.8 89.3
150 159.3 0.0 349.2

