
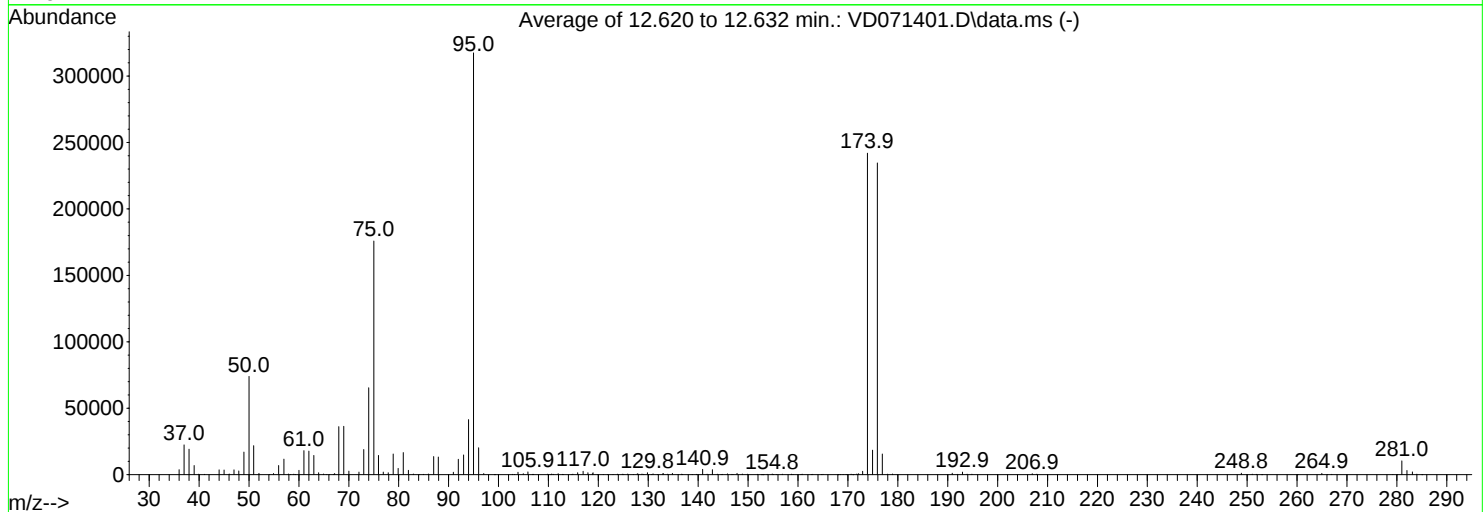


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122121\
Data File : VD071401.D
Acq On : 21 Dec 2021 08:24
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D112921S.M
Title : SW846 8260
Last Update : Mon Nov 29 17:54:09 2021

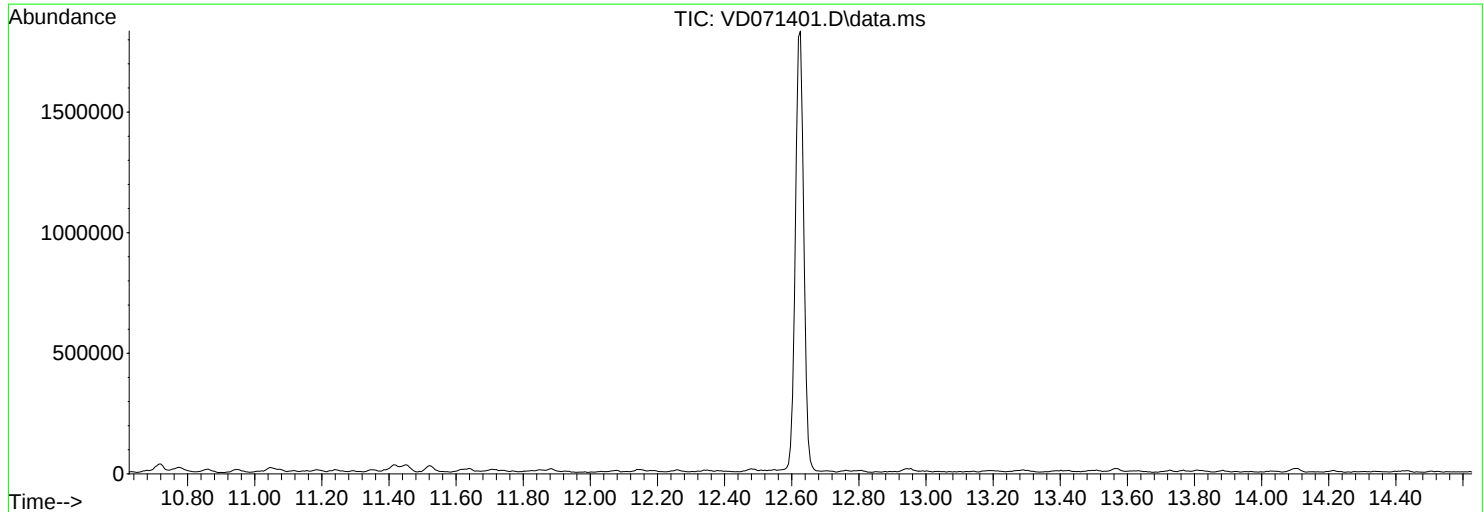

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1806

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	73909	PASS
75	95	30	60	55.4	175851	PASS
95	95	100	100	100.0	317504	PASS
96	95	5	9	6.4	20192	PASS
173	174	0.00	2	1.0	2515	PASS
174	95	50	100	76.2	241920	PASS
175	174	5	9	7.6	18427	PASS
176	174	95	101	97.0	234603	PASS
177	176	5	9	6.6	15539	PASS