

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
 Data File : VD078022.D
 Acq On : 21 Dec 2023 13:17
 Operator : RP/MD
 Sample : VD1221SBL01
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1221SBL01

Quant Time: Dec 22 05:11:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	188491	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.781	114	335909	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	316975	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	142888	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	83426	37.561	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	75.120%
35) Dibromofluoromethane	7.810	113	102167	43.421	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	86.840%
50) Toluene-d8	10.269	98	421201	44.695	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	89.400%
62) 4-Bromofluorobenzene	12.575	95	119969	42.580	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	85.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
Data File : VD078022.D
Acq On : 21 Dec 2023 13:17
Operator : RP/MD
Sample : VD1221SBL01
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1221SBL01

Quant Time: Dec 22 05:11:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




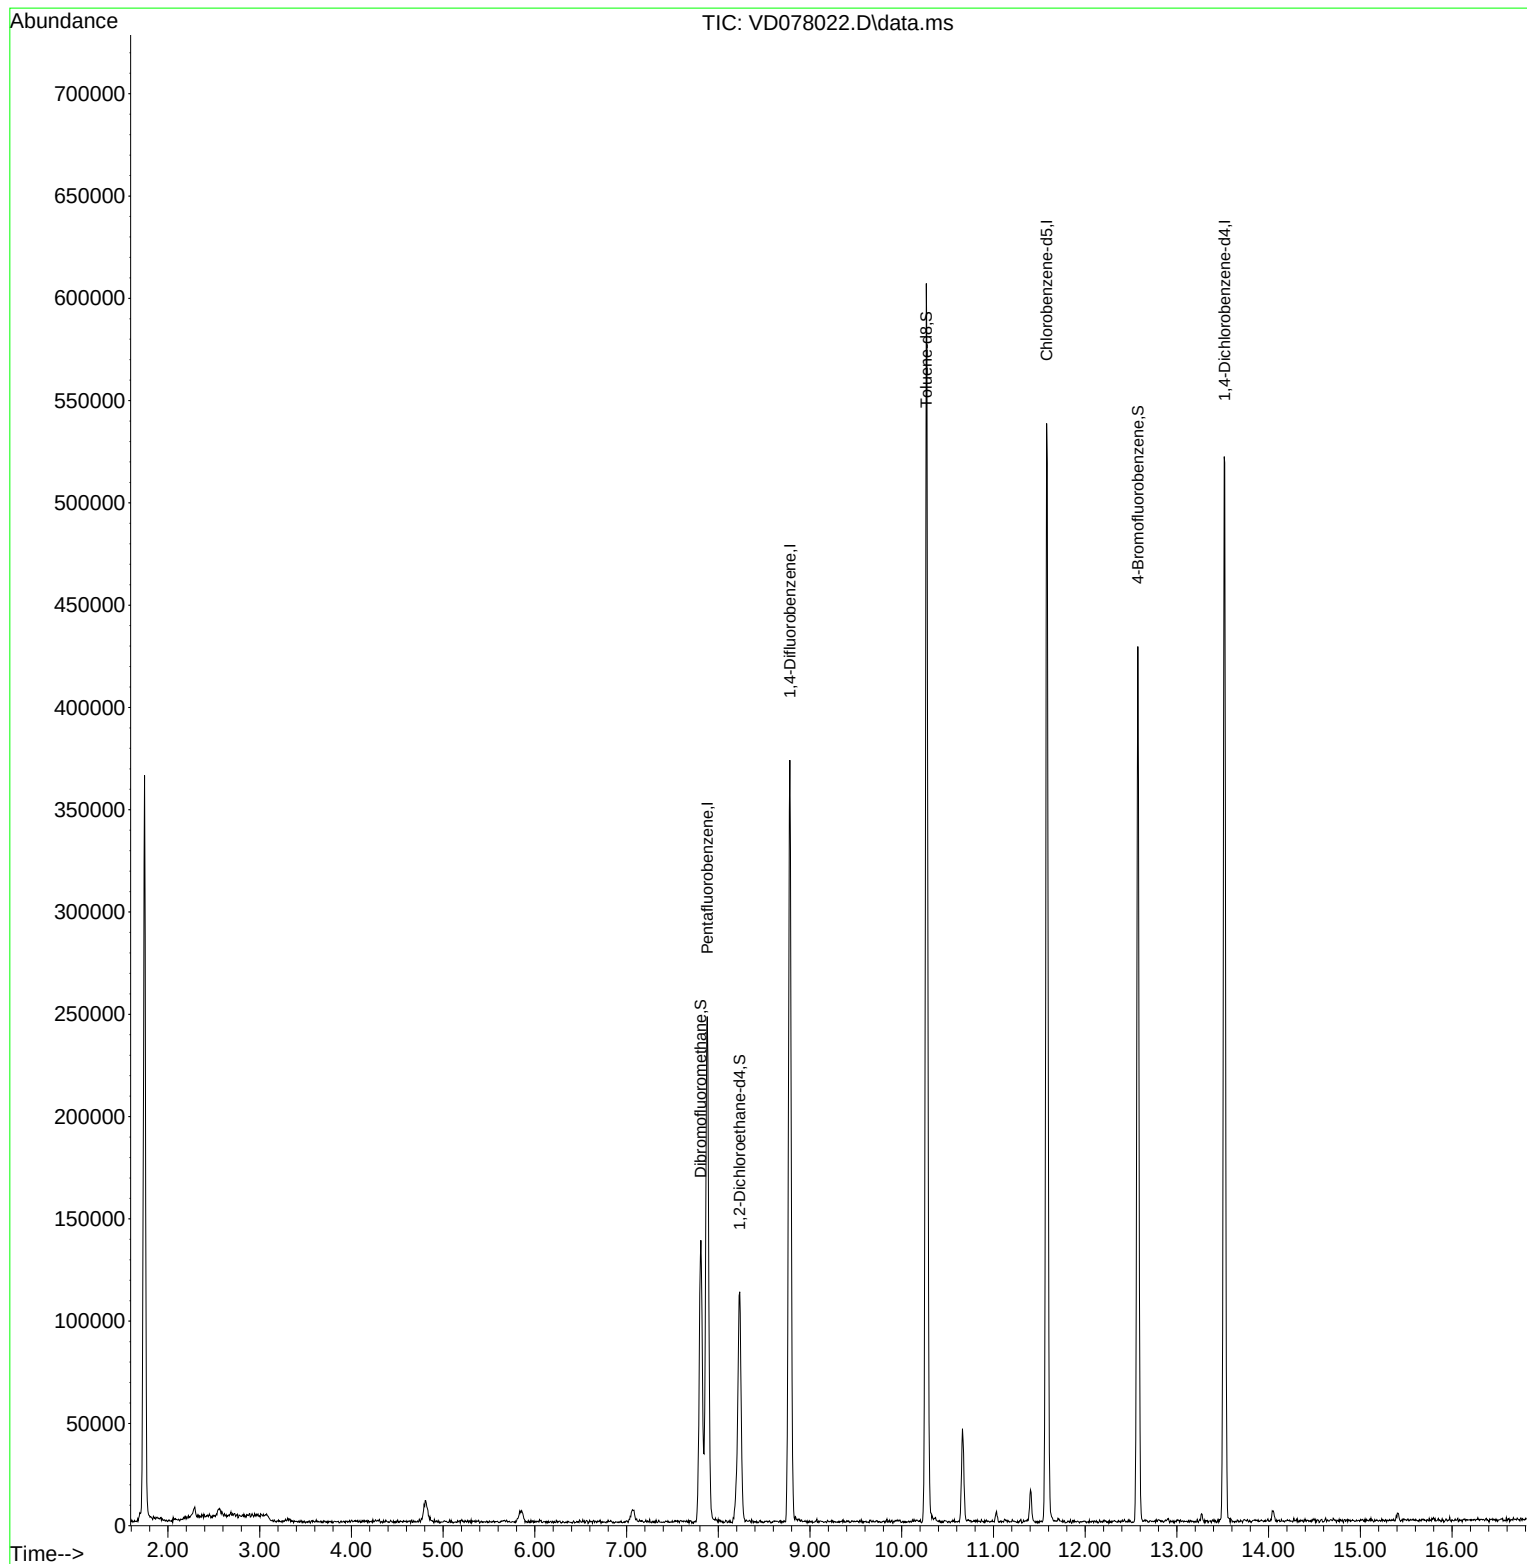


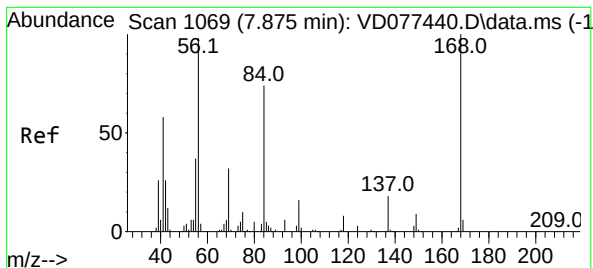

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 110
Delta R.T. 0.006 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17




Instrument :
MSVOA_D
ClientSampleId :
VD1221SBL01


Tgt Ion:168 Resp: 188491
Ion Ratio Lower Upper
168 100
99 55.2 36.7 55.1#

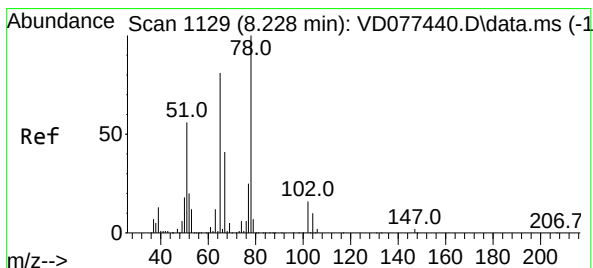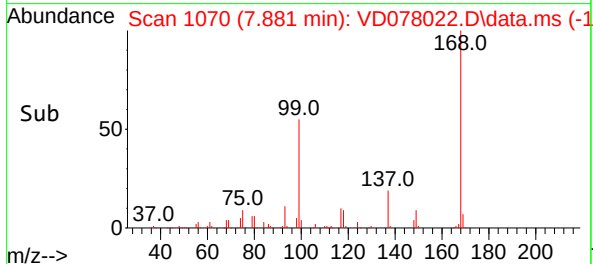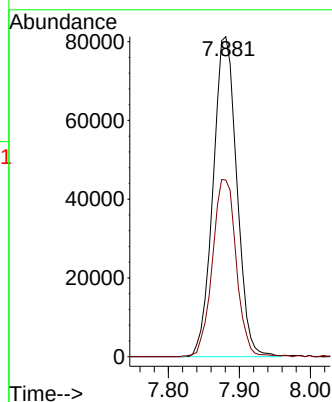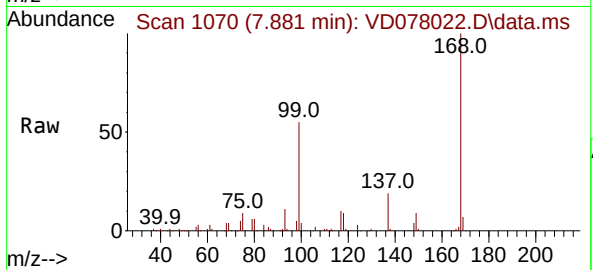

#33
1,2-Dichloroethane-d4
Concen: 37.561 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17

Tgt Ion: 65 Resp: 83426
Ion Ratio Lower Upper
65 100
67 55.7 0.0 115.0

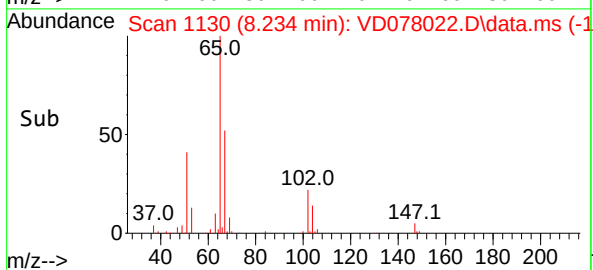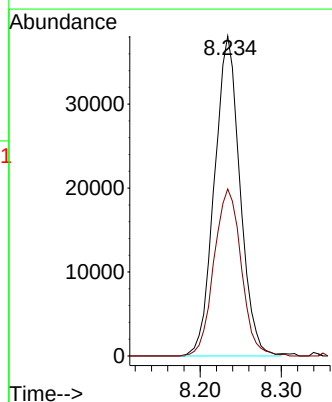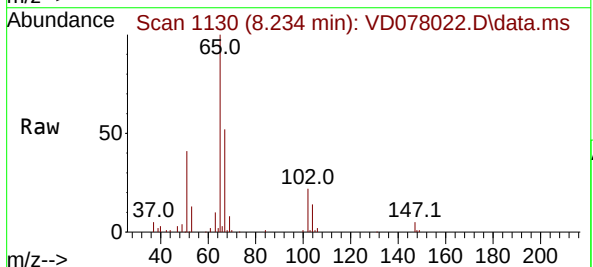

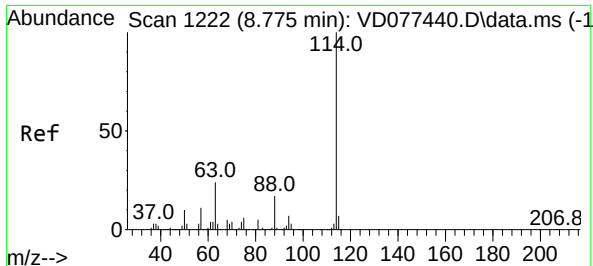

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD078022.D

Acq: 21 Dec 2023 13:17

Instrument :

MSVOA_D

ClientSampleId :

VD1221SBL01





Tgt Ion:114 Resp: 335909

Ion Ratio Lower Upper

114 100

63 17.4 0.0 33.4

88 15.0 0.0 26.2

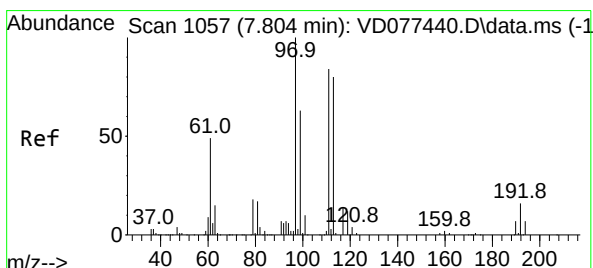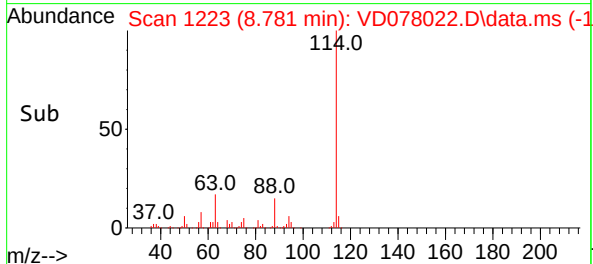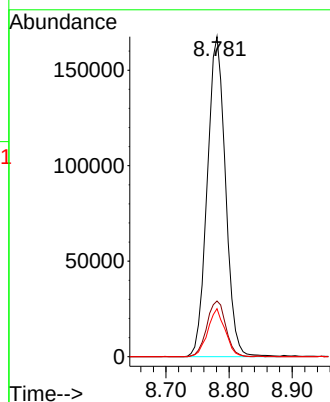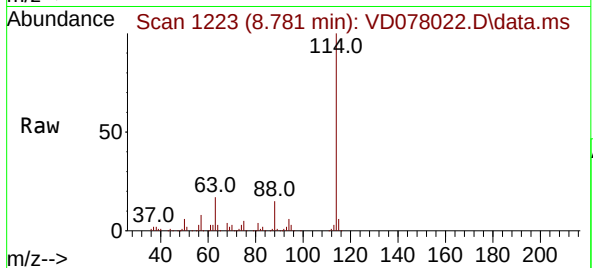

#35

Dibromofluoromethane

Concen: 43.421 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078022.D

Acq: 21 Dec 2023 13:17




Tgt Ion:113 Resp: 102167


Ion Ratio Lower Upper

113 100

111 101.6 84.7 127.1

192 17.8 16.8 25.2


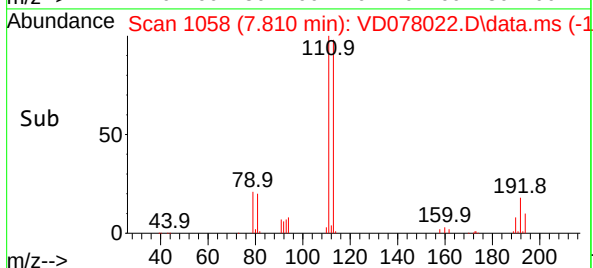
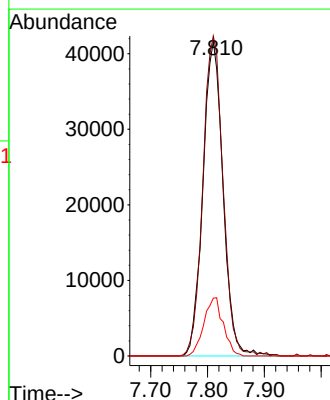
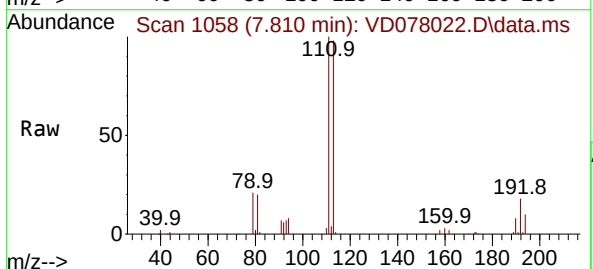


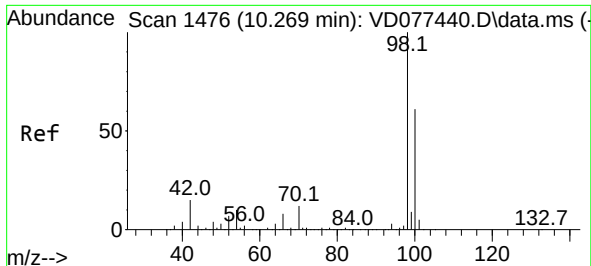

#50
Toluene-d8
Concen: 44.695 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17




Instrument :
MSVOA_D
ClientSampleId :
VD1221SBL01


Tgt Ion: 98 Resp: 421201
Ion Ratio Lower Upper
98 100
100 63.8 50.3 75.5

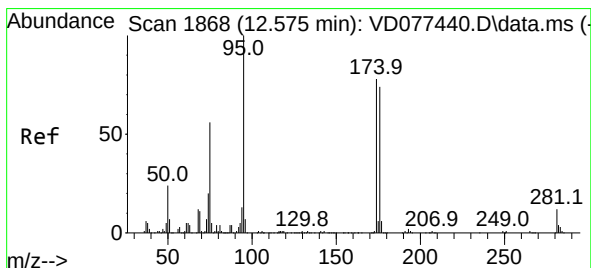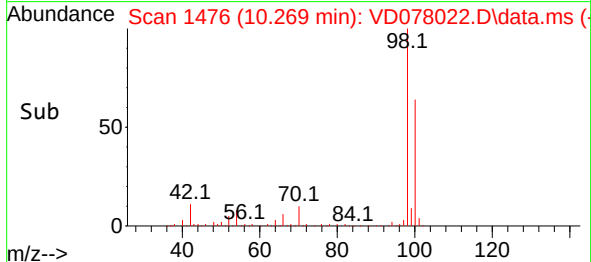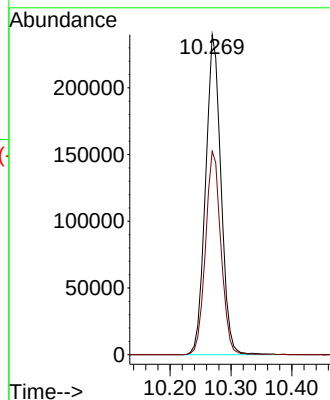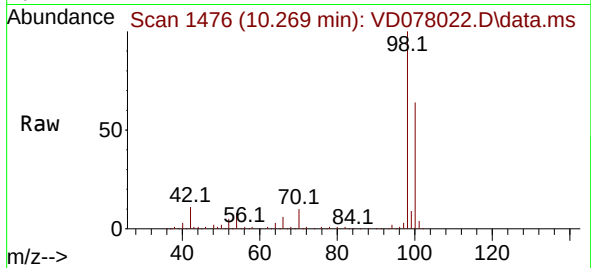

#62
4-Bromofluorobenzene
Concen: 42.580 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17

Tgt Ion: 95 Resp: 119969
Ion Ratio Lower Upper
95 100
174 90.9 0.0 201.8
176 86.7 0.0 191.8


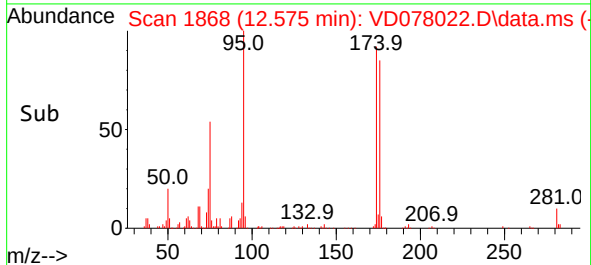
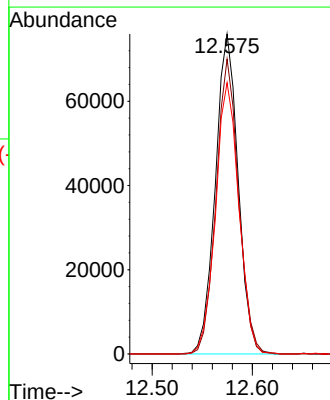
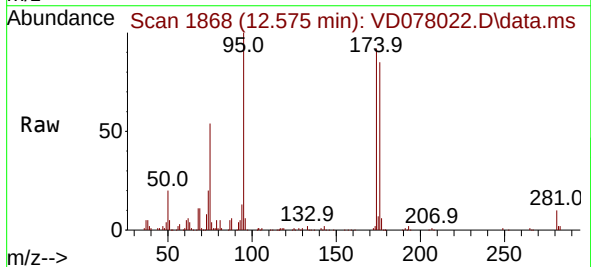


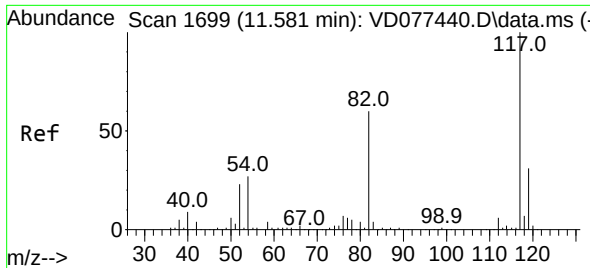

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17

Instrument :
MSVOA_D
ClientSampleId :
VD1221SBL01

Tgt Ion:117 Resp: 316975
Ion Ratio Lower Upper
117 100
82 53.3 38.3 57.5
119 32.6 25.0 37.4

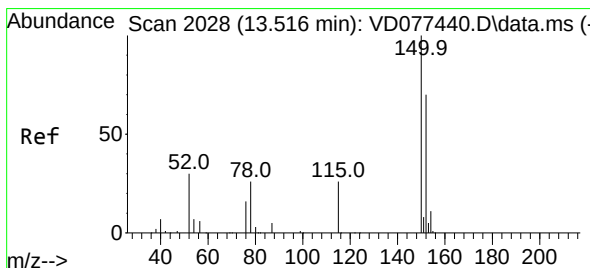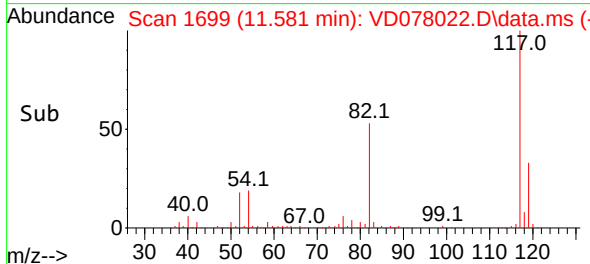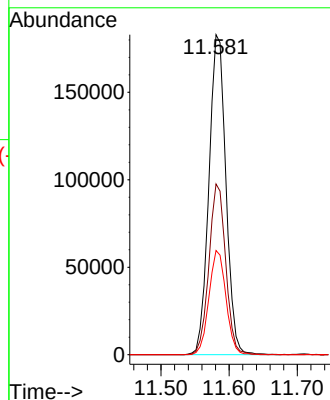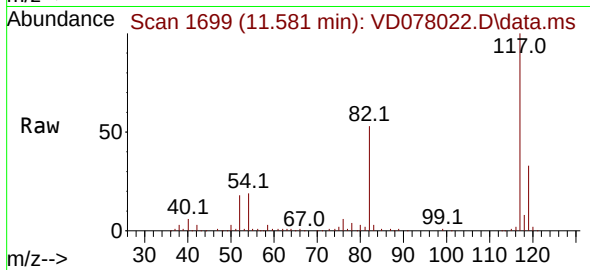

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD078022.D
Acq: 21 Dec 2023 13:17

Tgt Ion:152 Resp: 142888
Ion Ratio Lower Upper
152 100
115 56.1 27.1 81.3
150 156.7 0.0 353.6

