

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
 Data File : VD078049.D
 Acq On : 22 Dec 2023 03:52
 Operator : RP/MD
 Sample : 05877-15
 Misc : 5.28G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 COM51

Quant Time: Dec 22 05:55:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	164438	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.781	114	298547	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	283741	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	121907	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	81873	42.253	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	84.500%
35) Dibromofluoromethane	7.810	113	91902	43.947	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	87.900%
50) Toluene-d8	10.269	98	379918	45.360	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	90.720%
62) 4-Bromofluorobenzene	12.575	95	111829	44.658	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	89.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
Data File : VD078049.D
Acq On : 22 Dec 2023 03:52
Operator : RP/MD
Sample : 05877-15
Misc : 5.28G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
COM51

Quant Time: Dec 22 05:55:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




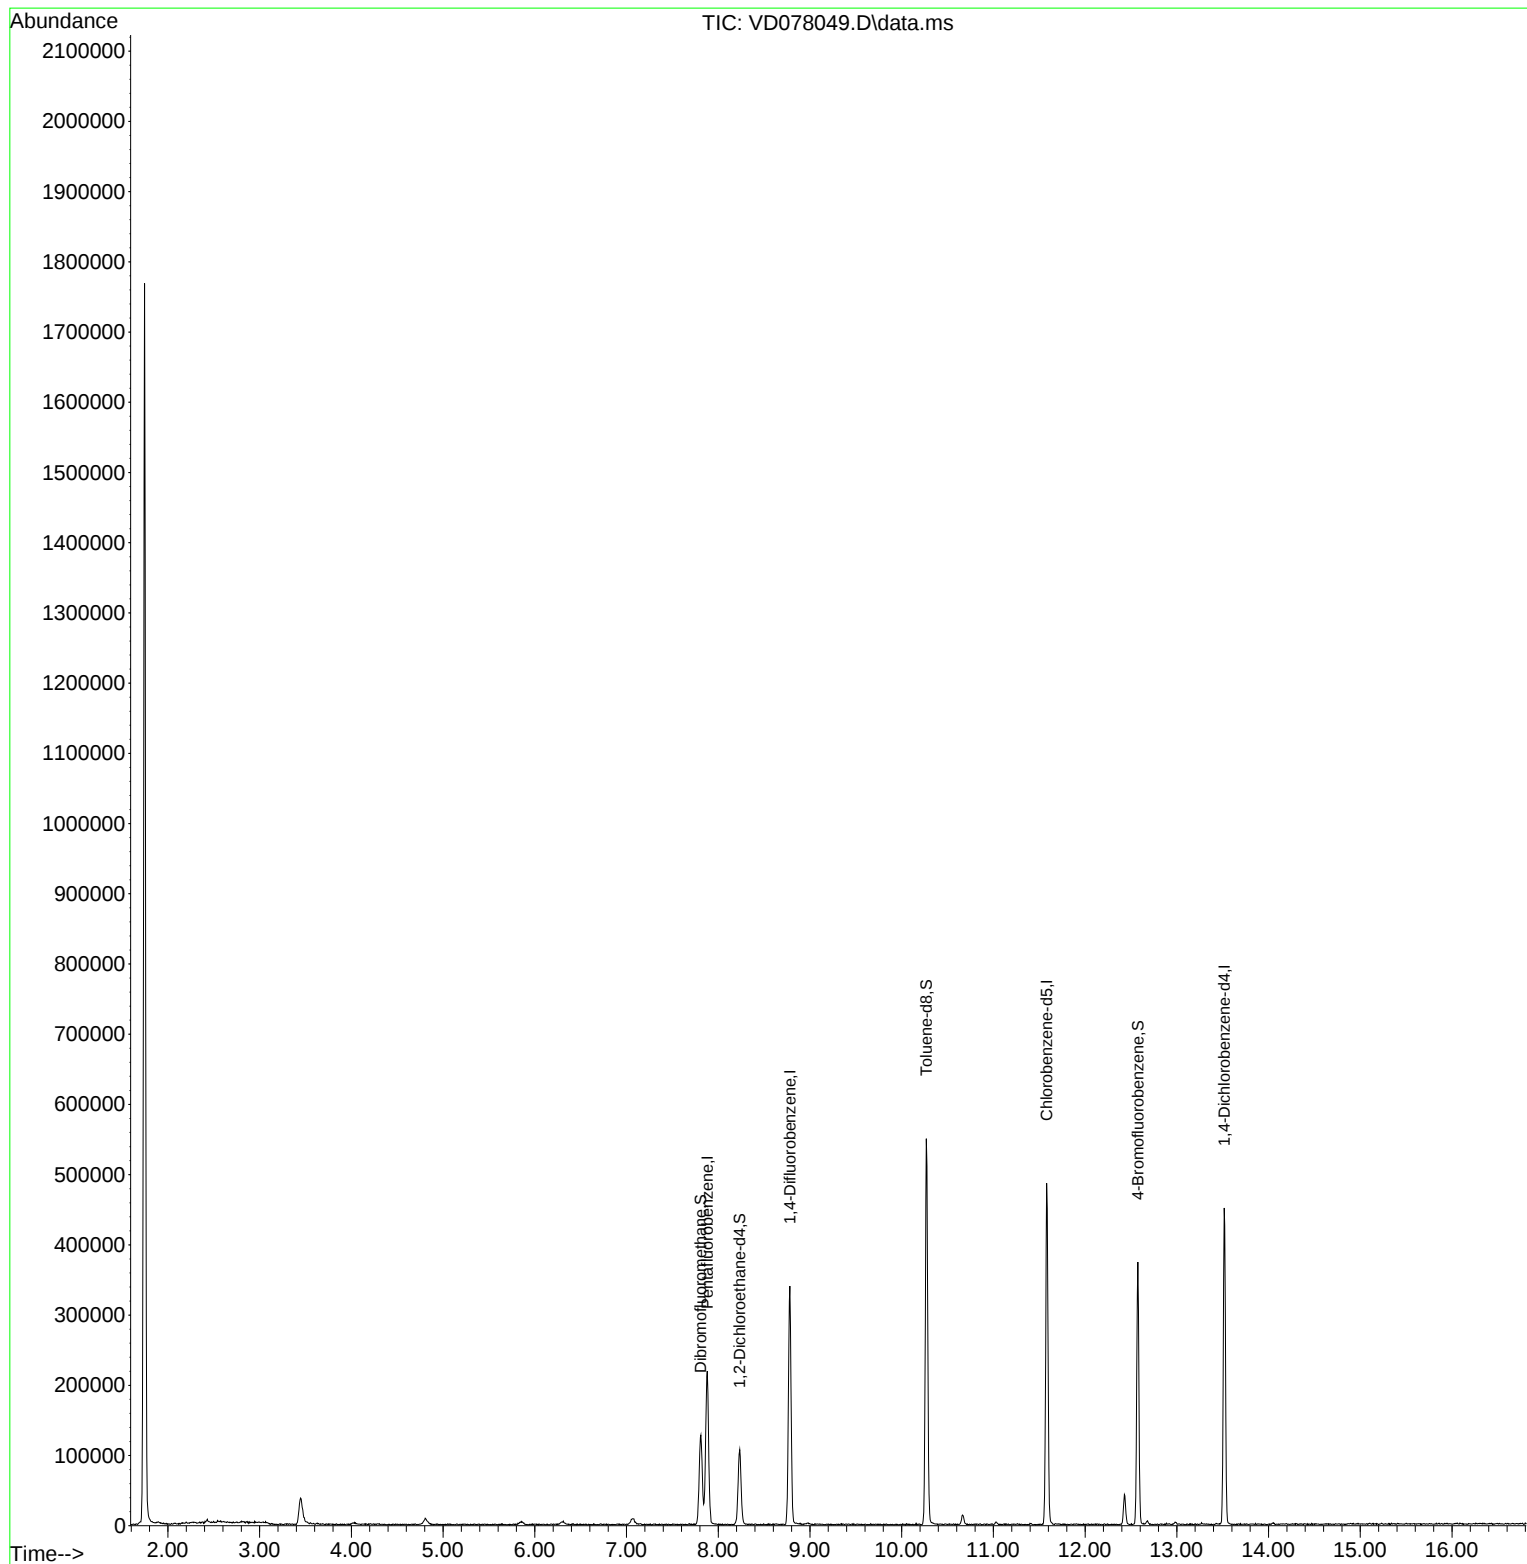


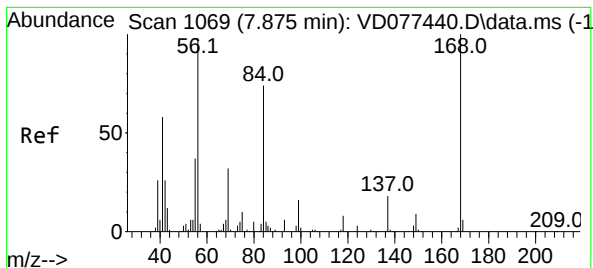

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52




Instrument :
MSVOA_D
ClientSampleId :
COM51


Tgt Ion:168 Resp: 164438
Ion Ratio Lower Upper
168 100
99 57.4 36.7 55.1#

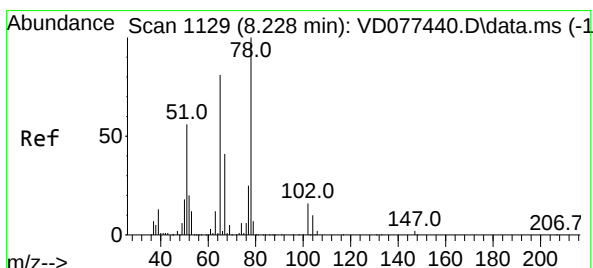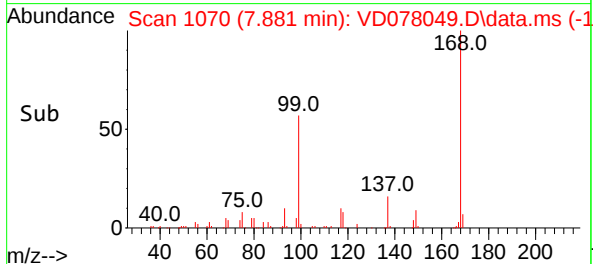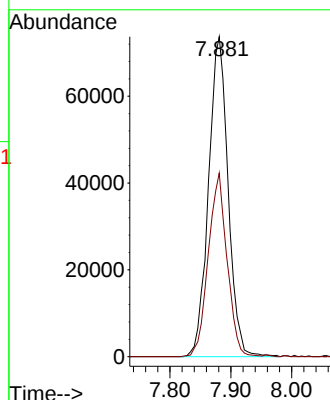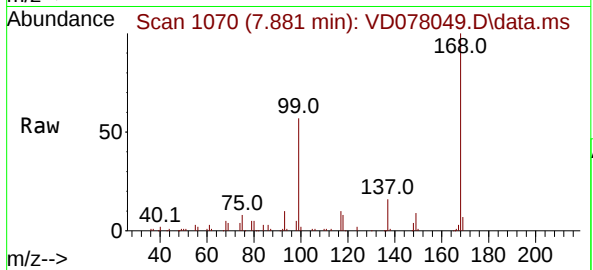

#33
1,2-Dichloroethane-d4
Concen: 42.253 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52

Tgt Ion: 65 Resp: 81873
Ion Ratio Lower Upper
65 100
67 54.6 0.0 115.0

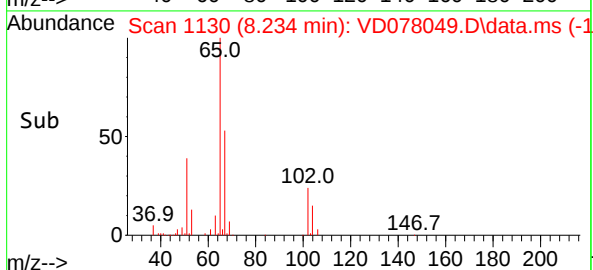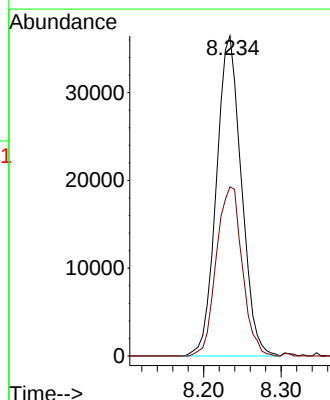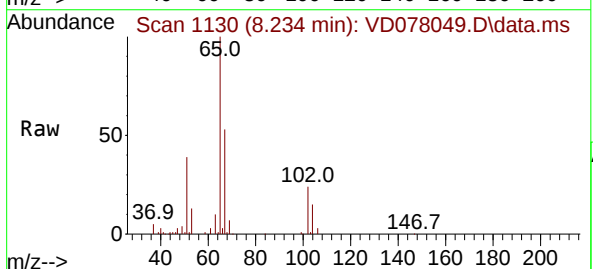

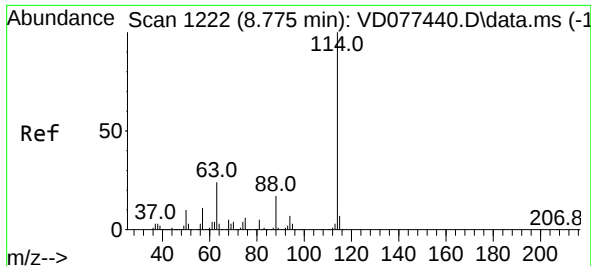

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD078049.D

Acq: 22 Dec 2023 03:52

Instrument :

MSVOA_D

ClientSampleId :

COM51





Tgt Ion:114 Resp: 298547

Ion Ratio Lower Upper

114 100

63 17.5 0.0 33.4

88 11.8 0.0 26.2

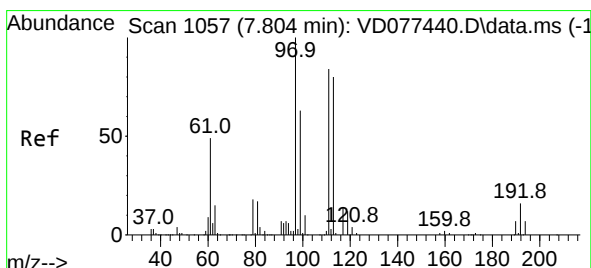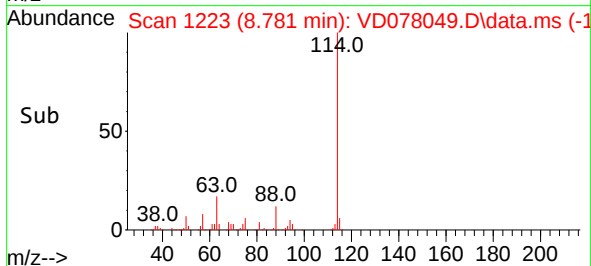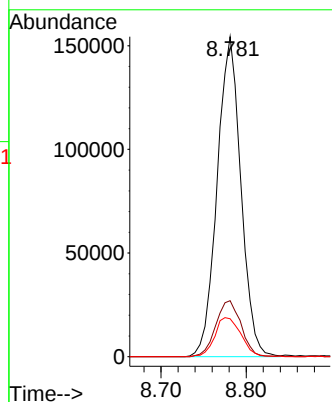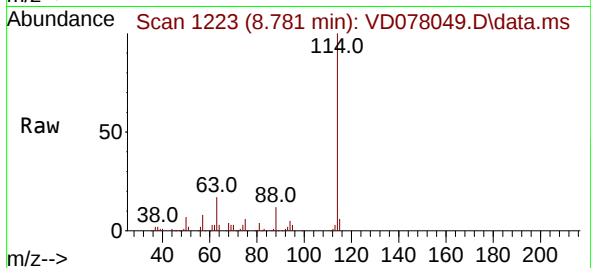

#35

Dibromofluoromethane

Concen: 43.947 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078049.D

Acq: 22 Dec 2023 03:52




Tgt Ion:113 Resp: 91902

Ion Ratio Lower Upper

113 100

111 105.9 84.7 127.1

192 17.6 16.8 25.2


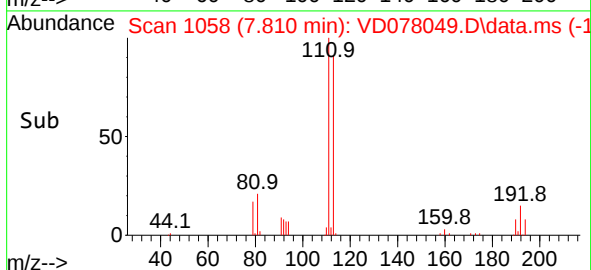
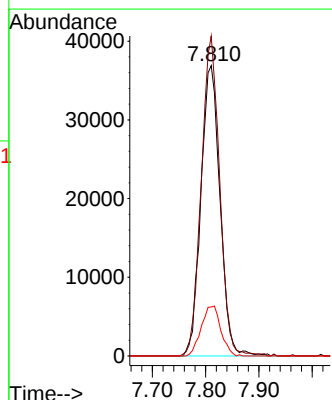
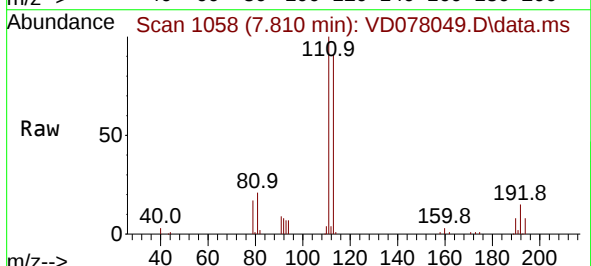




#50
Toluene-d8
Concen: 45.360 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52




Instrument :
MSVOA_D
ClientSampleId :
COM51


Tgt Ion: 98 Resp: 379918
Ion Ratio Lower Upper
98 100
100 64.9 50.3 75.5

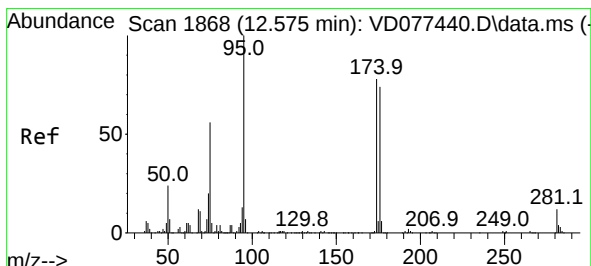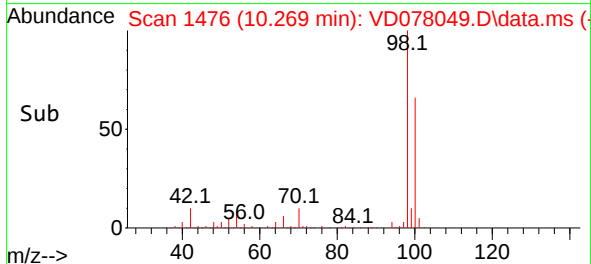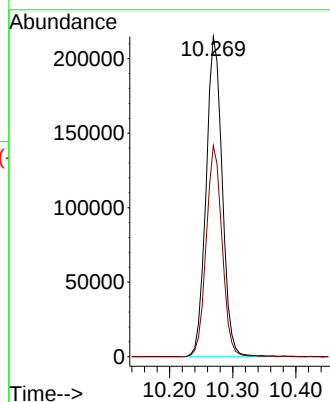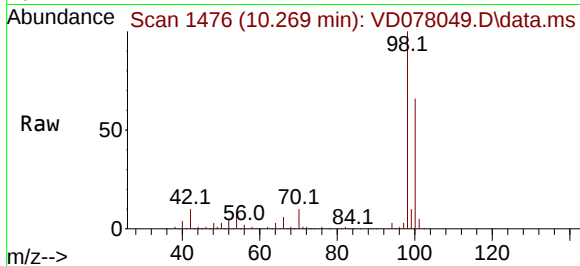

#62
4-Bromofluorobenzene
Concen: 44.658 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52

Tgt Ion: 95 Resp: 111829
Ion Ratio Lower Upper
95 100
174 88.1 0.0 201.8
176 83.9 0.0 191.8


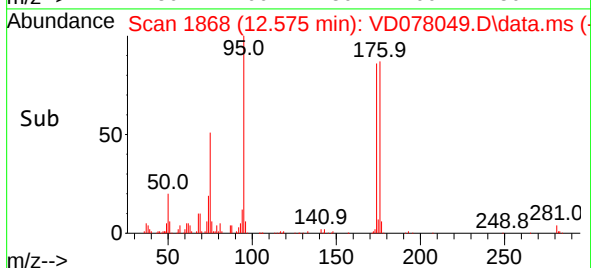
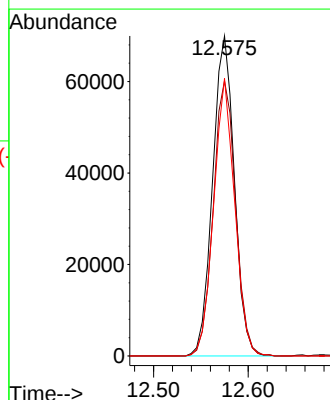
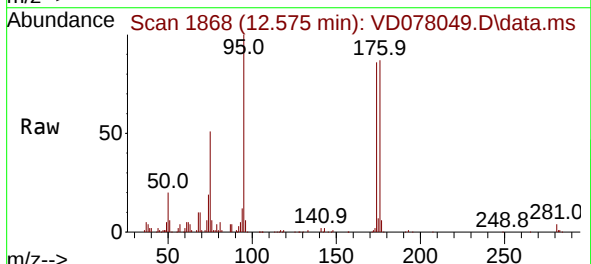


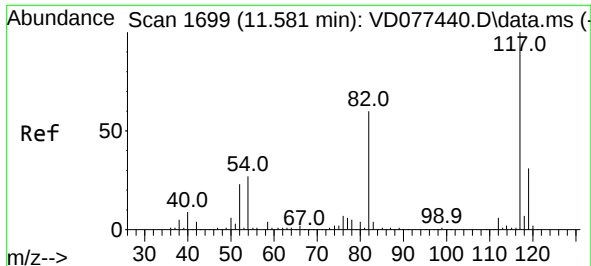

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52

Instrument :
MSVOA_D
ClientSampleId :
COM51

Tgt Ion:117 Resp: 283741
Ion Ratio Lower Upper
117 100
82 56.2 38.3 57.5
119 33.2 25.0 37.4

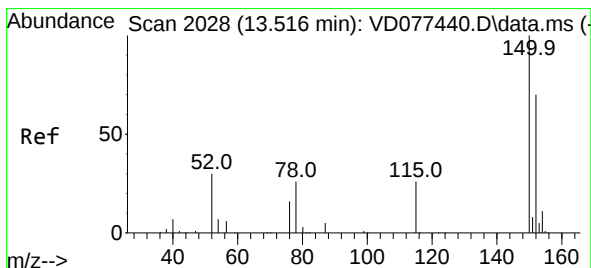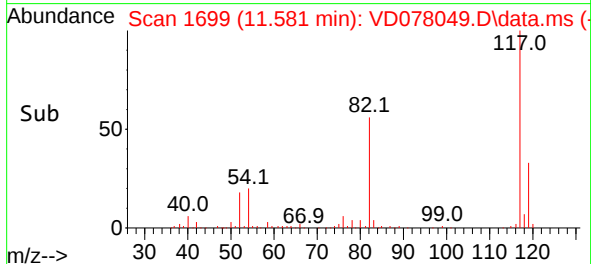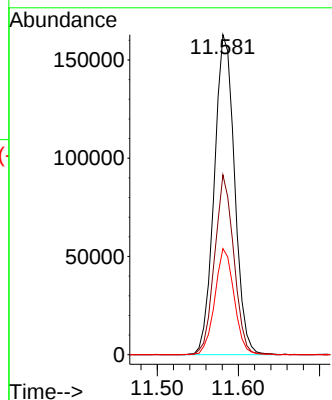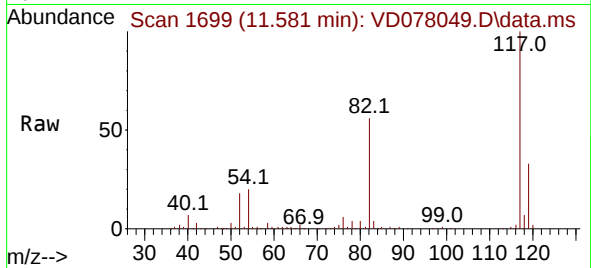

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD078049.D
Acq: 22 Dec 2023 03:52

Tgt Ion:152 Resp: 121907
Ion Ratio Lower Upper
152 100
115 57.4 27.1 81.3
150 157.9 0.0 353.6

